

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070323\
 Data File : VV031637.D
 Acq On : 03 Jul 2023 15:15
 Operator : SY/MD
 Sample : VIBLK220
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK220

Quant Time: Jul 04 07:08:55 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Jul 04 07:06:08 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.539	114	232185	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.792	117	229891	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.194	152	121728	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	57080	36.939	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	73.880%		
7) Chloroethane-d5	1.516	69	27741	20.575	ug/L	-0.02
Spiked Amount 50.000	Range 70 - 130		Recovery =	41.140%#		
11) 1,1-Dichloroethene-d2	2.043	65	30012	37.684	ug/L	-0.02
Spiked Amount 50.000	Range 60 - 125		Recovery =	75.360%		
21) 2-Butanone-d5	3.809	46	115346	92.185	ug/L	0.02
Spiked Amount 100.000	Range 40 - 130		Recovery =	92.180%		
24) Chloroform-d	4.252	84	144794	37.415	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	74.820%		
26) 1,2-Dichloroethane-d4	4.947	65	97524	40.277	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	80.560%		
32) Benzene-d6	4.960	84	236155	36.495	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	72.980%		
36) 1,2-Dichloropropane-d6	5.995	67	91851	40.048	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	80.100%		
41) Toluene-d8	7.249	98	188373	31.723	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	63.440%#		
43) trans-1,3-Dichloroprop...	7.561	79	40518	36.239	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	72.480%		
47) 2-Hexanone-d5	8.053	63	78882	87.110	ug/L	0.02
Spiked Amount 100.000	Range 45 - 130		Recovery =	87.110%		
56) 1,1,2,2-Tetrachloroeth...	10.165	84	143102	41.337	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	82.680%		
66) 1,2-Dichlorobenzene-d4	11.570	152	90070	38.817	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	77.640%#		
Target Compounds						Qvalue
15) Methyl Acetate	2.388	43	19196	9.234	ug/L	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070323\
Data File : VV031637.D
Acq On : 03 Jul 2023 15:15
Operator : SY/MD
Sample : VIBLK220
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK220

Quant Time: Jul 04 07:08:55 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Jul 04 07:06:08 2023
Response via : Initial Calibration

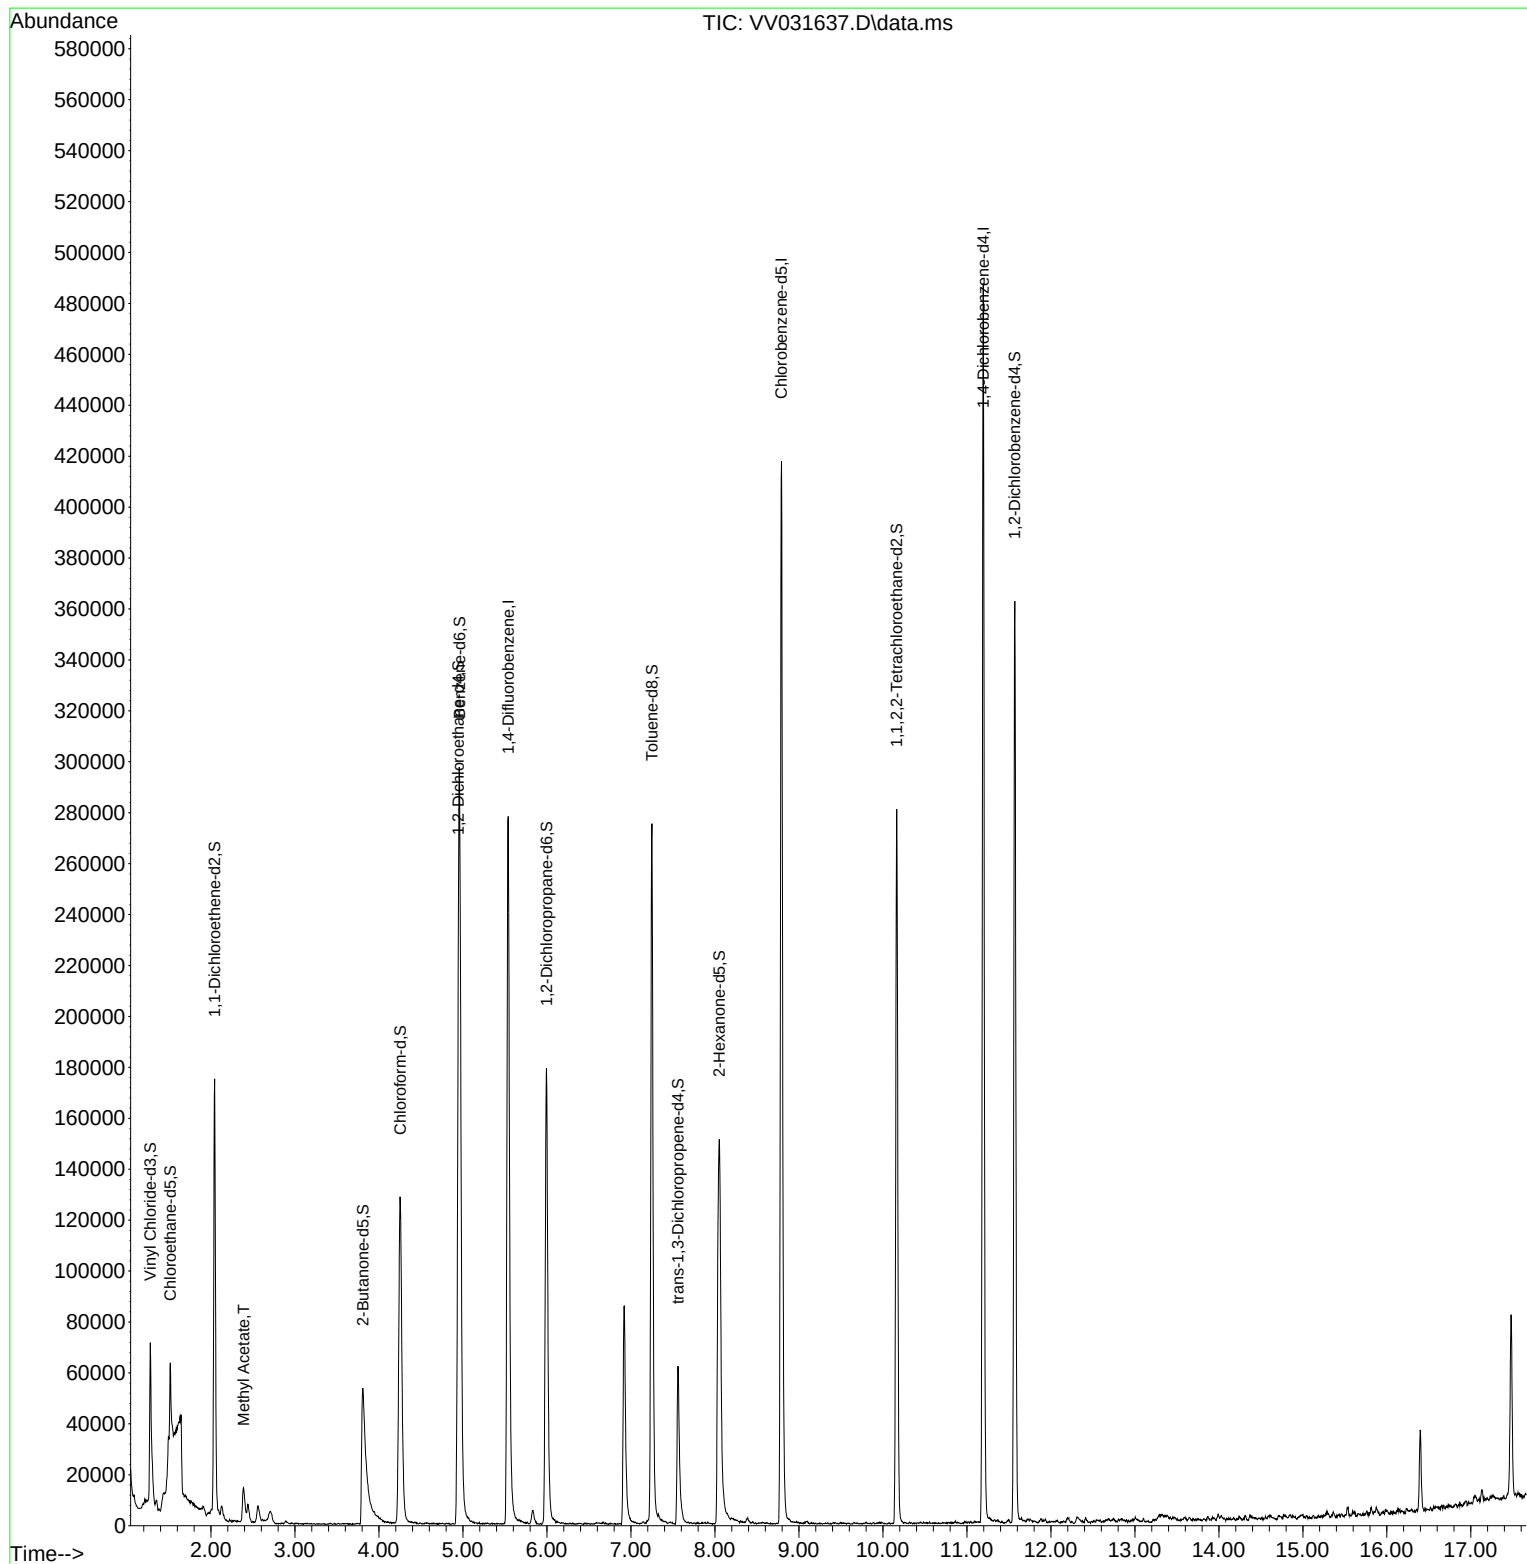

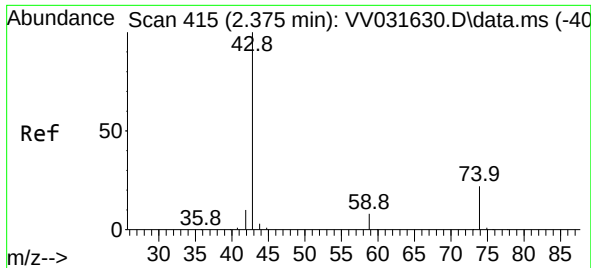

#15
Methyl Acetate
Concen: 9.234 ug/L
RT: 2.388 min Scan# 41
Delta R.T. 0.013 min
Lab File: VV031637.D
Acq: 03 Jul 2023 15:15

Instrument :
MSVOA_V
ClientSampleId :
VIBLK220

Tgt Ion: 43 Resp: 19196
Ion Ratio Lower Upper
43 100
74 22.1 17.8 26.6

