

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070323\
 Data File : VV031631.D
 Acq On : 03 Jul 2023 11:58
 Operator : SY/MD
 Sample : VV0703MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK364

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

Signal : TIC: VV031631.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	69	75	88	rVB	118532	128348	14.14%	1.791%
2	1.532	147	153	166	rVB	113640	130689	14.40%	1.824%
3	2.063	308	318	333	rBV	220457	321755	35.45%	4.491%
4	2.452	431	439	449	rBV3	4457	7263	0.80%	0.101%
5	2.510	454	457	460	rBV3	418	225	0.02%	0.003%
6	2.622	489	492	497	rVB3	362	351	0.04%	0.005%
7	2.677	506	509	512	rBV2	311	175	0.02%	0.002%
8	2.703	512	517	526	rVB5	1260	1632	0.18%	0.023%
9	2.838	557	559	564	rVB2	359	232	0.03%	0.003%
10	2.886	571	574	576	rBV	379	199	0.02%	0.003%
11	2.899	576	578	579	rBV2	340	121	0.01%	0.002%
12	2.966	596	599	602	rBV2	450	349	0.04%	0.005%
13	3.005	609	611	616	rBV2	343	279	0.03%	0.004%
14	3.072	628	632	637	rVB2	495	466	0.05%	0.007%
15	3.153	655	657	660	rBV	211	142	0.02%	0.002%
16	3.207	672	674	678	rVB2	411	249	0.03%	0.003%
17	3.230	678	681	683	rBV2	467	294	0.03%	0.004%
18	3.256	683	689	696	rBV4	447	602	0.07%	0.008%
19	3.343	713	716	720	rVB2	563	309	0.03%	0.004%
20	3.371	721	725	729	rVB	323	284	0.03%	0.004%
21	3.397	729	733	738	rBV2	285	296	0.03%	0.004%
22	3.429	742	743	746	rBV	229	126	0.01%	0.002%
23	3.545	776	779	785	rBV3	260	285	0.03%	0.004%
24	3.584	789	791	796	rVV	214	179	0.02%	0.002%
25	3.629	803	805	810	rVB3	257	204	0.02%	0.003%
26	3.654	810	813	816	rBV2	202	183	0.02%	0.003%
27	3.683	819	822	826	rBV2	324	290	0.03%	0.004%
28	3.744	837	841	845	rBV2	309	237	0.03%	0.003%
29	3.793	845	856	893	rBV	75050	211738	23.33%	2.955%
30	4.252	983	999	1030	rBV	157359	406332	44.77%	5.671%
31	4.584	1100	1102	1106	rBV3	376	315	0.03%	0.004%
32	4.622	1111	1114	1115	rBV2	230	136	0.01%	0.002%
33	4.732	1146	1148	1151	rBV2	490	368	0.04%	0.005%
34	4.815	1168	1174	1178	rBV3	321	386	0.04%	0.005%
35	4.838	1178	1181	1182	rBV	501	256	0.03%	0.004%
36	4.892	1196	1198	1201	rVB2	454	194	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070323\
 Data File : VV031631.D
 Acq On : 03 Jul 2023 11:58
 Operator : SY/MD
 Sample : VV0703MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK364

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

37	4.960	1201	1219	1243	rBV2	339862	907668	100.00%	12.669%
38	5.265	1313	1314	1316	rBV	353	118	0.01%	0.002%
39	5.304	1324	1326	1329	rBV	262	186	0.02%	0.003%
40	5.394	1350	1354	1358	rVB	428	312	0.03%	0.004%
41	5.423	1358	1363	1365	rBV3	424	386	0.04%	0.005%
42	5.539	1385	1399	1424	rBV	276632	571903	63.01%	7.982%
43	5.783	1472	1475	1477	rBV3	610	365	0.04%	0.005%
44	5.831	1481	1490	1491	rBV5	3645	4037	0.44%	0.056%
45	5.892	1506	1509	1513	rVB4	387	241	0.03%	0.003%
46	5.992	1526	1540	1563	rBV	217172	454231	50.04%	6.340%
47	6.236	1614	1616	1618	rBV2	213	127	0.01%	0.002%
48	6.249	1618	1620	1622	rVB2	393	162	0.02%	0.002%
49	6.307	1636	1638	1641	rBV	501	264	0.03%	0.004%
50	6.323	1641	1643	1647	rVV2	332	209	0.02%	0.003%
51	6.349	1647	1651	1655	rVB3	431	431	0.05%	0.006%
52	6.397	1662	1666	1669	rBV2	539	418	0.05%	0.006%
53	6.452	1680	1683	1685	rBV3	367	206	0.02%	0.003%
54	6.503	1697	1699	1702	rBV2	403	147	0.02%	0.002%
55	6.564	1713	1718	1722	rBV4	929	1199	0.13%	0.017%
56	6.703	1759	1761	1766	rBV3	565	419	0.05%	0.006%
57	6.796	1786	1790	1792	rBV2	287	187	0.02%	0.003%
58	6.863	1808	1811	1813	rBV2	233	150	0.02%	0.002%
59	6.918	1817	1828	1854	rBV	100900	195211	21.51%	2.725%
60	7.175	1903	1908	1911	rBV5	823	815	0.09%	0.011%
61	7.191	1911	1913	1914	rBV	364	127	0.01%	0.002%
62	7.249	1918	1931	1951	rBV	347399	602883	66.42%	8.415%
63	7.558	2015	2027	2049	rBV	75904	142180	15.66%	1.984%
64	7.751	2085	2087	2090	rBV3	355	156	0.02%	0.002%
65	7.876	2123	2126	2129	rBV2	515	393	0.04%	0.005%
66	8.030	2164	2174	2205	rBV	251675	455810	50.22%	6.362%
67	8.442	2298	2302	2303	rBV	221	159	0.02%	0.002%
68	8.481	2308	2314	2316	rBV3	502	456	0.05%	0.006%
69	8.542	2328	2333	2335	rBV2	560	469	0.05%	0.007%
70	8.616	2353	2356	2358	rBV3	634	370	0.04%	0.005%
71	8.667	2369	2372	2374	rBV	598	258	0.03%	0.004%
72	8.741	2393	2395	2398	rVB3	391	227	0.03%	0.003%
73	8.789	2398	2410	2430	rBV	425784	707319	77.93%	9.872%
74	9.085	2500	2502	2506	rBV3	688	480	0.05%	0.007%
75	9.165	2523	2527	2532	rBV	438	467	0.05%	0.007%
76	9.217	2542	2543	2546	rVB	442	137	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070323\
 Data File : VV031631.D
 Acq On : 03 Jul 2023 11:58
 Operator : SY/MD
 Sample : VV0703MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK364

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

77	9.358	2584	2587	2588	rBV	288	133	0.01%	0.002%
78	9.429	2604	2609	2611	rBV2	560	313	0.03%	0.004%
79	9.590	2657	2659	2661	rBV2	463	190	0.02%	0.003%
80	9.635	2670	2673	2678	rBV2	281	282	0.03%	0.004%
81	9.770	2713	2715	2717	rBV3	364	155	0.02%	0.002%
82	9.805	2723	2726	2730	rVB2	388	228	0.03%	0.003%
83	9.828	2730	2733	2735	rBV2	252	144	0.02%	0.002%
84	9.847	2735	2739	2740	rBV2	342	201	0.02%	0.003%
85	10.001	2784	2787	2789	rBV	314	225	0.02%	0.003%
86	10.066	2805	2807	2810	rVB2	219	122	0.01%	0.002%
87	10.159	2824	2836	2859	rBV	330284	518306	57.10%	7.234%
88	10.390	2903	2908	2911	rBV3	415	375	0.04%	0.005%
89	10.628	2979	2982	2985	rBV	285	196	0.02%	0.003%
90	10.760	3019	3023	3026	rBV2	364	322	0.04%	0.004%
91	10.808	3035	3038	3040	rBV2	349	202	0.02%	0.003%
92	10.863	3049	3055	3057	rBV2	597	606	0.07%	0.008%
93	10.979	3089	3091	3094	rVB	380	147	0.02%	0.002%
94	11.001	3094	3098	3101	rBV2	446	347	0.04%	0.005%
95	11.034	3105	3108	3111	rBV	325	229	0.03%	0.003%
96	11.085	3120	3124	3125	rBV3	327	238	0.03%	0.003%
97	11.191	3145	3157	3185	rBV	451263	693548	76.41%	9.680%
98	11.567	3262	3274	3299	rBV	417278	660816	72.80%	9.223%
99	13.207	3776	3784	3793	rBV7	3565	5212	0.57%	0.073%
100	13.451	3852	3860	3869	rVB2	9667	15318	1.69%	0.214%




Sum of corrected areas: 7164627

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070323\
Data File : VV031631.D
Acq On : 03 Jul 2023 11:58
Operator : SY/MD
Sample : VV0703MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK364

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

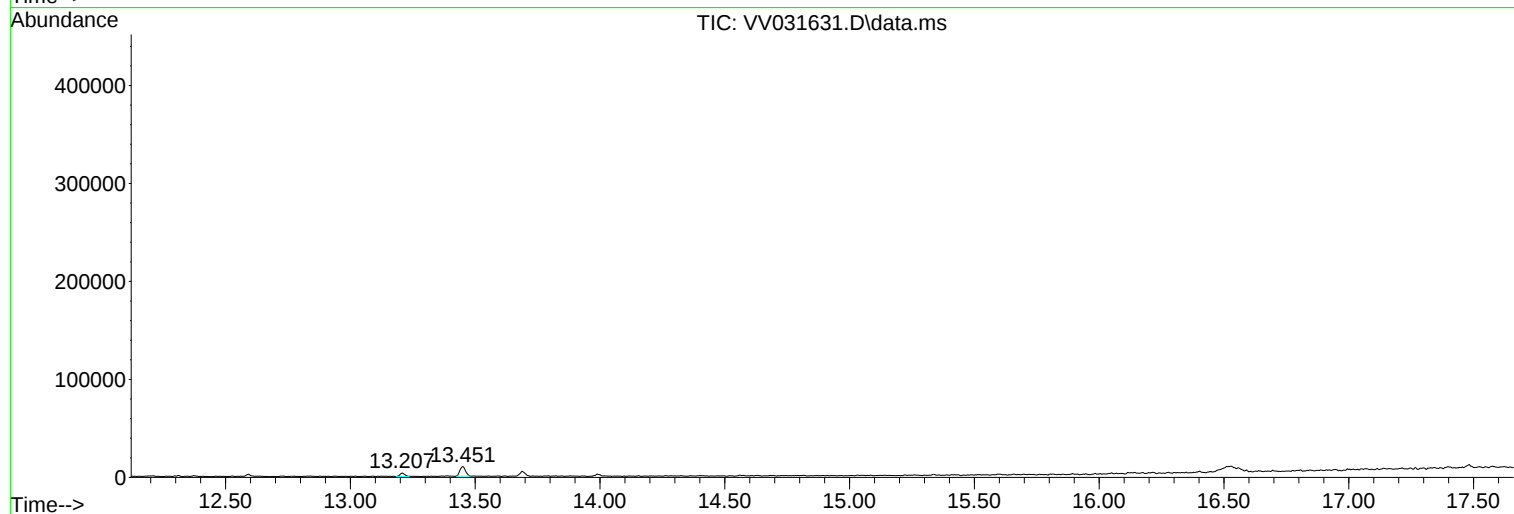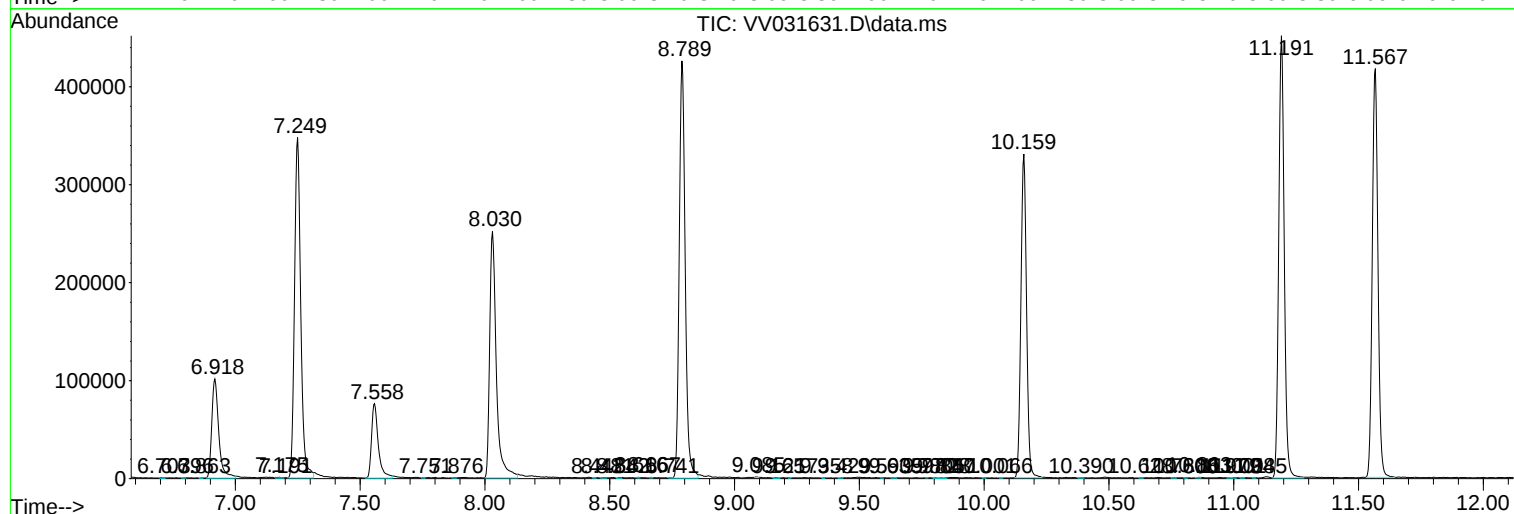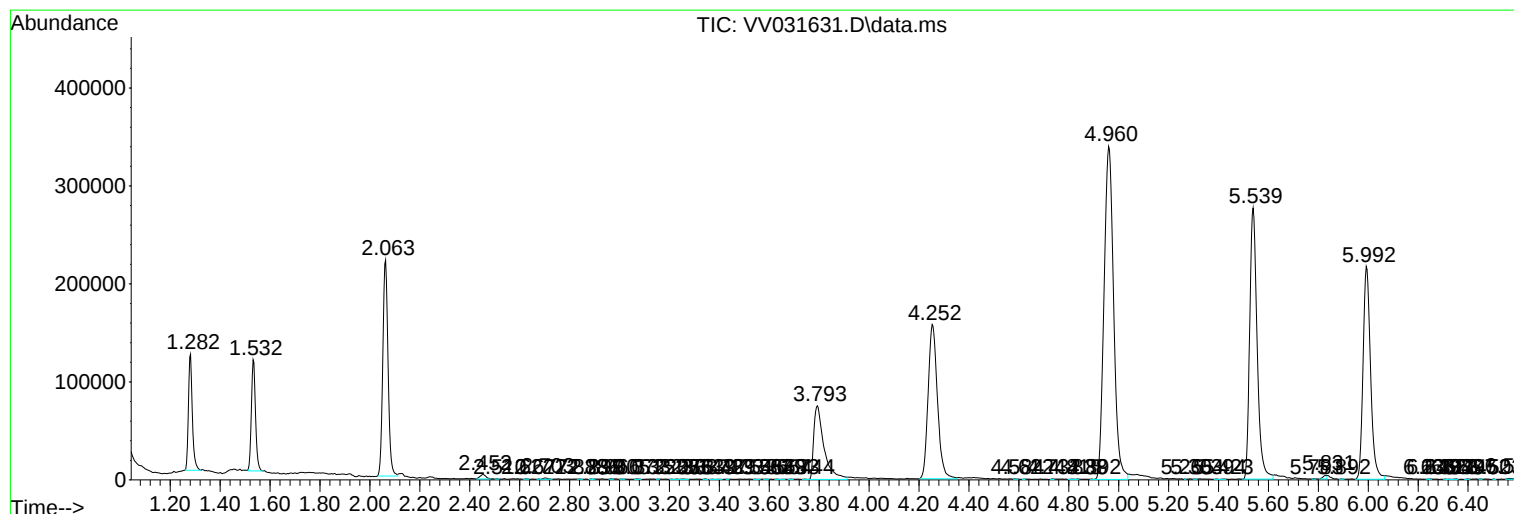

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070323\
Data File : VV031631.D
Acq On : 03 Jul 2023 11:58
Operator : SY/MD
Sample : VV0703MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK364

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070323\
Data File : VV031631.D
Acq On : 03 Jul 2023 11:58
Operator : SY/MD
Sample : VV0703MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK364

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------