

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070323\
 Data File : VV031632.D
 Acq On : 03 Jul 2023 12:50
 Operator : SY/MD
 Sample : 03452-15ME
 Misc : 4.19g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A46P7ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

Signal : TIC: VV031632.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	69	74	92	rVB	76935	111681	13.51%	1.654%
2	2.044	303	312	330	rVB	197540	288911	34.95%	4.279%
3	2.558	462	472	484	rBV4	5239	11033	1.33%	0.163%
4	2.841	557	560	561	rBV2	312	183	0.02%	0.003%
5	3.095	637	639	640	rBV	343	156	0.02%	0.002%
6	3.150	651	656	657	rBV2	313	232	0.03%	0.003%
7	3.227	677	680	682	rBV2	379	167	0.02%	0.002%
8	3.320	706	709	712	rBV3	376	211	0.03%	0.003%
9	3.368	719	724	731	rBV3	291	359	0.04%	0.005%
10	3.397	731	733	735	rBV	254	133	0.02%	0.002%
11	3.410	735	737	743	rBV2	240	178	0.02%	0.003%
12	3.439	743	746	748	rBV3	296	205	0.02%	0.003%
13	3.468	753	755	760	rVB3	210	169	0.02%	0.003%
14	3.719	829	833	836	rBV3	296	277	0.03%	0.004%
15	3.745	838	841	843	rBV	307	150	0.02%	0.002%
16	3.802	846	859	897	rBV	49931	186136	22.52%	2.757%
17	4.159	968	970	971	rBV2	339	124	0.02%	0.002%
18	4.249	983	998	1023	rBV2	133536	346946	41.97%	5.138%
19	4.536	1085	1087	1088	rBV	514	208	0.03%	0.003%
20	4.564	1095	1096	1098	rBV	341	153	0.02%	0.002%
21	4.629	1115	1116	1118	rBV	302	166	0.02%	0.002%
22	4.722	1143	1145	1146	rVB	386	147	0.02%	0.002%
23	4.735	1146	1149	1151	rVB2	362	202	0.02%	0.003%
24	4.751	1151	1154	1159	rBV2	184	162	0.02%	0.002%
25	4.860	1185	1188	1192	rBV	292	239	0.03%	0.004%
26	4.954	1197	1217	1244	rBV3	310008	805066	97.39%	11.923%
27	5.372	1345	1347	1351	rBV2	356	265	0.03%	0.004%
28	5.407	1356	1358	1362	rBV2	444	306	0.04%	0.005%
29	5.445	1367	1370	1375	rBV2	229	180	0.02%	0.003%
30	5.468	1375	1377	1379	rVB2	342	149	0.02%	0.002%
31	5.481	1379	1381	1384	rVB2	371	151	0.02%	0.002%
32	5.535	1385	1398	1428	rBV	295584	627954	75.96%	9.300%
33	5.786	1474	1476	1478	rBV2	424	269	0.03%	0.004%
34	5.925	1514	1519	1520	rBV3	520	441	0.05%	0.007%
35	5.992	1527	1540	1566	rBV	183376	394185	47.68%	5.838%
36	6.249	1618	1620	1621	rBV	266	120	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070323\
 Data File : VV031632.D
 Acq On : 03 Jul 2023 12:50
 Operator : SY/MD
 Sample : 03452-15ME
 Misc : 4.19g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A46P7ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

37	6.259	1621	1623	1626	rVV2	388	203	0.02%	0.003%
38	6.275	1626	1628	1631	rVV2	310	152	0.02%	0.002%
39	6.307	1636	1638	1641	rVB3	451	237	0.03%	0.004%
40	6.359	1650	1654	1657	rBV3	482	431	0.05%	0.006%
41	6.445	1677	1681	1688	rBV3	514	672	0.08%	0.010%
42	6.500	1696	1698	1702	rBV	394	306	0.04%	0.005%
43	6.542	1708	1711	1713	rBV	365	218	0.03%	0.003%
44	6.558	1713	1716	1717	rBV	264	132	0.02%	0.002%
45	6.722	1764	1767	1769	rBV	385	285	0.03%	0.004%
46	6.761	1776	1779	1782	rBV3	399	295	0.04%	0.004%
47	6.796	1788	1790	1793	rVB	377	210	0.03%	0.003%
48	6.860	1807	1810	1811	rBV	269	143	0.02%	0.002%
49	6.918	1814	1828	1856	rBV2	88546	177505	21.47%	2.629%
50	7.191	1905	1913	1915	rBV4	912	1055	0.13%	0.016%
51	7.246	1919	1930	1956	rVV	294292	533778	64.57%	7.905%
52	7.558	2015	2027	2051	rBV	63630	130393	15.77%	1.931%
53	7.728	2078	2080	2083	rBV	393	322	0.04%	0.005%
54	7.789	2097	2099	2102	rBV2	457	226	0.03%	0.003%
55	7.912	2134	2137	2142	rVB2	1016	846	0.10%	0.013%
56	7.960	2149	2152	2158	rBV2	459	413	0.05%	0.006%
57	7.986	2158	2160	2163	rVB2	316	167	0.02%	0.002%
58	8.050	2163	2180	2203	rBV	153013	400420	48.44%	5.930%
59	8.371	2272	2280	2281	rBV4	1513	1336	0.16%	0.020%
60	8.487	2313	2316	2318	rBV2	327	245	0.03%	0.004%
61	8.529	2327	2329	2334	rVB4	747	480	0.06%	0.007%
62	8.548	2334	2335	2336	rBV4	312	115	0.01%	0.002%
63	8.619	2355	2357	2360	rVB	291	150	0.02%	0.002%
64	8.635	2360	2362	2363	rBV2	362	135	0.02%	0.002%
65	8.658	2367	2369	2371	rBV	496	306	0.04%	0.005%
66	8.789	2398	2410	2434	rBV	448500	773670	93.59%	11.458%
67	8.947	2457	2459	2463	rBV5	718	505	0.06%	0.007%
68	9.072	2495	2498	2499	rBV	542	220	0.03%	0.003%
69	9.159	2523	2525	2529	rBV3	452	346	0.04%	0.005%
70	9.198	2534	2537	2541	rBV2	241	233	0.03%	0.003%
71	9.336	2576	2580	2582	rBV2	404	305	0.04%	0.005%
72	9.410	2600	2603	2604	rBV2	527	291	0.04%	0.004%
73	9.465	2617	2620	2622	rBV2	341	202	0.02%	0.003%
74	9.484	2622	2626	2628	rBV2	440	356	0.04%	0.005%
75	9.574	2652	2654	2658	rBV2	269	200	0.02%	0.003%
76	9.641	2673	2675	2678	rBV	299	170	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070323\
 Data File : VV031632.D
 Acq On : 03 Jul 2023 12:50
 Operator : SY/MD
 Sample : 03452-15ME
 Misc : 4.19g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A46P7ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

77	9.664	2678	2682	2684	rVV3	653	501	0.06%	0.007%
78	9.706	2693	2695	2699	rBV2	611	543	0.07%	0.008%
79	9.757	2708	2711	2714	rBV3	269	153	0.02%	0.002%
80	9.773	2714	2716	2718	rBV	436	273	0.03%	0.004%
81	9.854	2737	2741	2742	rBV2	387	217	0.03%	0.003%
82	9.870	2742	2746	2749	rVV4	610	514	0.06%	0.008%
83	9.947	2767	2770	2771	rBV2	471	281	0.03%	0.004%
84	10.005	2784	2788	2789	rBV2	377	221	0.03%	0.003%
85	10.162	2824	2837	2855	rBV	291728	478733	57.91%	7.090%
86	10.323	2882	2887	2890	rBV2	734	761	0.09%	0.011%
87	10.593	2969	2971	2973	rBV2	328	164	0.02%	0.002%
88	10.612	2975	2977	2979	rVB	439	129	0.02%	0.002%
89	10.625	2979	2981	2984	rVB2	348	154	0.02%	0.002%
90	10.693	2998	3002	3003	rBV	527	302	0.04%	0.004%
91	10.809	3036	3038	3040	rBV2	874	518	0.06%	0.008%
92	10.850	3049	3051	3054	rBV3	753	440	0.05%	0.007%
93	10.899	3063	3066	3067	rBV2	622	317	0.04%	0.005%
94	10.966	3084	3087	3088	rBV2	315	134	0.02%	0.002%
95	11.047	3110	3112	3120	rVB4	840	617	0.07%	0.009%
96	11.194	3146	3158	3178	rBV	520990	826651	100.00%	12.242%
97	11.468	3239	3243	3245	rBV3	904	721	0.09%	0.011%
98	11.571	3263	3275	3294	rBV	390682	629575	76.16%	9.324%
99	11.850	3360	3362	3363	rBV	825	426	0.05%	0.006%
100	12.201	3462	3471	3477	rBV9	3136	4747	0.57%	0.070%




Sum of corrected areas: 6752380

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070323\
Data File : VV031632.D
Acq On : 03 Jul 2023 12:50
Operator : SY/MD
Sample : 03452-15ME
Misc : 4.19g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A46P7ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

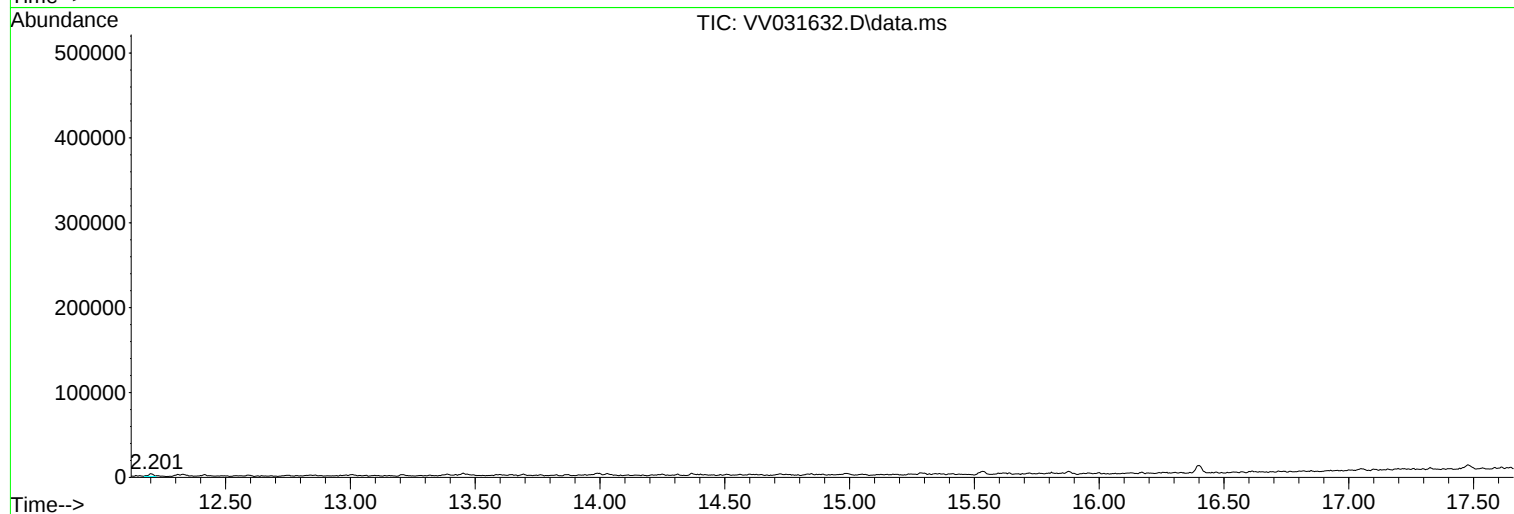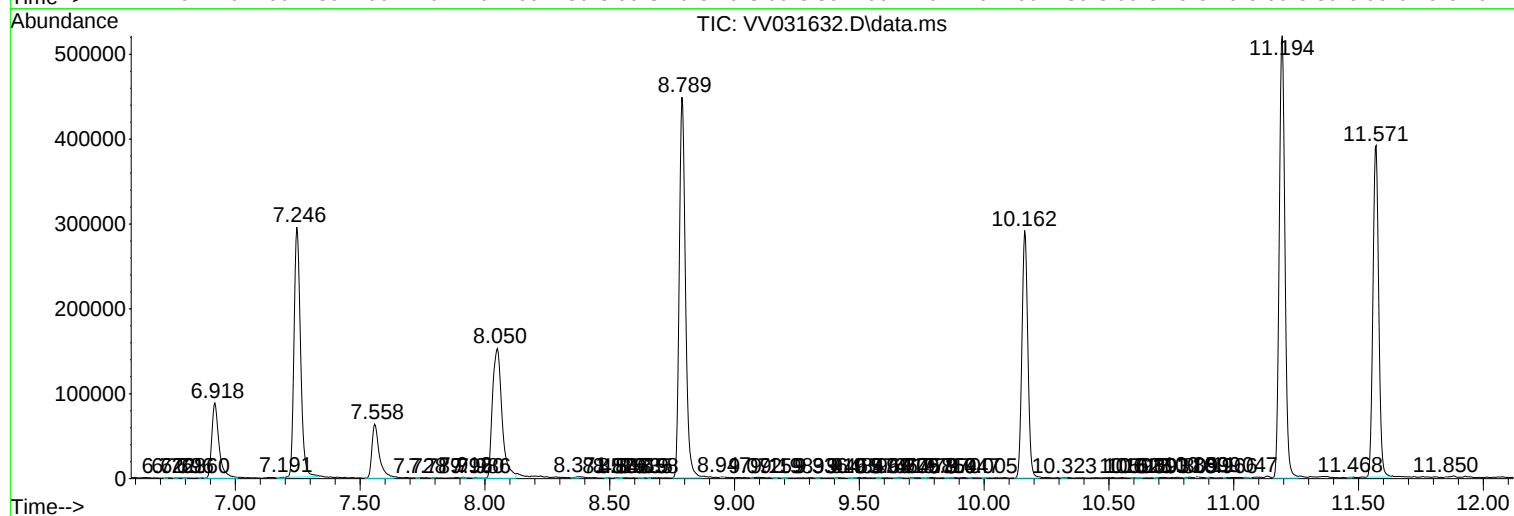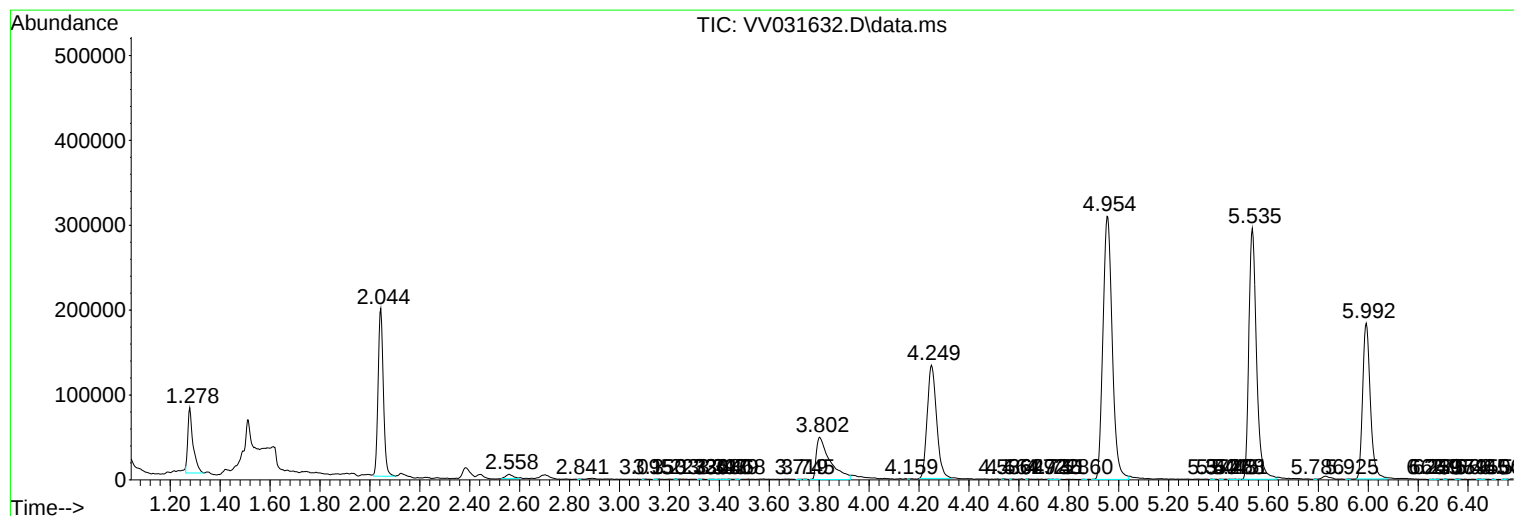

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070323\
Data File : VV031632.D
Acq On : 03 Jul 2023 12:50
Operator : SY/MD
Sample : 03452-15ME
Misc : 4.19g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A46P7ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070323\
Data File : VV031632.D
Acq On : 03 Jul 2023 12:50
Operator : SY/MD
Sample : 03452-15ME
Misc : 4.19g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A46P7ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------