

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070323\
 Data File : VV031637.D
 Acq On : 03 Jul 2023 15:15
 Operator : SY/MD
 Sample : VIBLK220
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK220

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

Signal : TIC: VV031637.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	69	74	91	rVB	63510	93699	12.15%	1.457%
2	2.044	303	312	325	rVB	169439	241183	31.28%	3.751%
3	2.388	411	419	429	rBV2	12721	24968	3.24%	0.388%
4	3.002	607	610	613	rBV	471	304	0.04%	0.005%
5	3.053	623	626	627	rBV2	221	142	0.02%	0.002%
6	3.088	635	637	641	rVB	271	173	0.02%	0.003%
7	3.114	641	645	646	rBV2	292	202	0.03%	0.003%
8	3.143	651	654	656	rVV	285	154	0.02%	0.002%
9	3.252	686	688	690	rBV	223	118	0.02%	0.002%
10	3.320	706	709	714	rBV3	281	237	0.03%	0.004%
11	3.346	715	717	722	rVB	392	226	0.03%	0.004%
12	3.391	729	731	733	rVB2	127	71	0.01%	0.001%
13	3.416	735	739	742	rVB2	335	272	0.04%	0.004%
14	3.471	751	756	757	rBV	307	216	0.03%	0.003%
15	3.510	765	768	769	rBV2	296	180	0.02%	0.003%
16	3.587	790	792	793	rBV	211	85	0.01%	0.001%
17	3.642	808	809	811	rBV	168	79	0.01%	0.001%
18	3.651	811	812	816	rVB	326	154	0.02%	0.002%
19	3.687	821	823	825	rBV	370	151	0.02%	0.002%
20	3.703	825	828	831	rBV	243	139	0.02%	0.002%
21	3.728	831	836	838	rBV2	352	285	0.04%	0.004%
22	3.809	850	861	900	rBV2	53475	201111	26.08%	3.127%
23	4.252	984	999	1029	rVB	127596	332651	43.14%	5.173%
24	4.542	1086	1089	1090	rBV	286	135	0.02%	0.002%
25	4.632	1116	1117	1120	rVB2	356	131	0.02%	0.002%
26	4.654	1120	1124	1129	rBV	420	259	0.03%	0.004%
27	4.703	1137	1139	1141	rBV	346	105	0.01%	0.002%
28	4.725	1144	1146	1151	rVV2	311	208	0.03%	0.003%
29	4.802	1166	1170	1173	rBV2	404	352	0.05%	0.005%
30	4.876	1189	1193	1201	rBV3	365	445	0.06%	0.007%
31	4.957	1201	1218	1251	rBV2	297355	771017	100.00%	11.990%
32	5.195	1291	1292	1296	rVB	626	202	0.03%	0.003%
33	5.249	1307	1309	1312	rVB2	366	199	0.03%	0.003%
34	5.268	1312	1315	1317	rBV2	431	225	0.03%	0.003%
35	5.339	1335	1337	1340	rVB	401	222	0.03%	0.003%
36	5.355	1340	1342	1343	rBV	285	115	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW070323\
 Data File : VW031637.D
 Acq On : 03 Jul 2023 15:15
 Operator : SY/MD
 Sample : VIBLK220
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK220

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

37	5.397	1352	1355	1357	rBV3	289	146	0.02%	0.002%
38	5.468	1375	1377	1380	rBV	257	140	0.02%	0.002%
39	5.494	1383	1385	1386	rBV	371	159	0.02%	0.002%
40	5.539	1386	1399	1428	rBV	277593	592515	76.85%	9.214%
41	5.834	1481	1491	1506	rVB9	5310	11549	1.50%	0.180%
42	5.928	1518	1520	1523	rVB3	462	252	0.03%	0.004%
43	5.995	1523	1541	1565	rBV	179141	386418	50.12%	6.009%
44	6.217	1609	1610	1611	rBV	271	62	0.01%	0.001%
45	6.275	1624	1628	1630	rBV2	407	303	0.04%	0.005%
46	6.310	1635	1639	1642	rBV2	423	315	0.04%	0.005%
47	6.352	1650	1652	1655	rBV2	203	130	0.02%	0.002%
48	6.371	1655	1658	1661	rBV2	311	218	0.03%	0.003%
49	6.442	1678	1680	1681	rBV	495	207	0.03%	0.003%
50	6.468	1686	1688	1690	rVB	377	172	0.02%	0.003%
51	6.526	1703	1706	1709	rBV3	352	243	0.03%	0.004%
52	6.667	1748	1750	1755	rVB3	817	617	0.08%	0.010%
53	6.693	1755	1758	1761	rBV3	527	256	0.03%	0.004%
54	6.706	1761	1762	1768	rVB2	361	243	0.03%	0.004%
55	6.731	1768	1770	1772	rVB2	267	112	0.01%	0.002%
56	6.754	1772	1777	1779	rBV2	544	416	0.05%	0.006%
57	6.767	1779	1781	1784	rBV	200	143	0.02%	0.002%
58	6.831	1799	1801	1803	rBV	180	101	0.01%	0.002%
59	6.860	1808	1810	1811	rBV	329	119	0.02%	0.002%
60	6.921	1818	1829	1854	rBV	85830	176285	22.86%	2.741%
61	7.188	1910	1912	1914	rBV	810	526	0.07%	0.008%
62	7.249	1919	1931	1953	rVV	273808	498367	64.64%	7.750%
63	7.561	2018	2028	2054	rBV	61972	125856	16.32%	1.957%
64	7.706	2071	2073	2075	rBV2	383	272	0.04%	0.004%
65	7.786	2094	2098	2100	rBV3	529	427	0.06%	0.007%
66	7.844	2114	2116	2118	rBV	373	122	0.02%	0.002%
67	7.915	2135	2138	2143	rBV4	664	557	0.07%	0.009%
68	7.982	2156	2159	2163	rBV3	391	395	0.05%	0.006%
69	8.053	2163	2181	2208	rBV	151195	418701	54.31%	6.511%
70	8.509	2319	2323	2325	rBV2	350	318	0.04%	0.005%
71	8.664	2369	2371	2373	rBV	401	202	0.03%	0.003%
72	8.792	2399	2411	2438	rBV	417174	729668	94.64%	11.347%
73	9.014	2478	2480	2484	rBV2	482	319	0.04%	0.005%
74	9.063	2493	2495	2498	rBV2	548	346	0.04%	0.005%
75	9.085	2499	2502	2503	rBV2	685	430	0.06%	0.007%
76	9.140	2515	2519	2520	rBV	292	181	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070323\
 Data File : VV031637.D
 Acq On : 03 Jul 2023 15:15
 Operator : SY/MD
 Sample : VIBLK220
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK220

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

77	9.149	2520	2522	2527	rVV2	629	435	0.06%	0.007%
78	9.172	2527	2529	2533	rVB2	491	304	0.04%	0.005%
79	9.198	2533	2537	2543	rVB3	351	294	0.04%	0.005%
80	9.233	2543	2548	2550	rBV3	314	280	0.04%	0.004%
81	9.262	2555	2557	2559	rBV	301	125	0.02%	0.002%
82	9.297	2563	2568	2570	rBV2	297	315	0.04%	0.005%
83	9.374	2591	2592	2596	rVB	286	173	0.02%	0.003%
84	9.509	2632	2634	2637	rBV4	450	260	0.03%	0.004%
85	9.574	2652	2654	2655	rBV	340	140	0.02%	0.002%
86	9.657	2674	2680	2683	rBV4	662	716	0.09%	0.011%
87	9.747	2706	2708	2710	rVB	318	124	0.02%	0.002%
88	9.767	2711	2714	2716	rBV3	365	254	0.03%	0.004%
89	9.889	2746	2752	2757	rVB4	656	696	0.09%	0.011%
90	9.982	2779	2781	2786	rBV2	413	271	0.04%	0.004%
91	10.098	2814	2817	2820	rBV	364	269	0.03%	0.004%
92	10.165	2825	2838	2857	rBV	280548	466020	60.44%	7.247%
93	10.484	2934	2937	2939	rBV3	637	372	0.05%	0.006%
94	10.783	3025	3030	3032	rBV4	482	449	0.06%	0.007%
95	10.821	3040	3042	3044	rBV	561	252	0.03%	0.004%
96	10.972	3086	3089	3091	rBV2	927	582	0.08%	0.009%
97	11.194	3147	3158	3175	rBV	486581	753841	97.77%	11.723%
98	11.570	3263	3275	3291	rBV	361866	582368	75.53%	9.056%
99	12.413	3532	3537	3547	rBV9	2047	2801	0.36%	0.044%
100	12.490	3555	3561	3564	rBV3	871	1064	0.14%	0.017%




Sum of corrected areas: 6430628

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070323\
Data File : VV031637.D
Acq On : 03 Jul 2023 15:15
Operator : SY/MD
Sample : VIBLK220
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK220

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

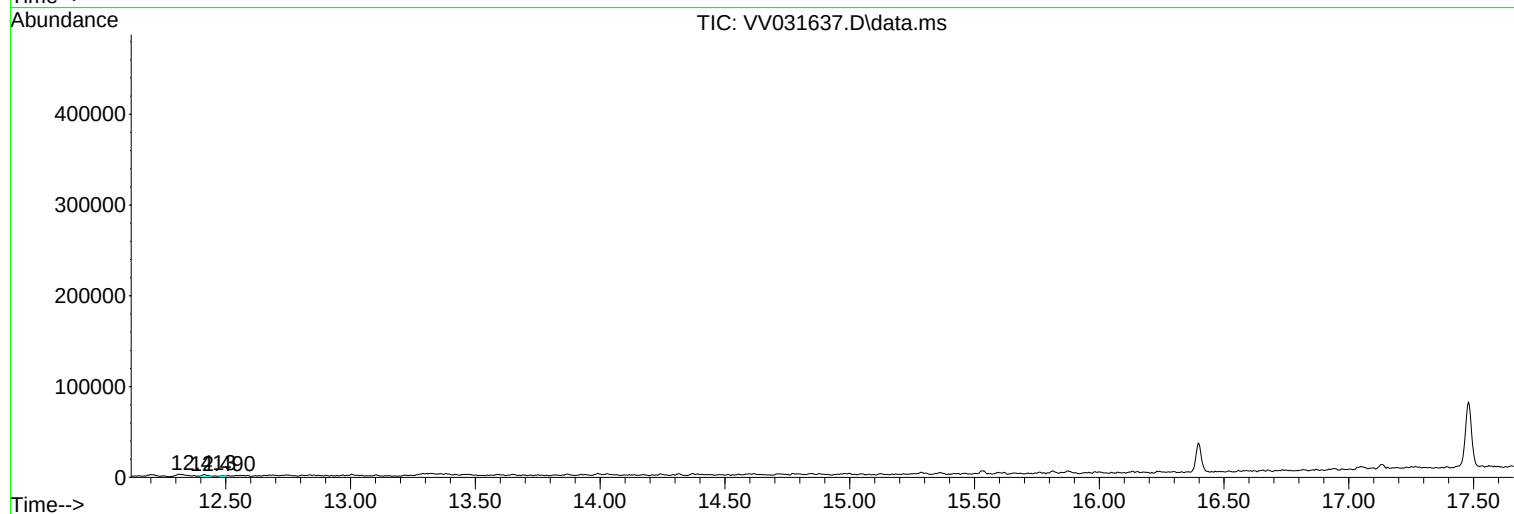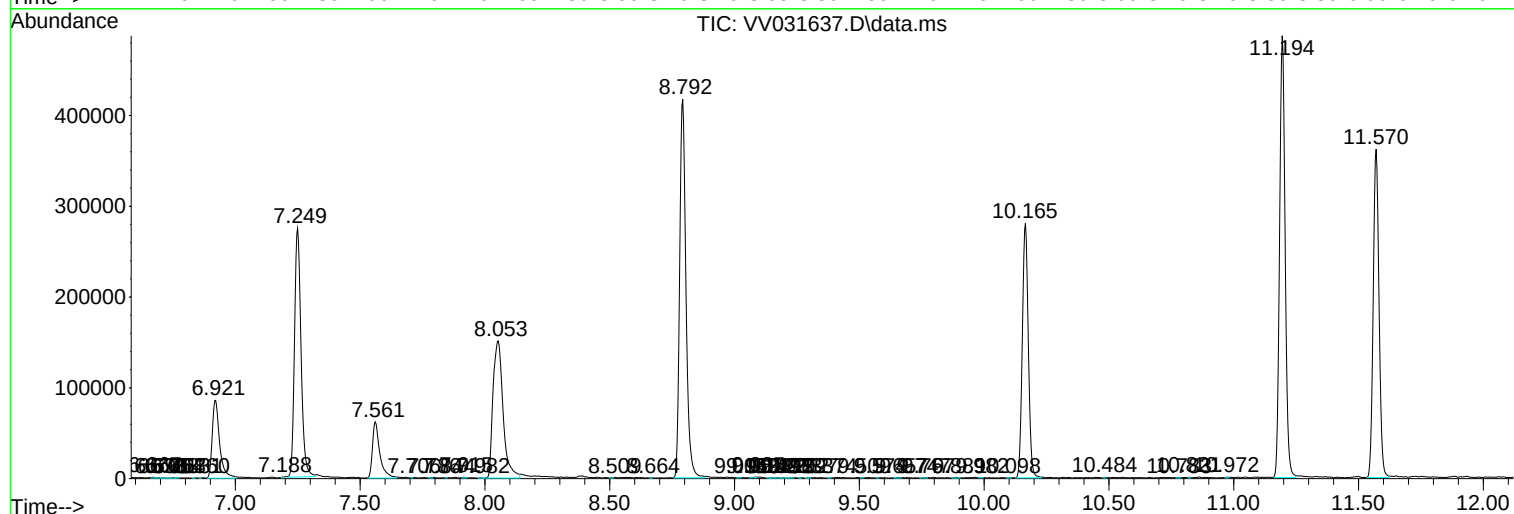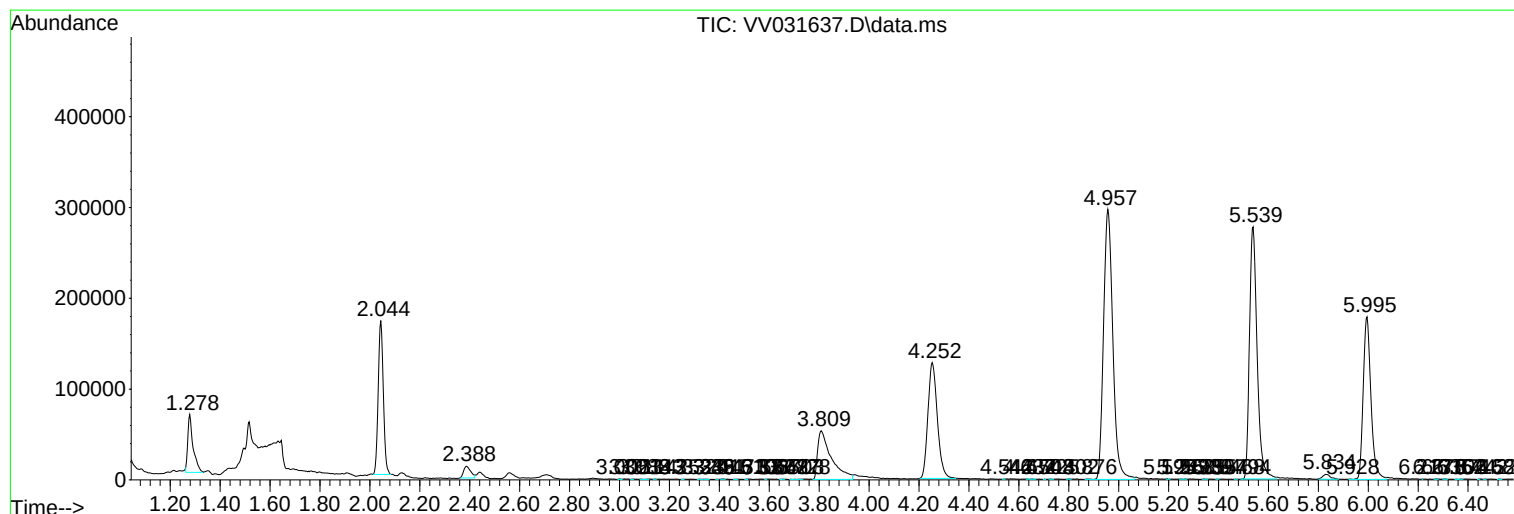

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070323\
Data File : VV031637.D
Acq On : 03 Jul 2023 15:15
Operator : SY/MD
Sample : VIBLK220
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK220

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070323\
Data File : VV031637.D
Acq On : 03 Jul 2023 15:15
Operator : SY/MD
Sample : VIBLK220
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK220

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------