


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070323\
Data File : VV031629.D
Acq On : 03 Jul 2023 10:49
Operator : SY/MD
Sample : BFB393
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB393

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Title : VOC Analysis
Last Update : Tue Jul 04 07:06:08 2023

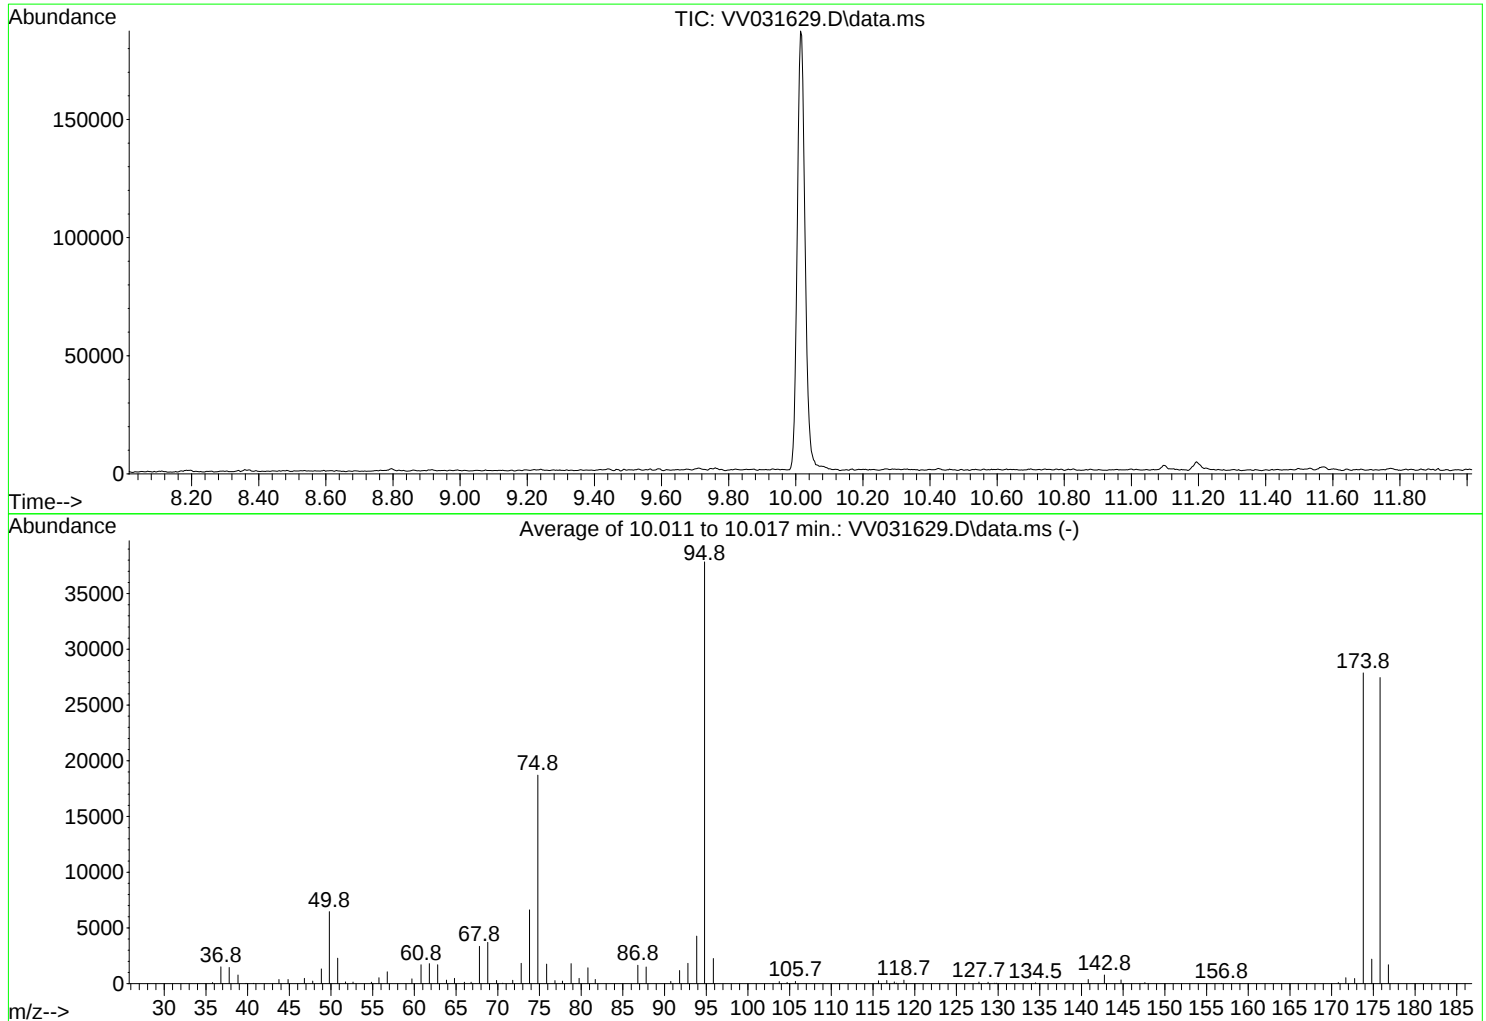

AutoFind: Scans 2790, 2791, 2792; Background Corrected with Scan 2780

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.1	6456	PASS
75	95	30	80	49.4	18707	PASS
95	95	100	100	100.0	37848	PASS
96	95	5	9	6.0	2253	PASS
173	174	0.00	2	1.6	458	PASS
174	95	50	120	73.7	27888	PASS
175	174	5	9	7.9	2196	PASS
176	174	95	105	98.5	27464	PASS
177	176	5	10	6.2	1691	PASS

m/z	Abundance
35.80	898.0
37.80	356.0
39.70	187.0
43.90	303.0

Instrument :
MSVOA_V
ClientSampleId :
BFB393

m/z	Abundance
35.80	954.0
36.80	1455.0
37.80	1701.0
38.90	781.0
39.90	230.0
43.80	595.0
44.90	385.0
46.80	532.0
47.80	226.0
48.80	1308.0
49.80	6358.0
50.80	2148.0
51.70	159.0
52.70	130.0
54.90	147.0
55.80	438.0
56.80	1030.0
59.70	396.0
60.80	1567.0
61.80	1637.0
62.80	1729.0
63.80	300.0
64.80	393.0
66.00	132.0
66.80	135.0
67.80	3233.0
68.80	3554.0
69.90	291.0
71.80	277.0
72.80	1718.0
73.80	6408.0
74.80	17568.0
75.90	1730.0
76.90	253.0
77.80	242.0
78.80	1845.0
79.70	469.0
80.80	1318.0
81.70	408.0
86.80	1563.0
87.80	1576.0
90.80	190.0
91.80	1072.0
92.80	1801.0
93.90	4074.0
94.80	36048.0
95.80	2237.0
103.80	169.0
104.70	102.0
105.70	182.0
115.70	188.0
116.60	263.0
117.50	154.0
117.80	146.0
118.70	275.0
127.80	122.0
128.80	116.0
129.60	118.0
140.80	423.0
142.70	722.0
144.80	360.0
171.70	466.0
172.70	456.0
173.80	25448.0
174.80	2046.0
175.80	26056.0
176.80	1587.0

Instrument :
MSVOA_V
ClientSampleId :
BFB393

m/z	Abundance
35.80	976.0
36.80	1512.0
37.80	1868.0
38.80	787.0
39.90	233.0
43.70	718.0
44.80	370.0
46.80	488.0
47.80	250.0
48.90	1373.0
49.80	6644.0
50.80	2356.0
51.70	148.0
52.70	145.0
54.80	127.0
55.70	536.0
56.80	1105.0
59.70	479.0
60.80	1739.0
61.80	1860.0
62.80	1767.0
63.90	328.0
64.80	477.0
66.00	142.0
66.80	120.0
67.80	3462.0
68.80	3887.0
69.80	294.0
71.80	304.0
72.80	1855.0
73.80	6816.0
74.80	19280.0
75.80	1834.0
76.90	266.0
77.70	250.0
78.80	1849.0
79.80	485.0
80.80	1451.0
81.70	399.0
86.80	1747.0
87.80	1546.0
90.80	207.0
91.80	1207.0
92.80	1904.0
93.80	4377.0
94.80	39272.0
95.80	2277.0
103.80	201.0
104.70	129.0
105.70	219.0
115.60	273.0
116.60	289.0
117.50	191.0
118.70	333.0
127.70	138.0
128.80	143.0
134.50	114.0
140.80	374.0
142.70	823.0
144.80	356.0
147.60	159.0
170.80	124.0
171.70	543.0
172.70	461.0
173.80	28728.0
174.80	2233.0
175.80	28312.0
176.80	1762.0

Instrument :
MSVOA_V
ClientSampleId :
BFB393

m/z	Abundance
35.80	1070.0
36.80	1550.0
37.80	1854.0
38.80	751.0
39.90	191.0
40.70	101.0
43.70	738.0
44.80	348.0
46.80	417.0
47.80	226.0
48.80	1280.0
49.80	6365.0
50.80	2365.0
51.80	149.0
52.60	138.0
54.80	120.0
55.80	603.0
56.70	1051.0
59.70	443.0
60.80	1763.0
61.80	1900.0
62.80	1596.0
63.90	333.0
64.80	552.0
66.00	116.0
66.80	123.0
67.80	3358.0
68.80	3666.0
69.80	266.0
70.60	124.0
71.80	317.0
72.80	1880.0
73.80	6642.0
74.80	19272.0
75.80	1684.0
76.80	319.0
77.70	214.0
78.80	1684.0
79.80	480.0
80.80	1483.0
81.70	332.0
86.80	1636.0
87.80	1366.0
90.70	193.0
91.80	1236.0
92.80	1752.0
93.80	4345.0
94.80	38224.0
95.90	2245.0
103.70	190.0
104.70	107.0
105.70	225.0
115.60	299.0
116.70	303.0
117.60	146.0
118.70	351.0
127.60	166.0
128.80	136.0
129.80	114.0
134.50	130.0
140.80	324.0
142.80	790.0
144.70	283.0
147.60	169.0
156.80	108.0
170.80	162.0
171.70	587.0
172.80	457.0
173.80	29488.0
174.80	2308.0
175.80	28024.0
176.80	1725.0

Instrument :
MSVOA_V
ClientSampleId :
BFB393