
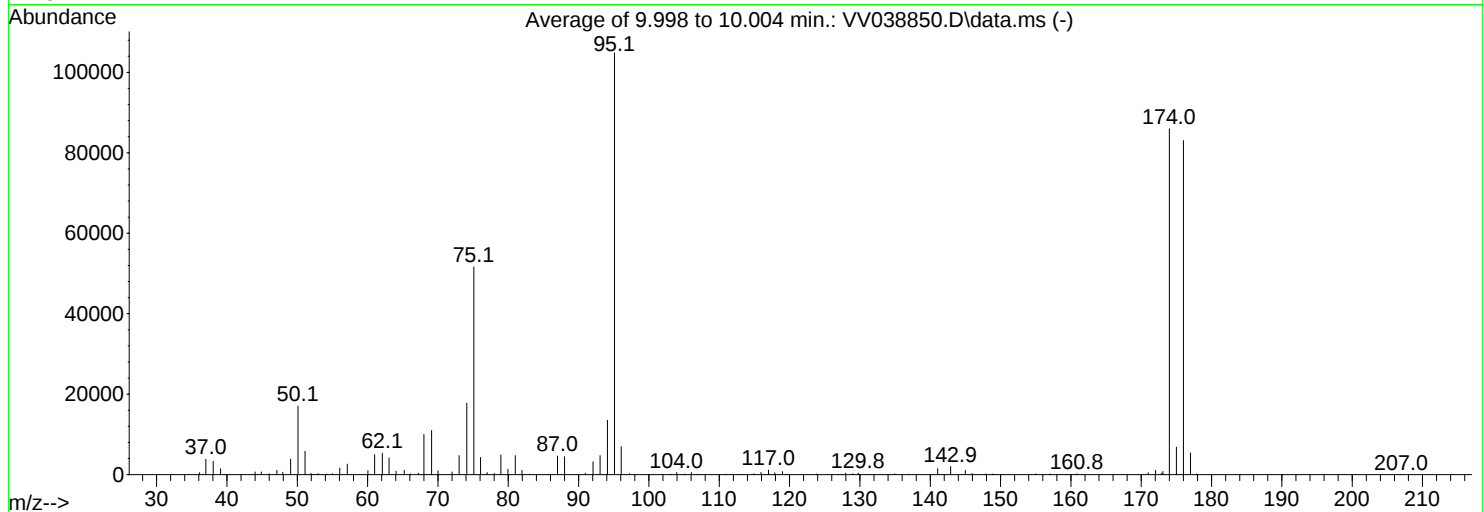


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV070325\
Data File : VV038850.D
Acq On : 03 Jul 2025 08:43
Operator : SY/MD
Sample : BFB
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\82V070225W.M
Title : SW846 8260
Last Update : Thu Jul 03 02:44:44 2025

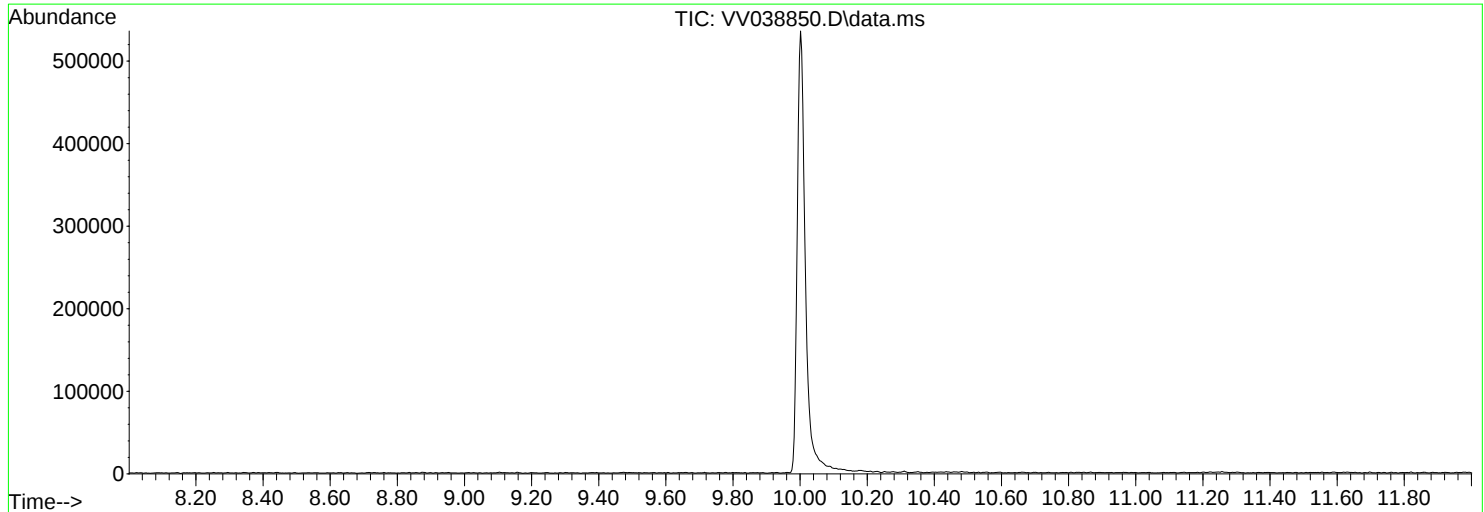

AutoFind: Scans 2786, 2787, 2788; Background Corrected with Scan 2775

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	16.2	17024	PASS
75	95	30	60	49.3	51645	PASS
95	95	100	100	100.0	104848	PASS
96	95	5	9	6.7	6975	PASS
173	174	0.00	2	0.9	816	PASS
174	95	50	100	82.0	85949	PASS
175	174	5	9	7.9	6826	PASS
176	174	95	101	96.6	83053	PASS
177	176	5	9	6.5	5423	PASS