




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070522\
 Data File : VV026644.D
 Acq On : 05 Jul 2022 15:07
 Operator : SY/MD
 Sample : N3506-12
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AM6

Manual IntegrationsAPPROVED

Quant Time: Jul 06 00:24:49 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Jul 06 00:22:14 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 07/06/2022
 Supervised By :Mahesh Dadoda 07/06/2022

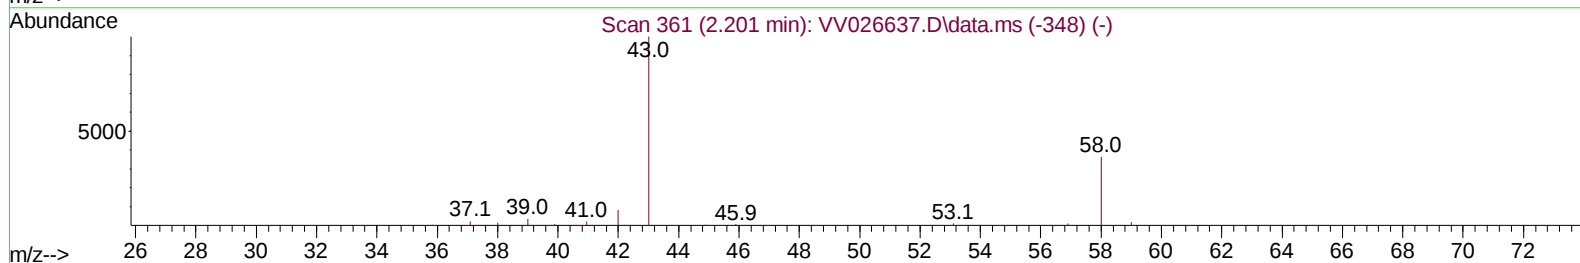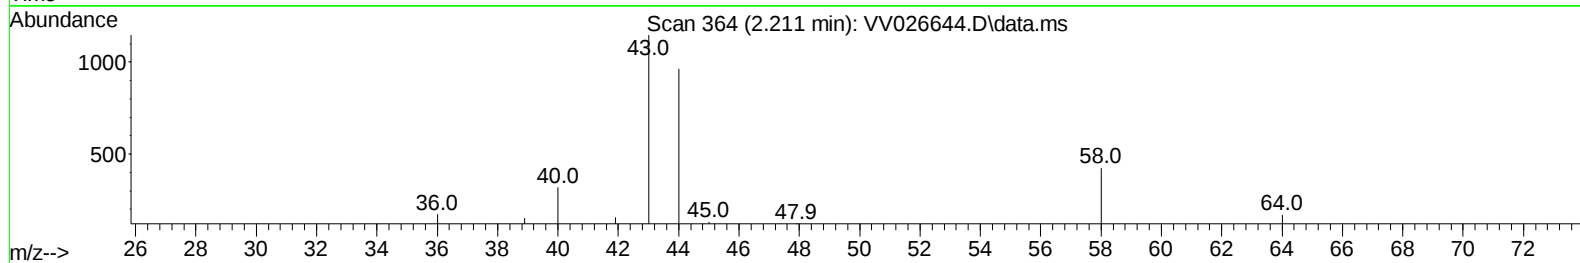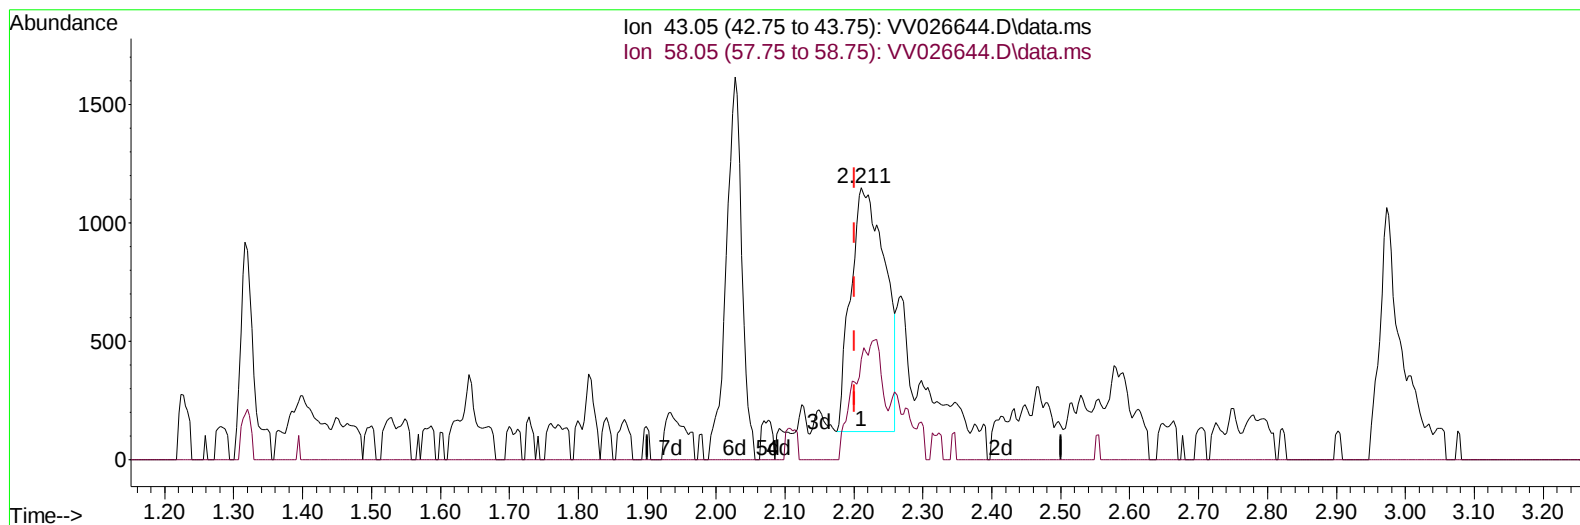

TIC: VV026644.D\data.ms

(13) Acetone (T)

2.211min (+ 0.010) 3.73 ug/L

response 3530

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	37.50	41.16
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070522\
 Data File : VV026644.D
 Acq On : 05 Jul 2022 15:07
 Operator : SY/MD
 Sample : N3506-12
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AM6

Manual IntegrationsAPPROVED

Quant Time: Jul 06 00:24:49 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Jul 06 00:22:14 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 07/06/2022
 Supervised By :Mahesh Dadoda 07/06/2022

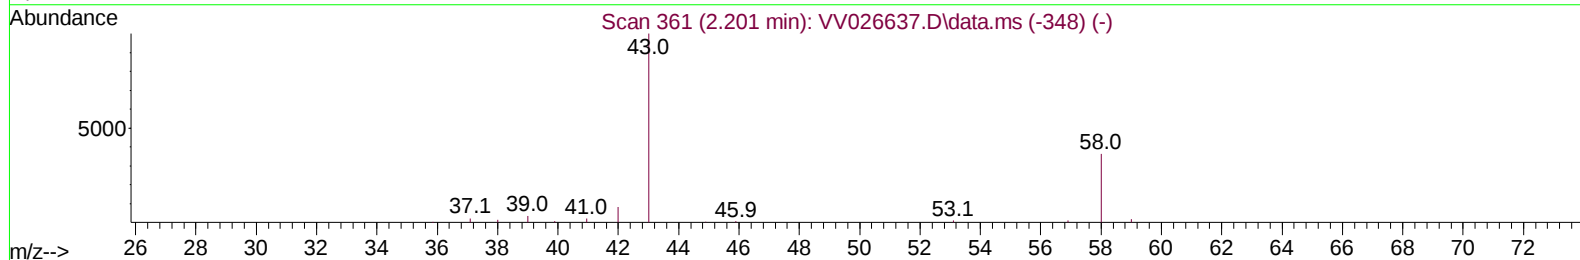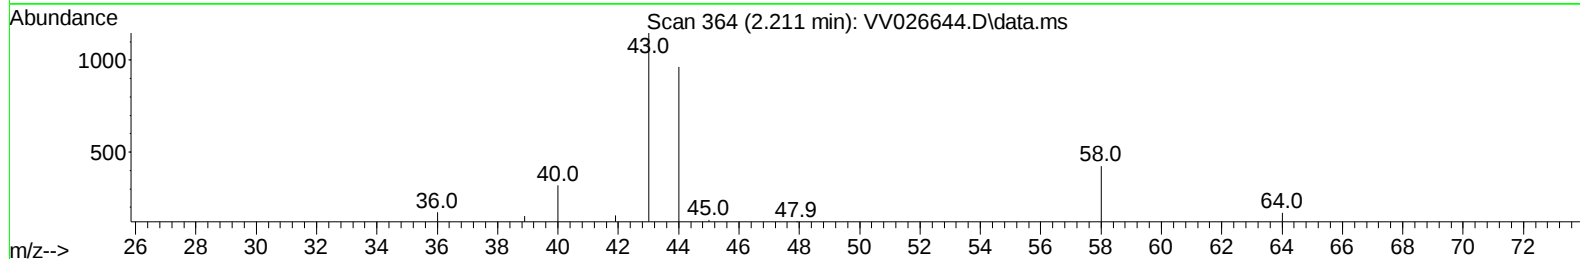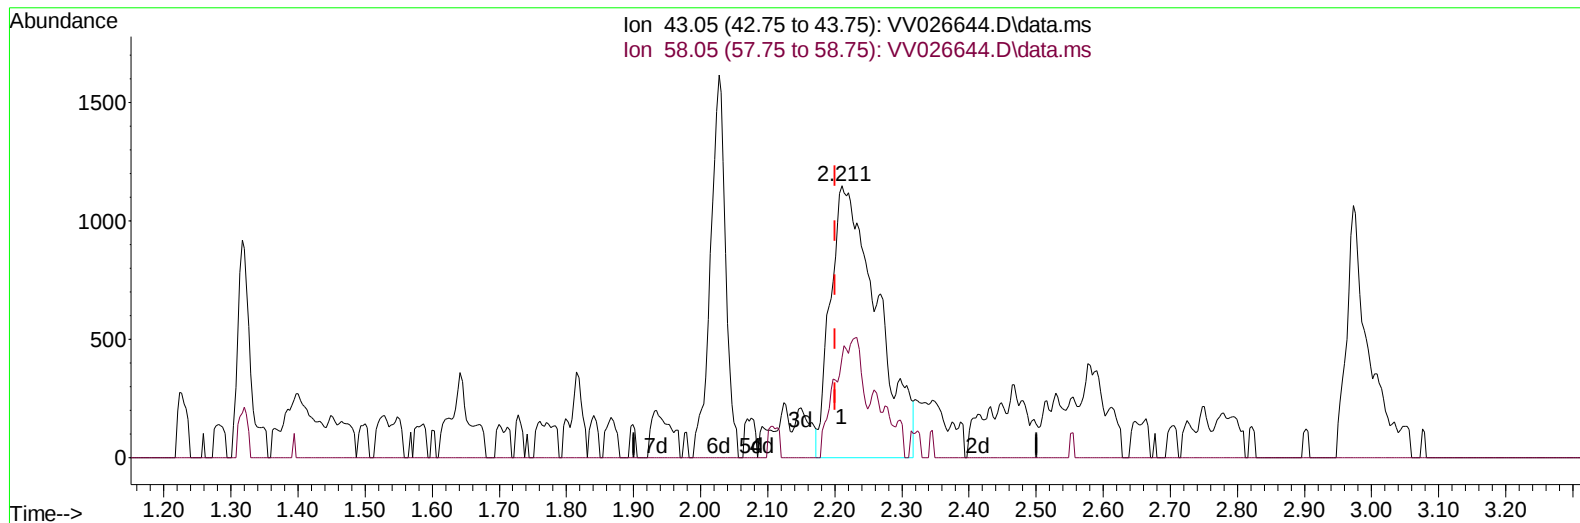

TIC: VV026644.D\data.ms

(13) Acetone (T)

2.211min (+ 0.010) 5.82 ug/L m

response 5505

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	37.50	26.39
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070522\
 Data File : VV026644.D
 Acq On : 05 Jul 2022 15:07
 Operator : SY/MD
 Sample : N3506-12
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AM6

Manual IntegrationsAPPROVED

Quant Time: Jul 06 00:24:49 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Jul 06 00:22:14 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 07/06/2022
 Supervised By :Mahesh Dadoda 07/06/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.622	114	186472	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	182459	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	76390	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.317	65	49642	3.310	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130	Recovery	=	66.200%	
7) Chloroethane-d5	1.577	69	50170	4.164	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130	Recovery	=	83.200%	
11) 1,1-Dichloroethene-d2	2.117	63	72214	2.710	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125	Recovery	=	54.200%#	
20) 2-Butanone-d5	3.924	46	108268	72.617	ug/L	0.00
Spiked Amount 50.000	Range 40	- 130	Recovery	=	145.240%#	
24) Chloroform-d	4.358	84	126542	5.162	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	103.200%	
26) 1,2-Dichloroethane-d4	5.043	65	49577	5.251	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	105.000%	
32) Benzene-d6	5.056	84	206738	3.945	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	78.800%	
36) 1,2-Dichloropropane-d6	6.075	67	69594	4.829	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140	Recovery	=	96.600%	
41) Toluene-d8	7.320	98	164746	3.496	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	70.000%	
43) trans-1,3-Dichloroprop...	7.628	79	16585	4.452	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130	Recovery	=	89.000%	
46) 2-Hexanone-d5	8.091	63	75265	53.044	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130	Recovery	=	106.080%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	52848	5.605	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120	Recovery	=	112.200%	
66) 1,2-Dichlorobenzene-d4	11.625	152	60365	4.775	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120	Recovery	=	95.600%	
Target Compounds						
					Qvalue	
13) Acetone	2.211	43	5505m	5.820	ug/L	
14) Carbon disulfide	2.304	76	18576	0.559	ug/L	99
16) Methylene chloride	2.519	84	6335	0.474	ug/L	97
25) Chloroform	4.387	83	135149	5.475	ug/L	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070522\
Data File : VV026644.D
Acq On : 05 Jul 2022 15:07
Operator : SY/MD
Sample : N3506-12
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 3

Instrument :
MSVOA_V
ClientSampleId :
C0AM6

Manual IntegrationsAPPROVED

Quant Time: Jul 06 00:24:49 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Jul 06 00:22:14 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 07/06/2022
Supervised By :Mahesh Dadoda 07/06/2022

