




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070522\
 Data File : VV026652.D
 Acq On : 05 Jul 2022 18:46
 Operator : SY/MD
 Sample : N3553-12
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AN1

Manual IntegrationsAPPROVED

Quant Time: Jul 06 00:30:23 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Jul 06 00:22:14 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 07/06/2022
 Supervised By :Mahesh Dadoda 07/06/2022

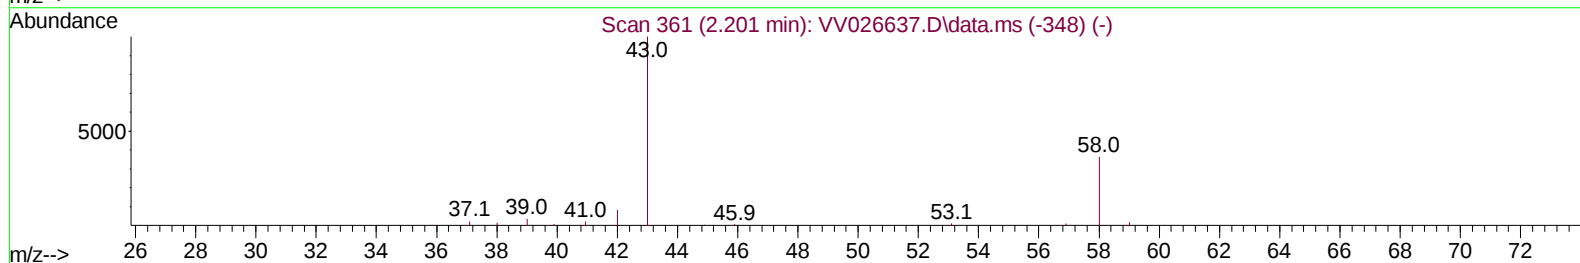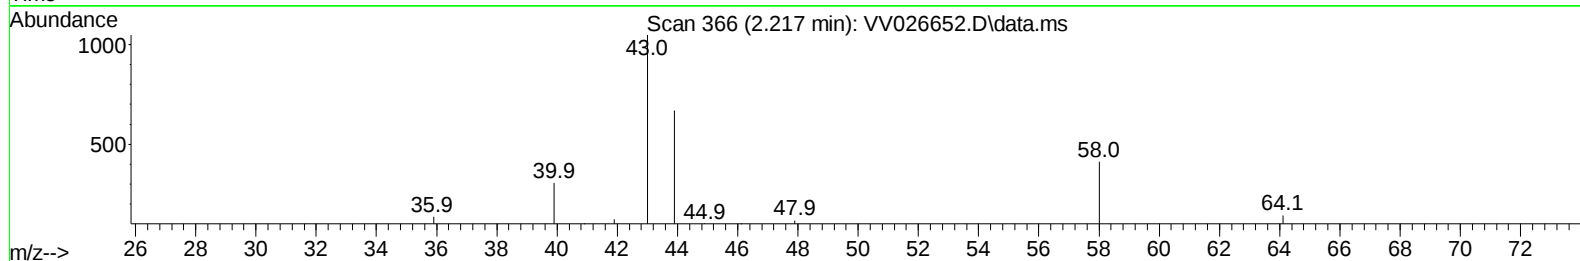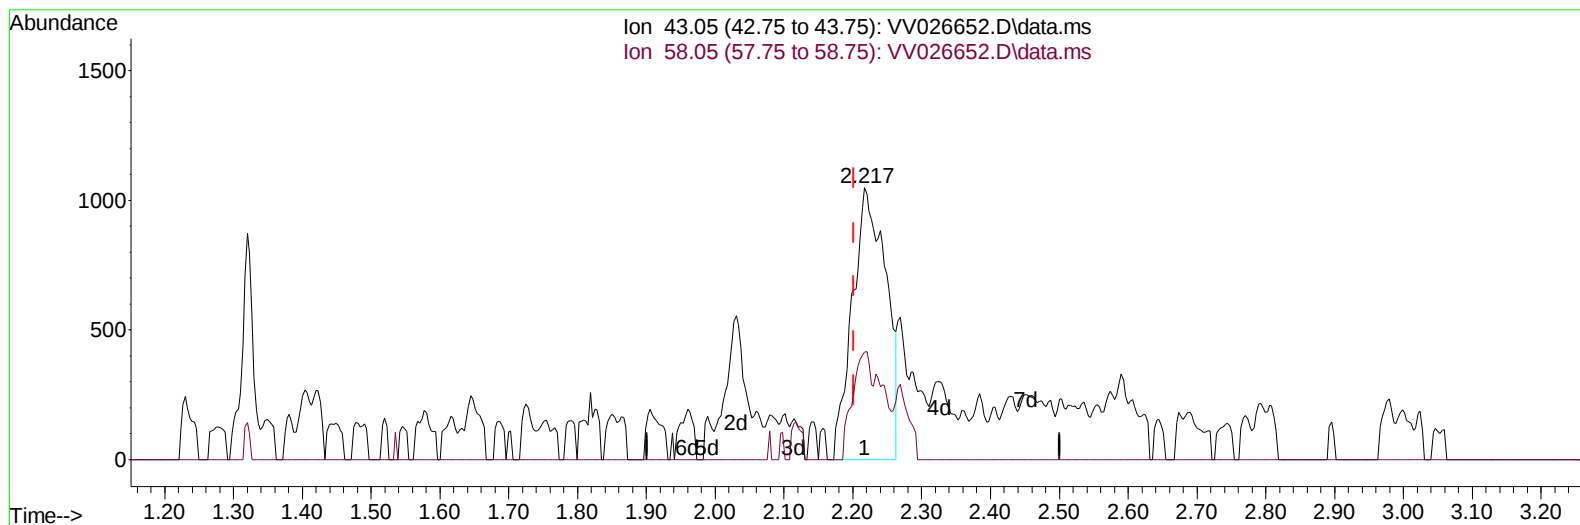

TIC: VV026652.D\data.ms

(13) Acetone (T)

2.217min (+ 0.016) 3.76 ug/L

response 3536

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	37.50	22.94
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070522\
 Data File : VV026652.D
 Acq On : 05 Jul 2022 18:46
 Operator : SY/MD
 Sample : N3553-12
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AN1

Manual IntegrationsAPPROVED

Quant Time: Jul 06 00:30:23 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Jul 06 00:22:14 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 07/06/2022
 Supervised By :Mahesh Dadoda 07/06/2022

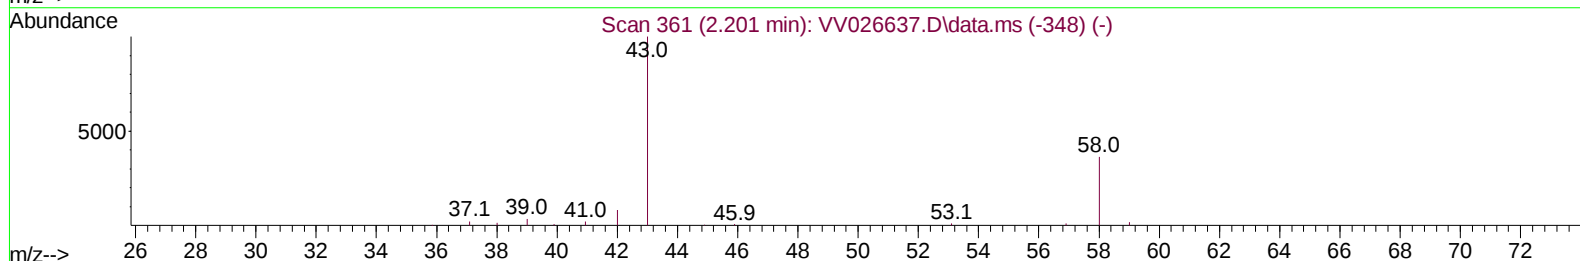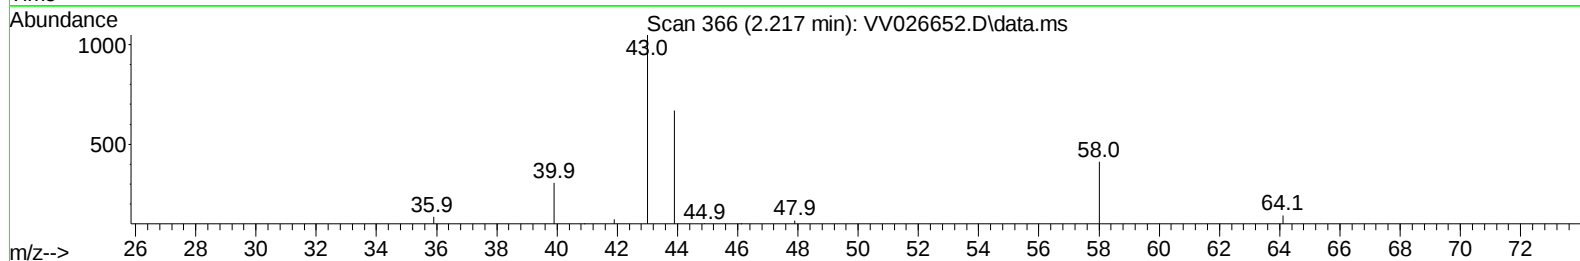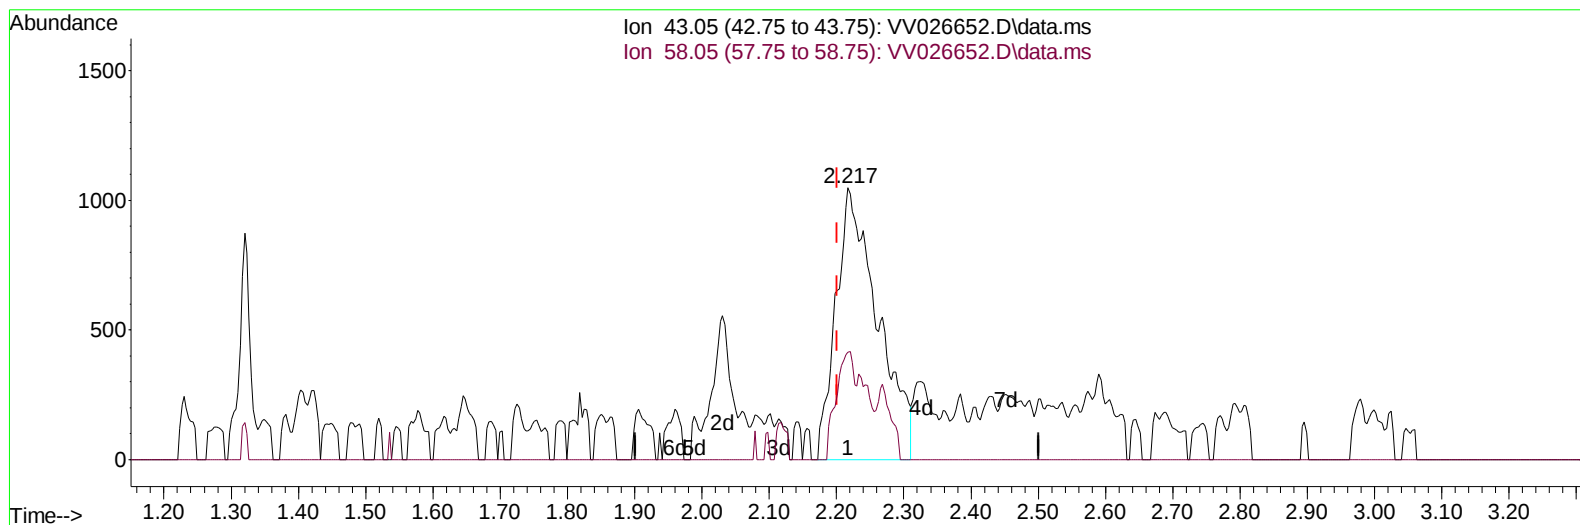

TIC: VV026652.D\data.ms

(13) Acetone (T)

2.217min (+ 0.016) 4.79 ug/L m

response 4505

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	37.50	18.00
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070522\
 Data File : VV026652.D
 Acq On : 05 Jul 2022 18:46
 Operator : SY/MD
 Sample : N3553-12
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AN1

Manual IntegrationsAPPROVED

Quant Time: Jul 06 00:30:23 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Jul 06 00:22:14 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 07/06/2022
 Supervised By :Mahesh Dadoda 07/06/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.625	114	185506	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	179561	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	76168	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.320	65	68329	4.580	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130	Recovery	=	91.600%	
7) Chloroethane-d5	1.581	69	57825	4.825	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130	Recovery	=	96.400%	
11) 1,1-Dichloroethene-d2	2.118	63	95322	3.596	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125	Recovery	=	72.000%	
20) 2-Butanone-d5	3.931	46	70362	47.439	ug/L	0.02
Spiked Amount 50.000	Range 40	- 130	Recovery	=	94.880%	
24) Chloroform-d	4.365	84	119025	4.881	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	97.600%	
26) 1,2-Dichloroethane-d4	5.043	65	45211	4.813	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	96.200%	
32) Benzene-d6	5.059	84	217239	4.212	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	84.200%	
36) 1,2-Dichloropropane-d6	6.076	67	64971	4.581	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140	Recovery	=	91.600%	
41) Toluene-d8	7.320	98	172948	3.729	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	74.600%	
43) trans-1,3-Dichloroprop...	7.629	79	14524	3.962	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130	Recovery	=	79.200%	
46) 2-Hexanone-d5	8.095	63	54668	39.150	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130	Recovery	=	78.300%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	42721	4.604	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120	Recovery	=	92.000%	
66) 1,2-Dichlorobenzene-d4	11.622	152	56901	4.514	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120	Recovery	=	90.200%	
Target Compounds						
					Qvalue	
13) Acetone	2.217	43	4505m	4.788	ug/L	
14) Carbon disulfide	2.307	76	14907	0.451	ug/L	96
16) Methylene chloride	2.519	84	5925	0.445	ug/L	93
25) Chloroform	4.388	83	118921	4.843	ug/L	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070522\
Data File : VV026652.D
Acq On : 05 Jul 2022 18:46
Operator : SY/MD
Sample : N3553-12
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 3

Instrument :
MSVOA_V
ClientSampleId :
C0AN1

Manual IntegrationsAPPROVED

Quant Time: Jul 06 00:30:23 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Jul 06 00:22:14 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 07/06/2022
Supervised By :Mahesh Dadoda 07/06/2022

