

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070522\
 Data File : VV026638.D
 Acq On : 05 Jul 2022 12:35
 Operator : SY/MD
 Sample : VV0705WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK388

Quant Time: Jul 06 00:23:20 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Jul 06 00:22:14 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.625	114	188987	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	184115	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	73042	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.320	65	77478	5.098	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	102.000%	
7) Chloroethane-d5	1.580	69	63660	5.214	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	104.200%	
11) 1,1-Dichloroethene-d2	2.117	63	107239	3.971	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	79.400%	
20) 2-Butanone-d5	3.924	46	58473	38.697	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	77.400%	
24) Chloroform-d	4.362	84	120546	4.852	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	97.000%	
26) 1,2-Dichloroethane-d4	5.043	65	48316	5.049	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	101.000%	
32) Benzene-d6	5.059	84	238718	4.514	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	90.200%	
36) 1,2-Dichloropropane-d6	6.075	67	70580	4.853	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	97.000%	
41) Toluene-d8	7.320	98	192754	4.053	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	81.000%	
43) trans-1,3-Dichloroprop...	7.628	79	17518	4.660	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	93.200%	
46) 2-Hexanone-d5	8.095	63	59339	41.444	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	82.880%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	45931	4.828	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	96.600%	
66) 1,2-Dichlorobenzene-d4	11.622	152	60906	5.039	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	100.800%	
Target Compounds						Qvalue
16) Methylene chloride	2.523	84	5747	0.424	ug/L	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070522\
Data File : VV026638.D
Acq On : 05 Jul 2022 12:35
Operator : SY/MD
Sample : VV0705WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK388


Quant Time: Jul 06 00:23:20 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Jul 06 00:22:14 2022
Response via : Initial Calibration

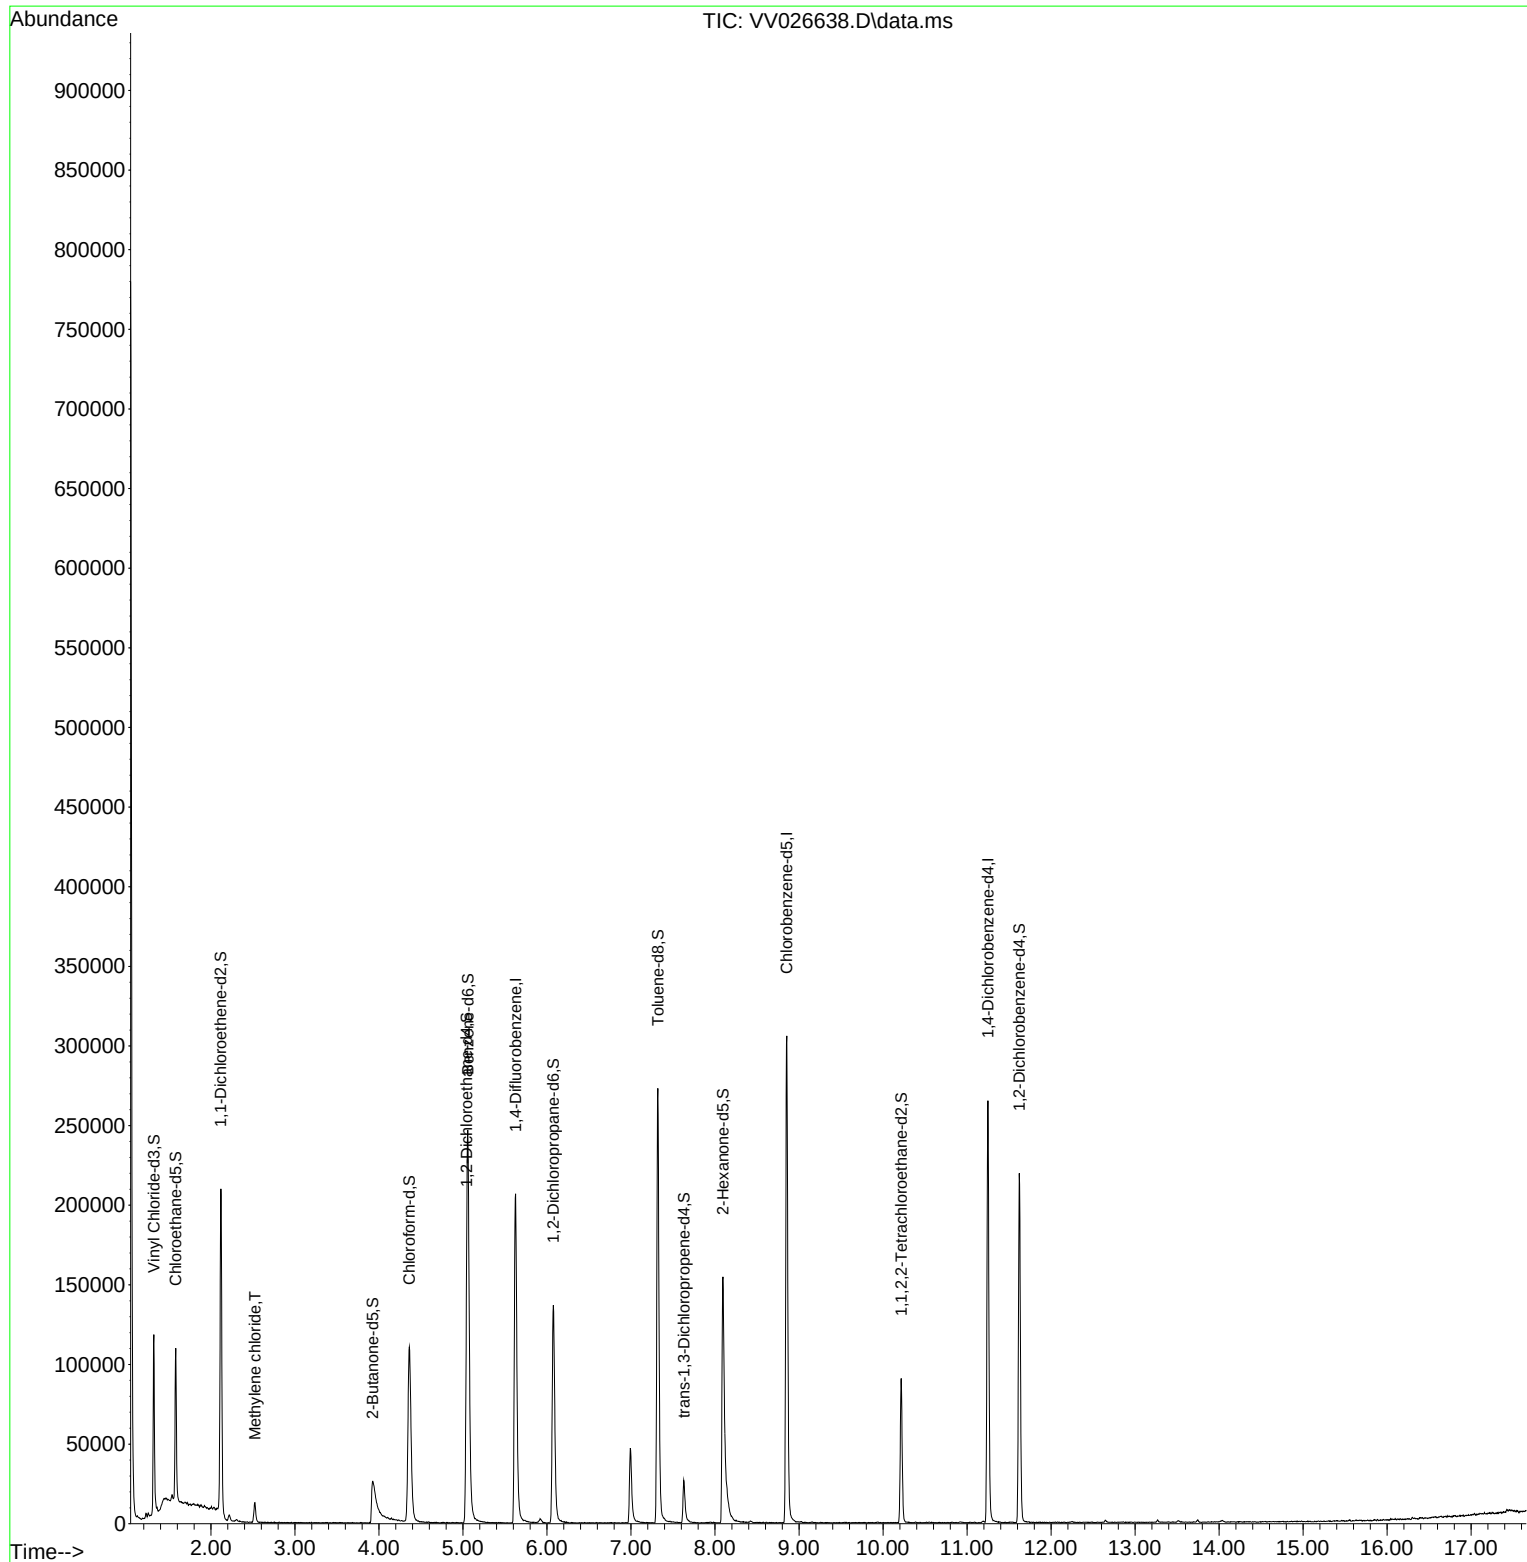

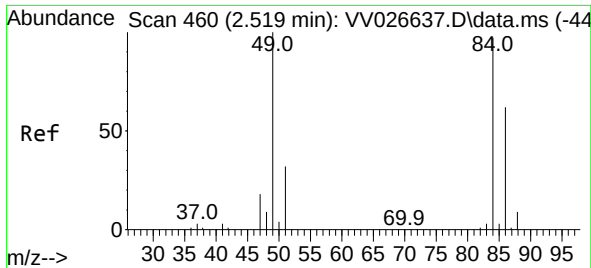

#16
Methylene chloride
Concen: 0.424 ug/L
RT: 2.523 min Scan# 4
Delta R.T. 0.003 min
Lab File: VV026638.D
Acq: 05 Jul 2022 12:35

Instrument :
MSVOA_V
ClientSampleId :
VBLK388

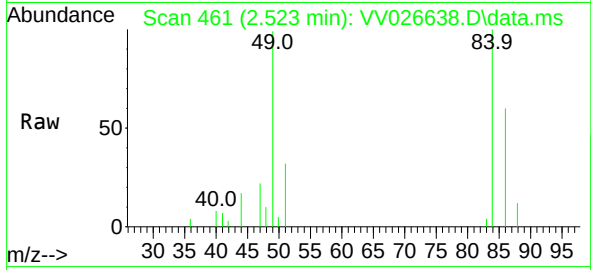

Tgt Ion: 84 Resp: 5747

Ion	Ratio	Lower	Upper
84	100		
86	60.2	46.0	85.4
49	99.0	77.7	144.3

