

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW070522\
 Data File : VW026646.D
 Acq On : 05 Jul 2022 15:55
 Operator : SY/MD
 Sample : N3506-06
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK002

Quant Time: Jul 06 00:25:19 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Jul 06 00:22:14 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.622	114	180378	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	177677	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	72418	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.314	65	74076	5.107	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	102.200%	
7) Chloroethane-d5	1.574	69	62459	5.360	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	107.200%	
11) 1,1-Dichloroethene-d2	2.111	63	103659	4.021	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	80.400%	
20) 2-Butanone-d5	3.921	46	78308	54.297	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	108.600%	
24) Chloroform-d	4.359	84	119182	5.026	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	100.600%	
26) 1,2-Dichloroethane-d4	5.040	65	47913	5.246	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	105.000%	
32) Benzene-d6	5.056	84	232521	4.556	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	91.200%	
36) 1,2-Dichloropropane-d6	6.075	67	69926	4.983	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	99.600%	
41) Toluene-d8	7.317	98	184795	4.027	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	80.600%	
43) trans-1,3-Dichloroprop...	7.628	79	16330	4.502	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	90.000%	
46) 2-Hexanone-d5	8.095	63	57687	41.750	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	83.500%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	45279	4.932	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	98.600%	
66) 1,2-Dichlorobenzene-d4	11.625	152	61062	5.095	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	102.000%	
Target Compounds						Qvalue
16) Methylene chloride	2.513	84	4065	0.314	ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070522\
Data File : VV026646.D
Acq On : 05 Jul 2022 15:55
Operator : SY/MD
Sample : N3506-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK002


Quant Time: Jul 06 00:25:19 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Jul 06 00:22:14 2022
Response via : Initial Calibration

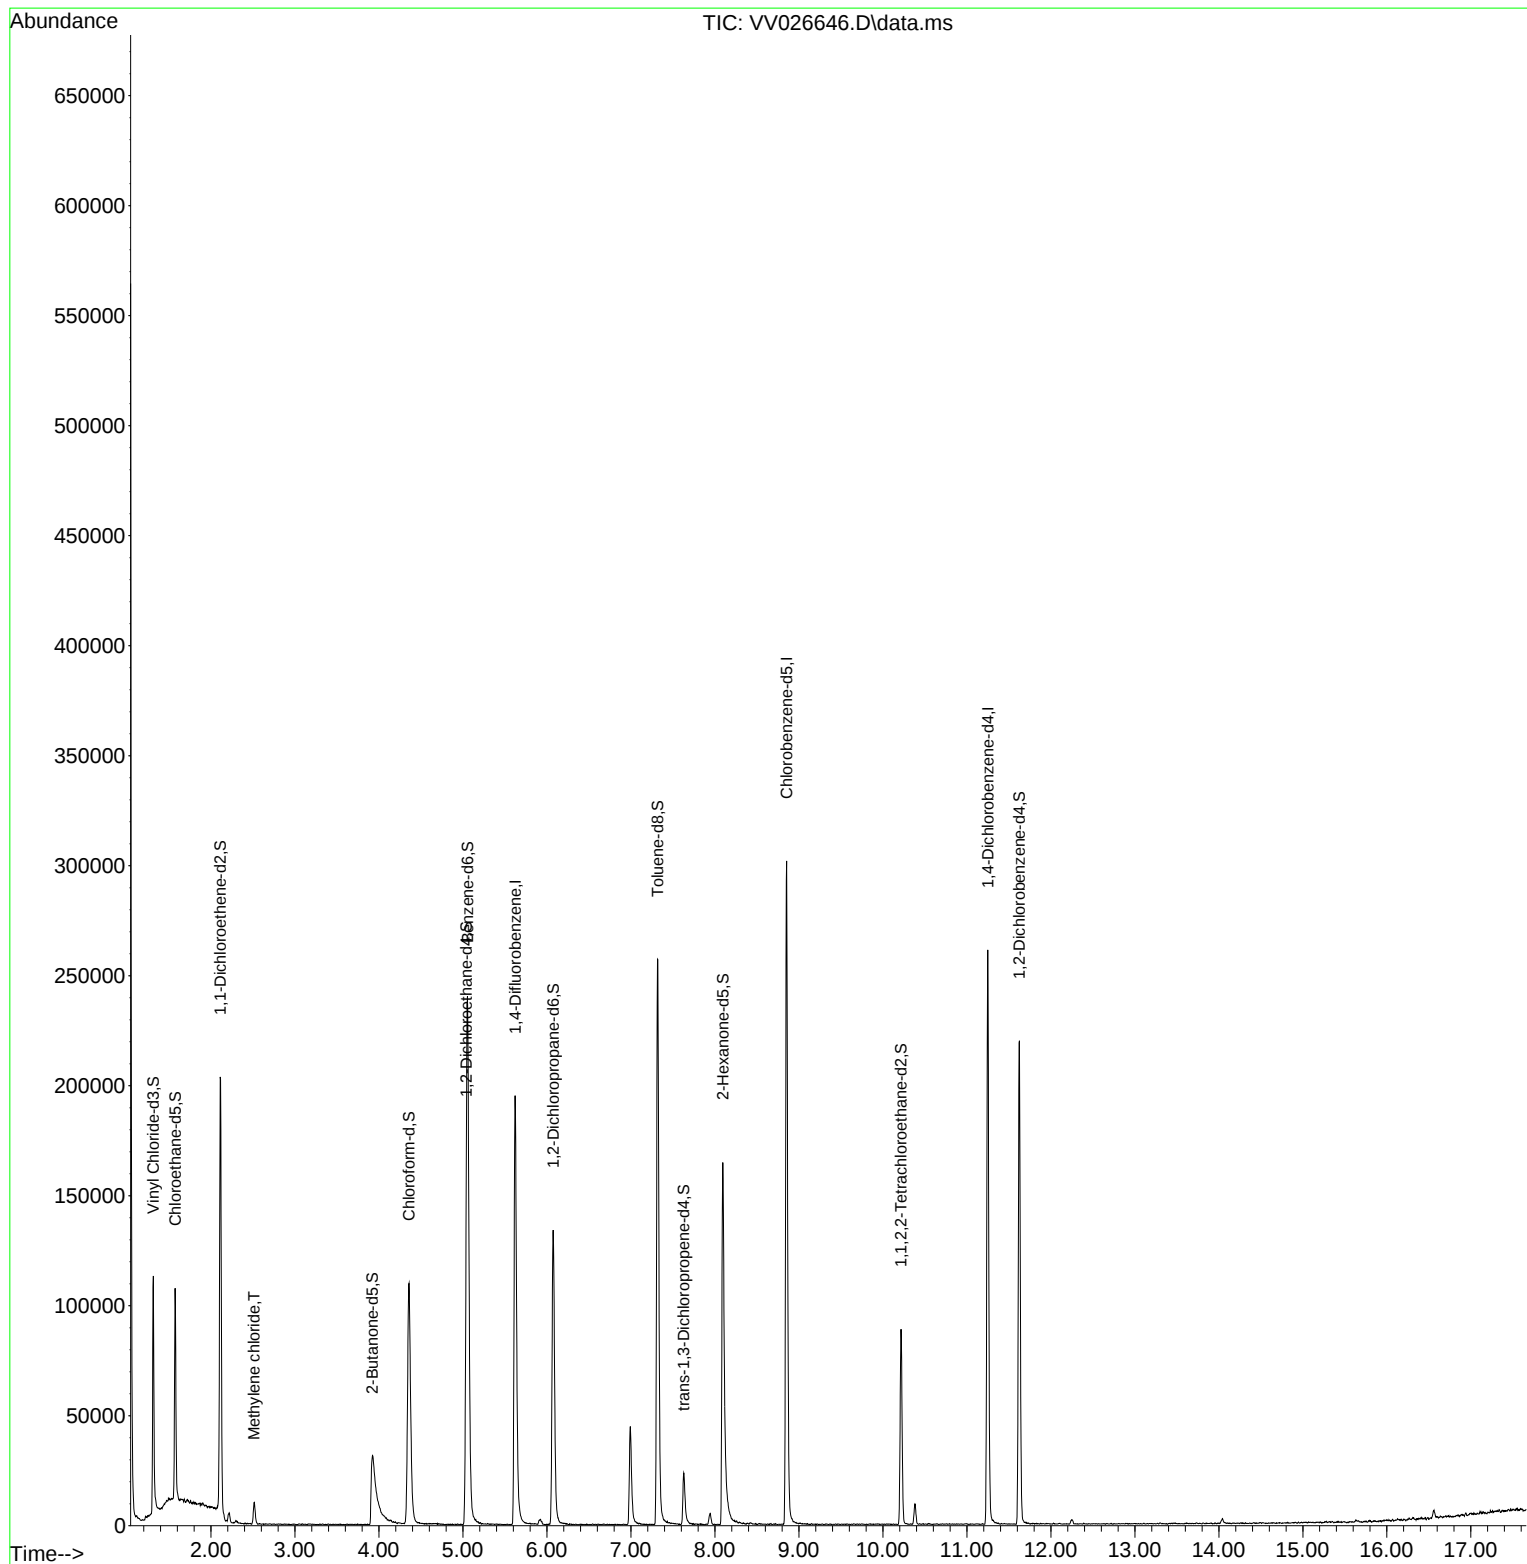

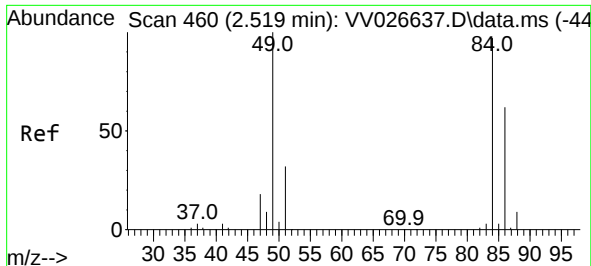

#16
Methylene chloride
Concen: 0.314 ug/L
RT: 2.513 min Scan# 4
Delta R.T. -0.006 min
Lab File: VV026646.D
Acq: 05 Jul 2022 15:55

Instrument :
MSVOA_V
ClientSampleId :
VHBLK002

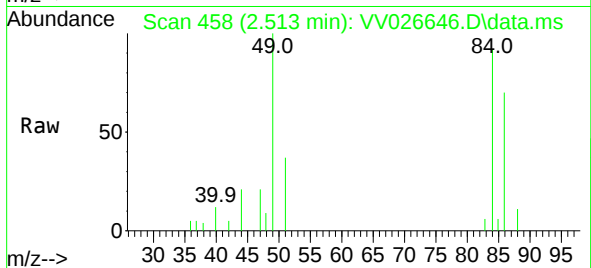

Tgt Ion: 84 Resp: 4065

Ion	Ratio	Lower	Upper
84	100		
86	75.5	46.0	85.4
49	108.6	77.7	144.3

