

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070522\
 Data File : VV026642.D
 Acq On : 05 Jul 2022 14:19
 Operator : SY/MD
 Sample : N3506-08
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AM4

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV026642.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.320	72	87	103	rBV	79795	105233	18.45%	2.172%
2	1.581	161	168	180	rVB	80571	91747	16.09%	1.894%
3	2.117	326	335	353	rVB	150824	220381	38.65%	4.549%
4	2.301	387	392	402	rVB2	3695	6037	1.06%	0.125%
5	3.921	886	896	936	rBV	41554	183883	32.25%	3.796%
6	4.365	1016	1034	1064	rBV3	127995	391893	68.72%	8.090%
7	5.056	1234	1249	1275	rBV2	230043	570254	100.00%	11.772%
8	5.625	1414	1426	1451	rBV	206224	420946	73.82%	8.690%
9	6.076	1552	1566	1590	rBV	142365	291644	51.14%	6.020%
10	6.584	1713	1724	1737	rBV4	5852	13142	2.30%	0.271%
11	6.992	1841	1851	1880	rBV	46189	90469	15.86%	1.868%
12	7.320	1942	1953	1970	rBV	237948	417945	73.29%	8.628%
13	7.400	1972	1978	1995	rVB2	7428	15344	2.69%	0.317%
14	7.629	2040	2049	2069	rBV	26658	48895	8.57%	1.009%
15	7.944	2137	2147	2156	rVB4	5240	8527	1.50%	0.176%
16	8.095	2182	2194	2225	rBV2	220532	468404	82.14%	9.669%
17	8.854	2419	2430	2448	rBV	310165	509984	89.43%	10.528%
18	10.217	2843	2854	2877	rBV	109606	172980	30.33%	3.571%
19	10.384	2896	2906	2923	rVB2	12982	19883	3.49%	0.410%
20	11.249	3163	3175	3199	rBV	273790	428150	75.08%	8.838%
21	11.622	3279	3291	3314	rBV	235614	368508	64.62%	7.607%




Sum of corrected areas: 4844249

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070522\
Data File : VV026642.D
Acq On : 05 Jul 2022 14:19
Operator : SY/MD
Sample : N3506-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AM4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

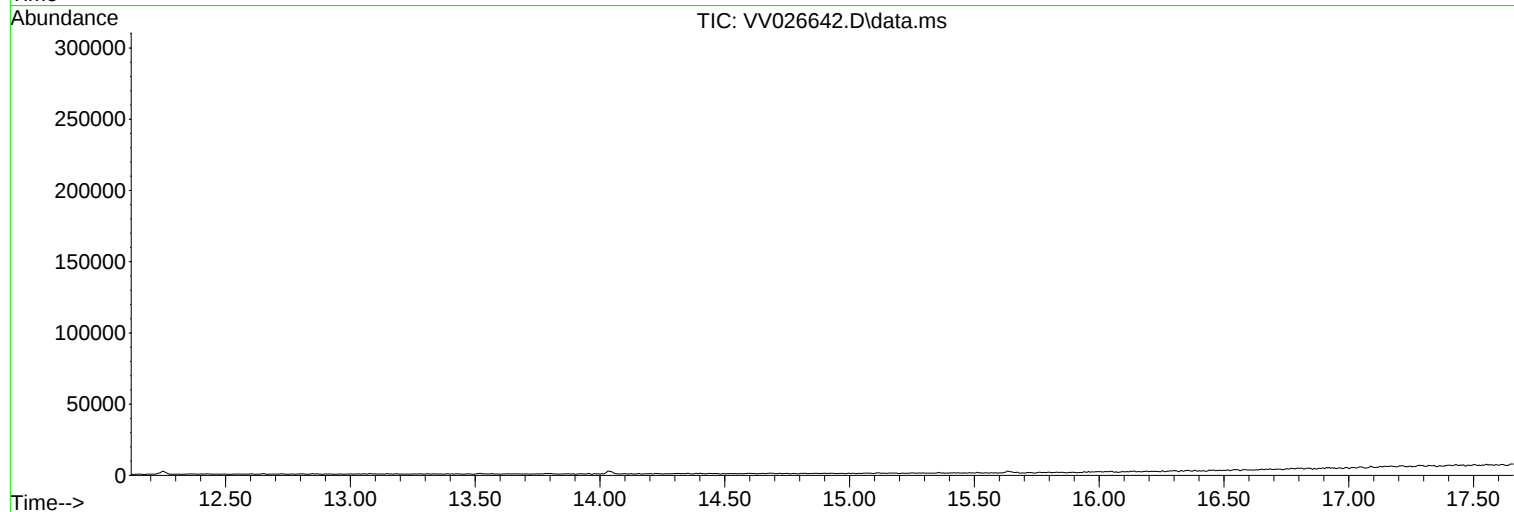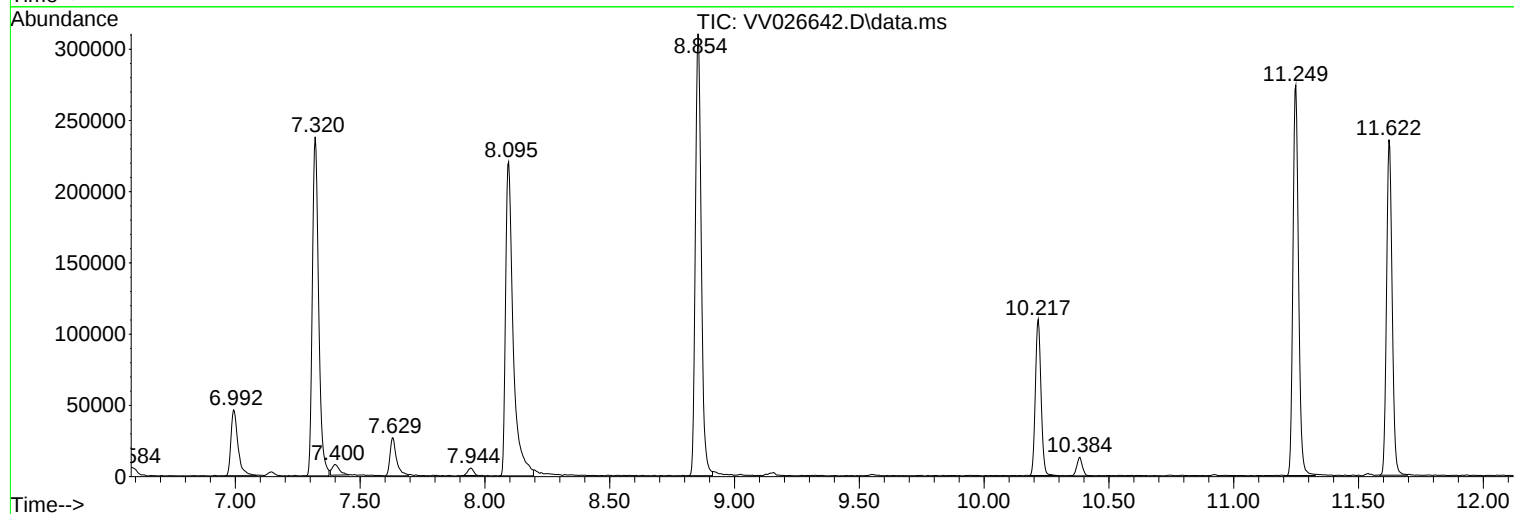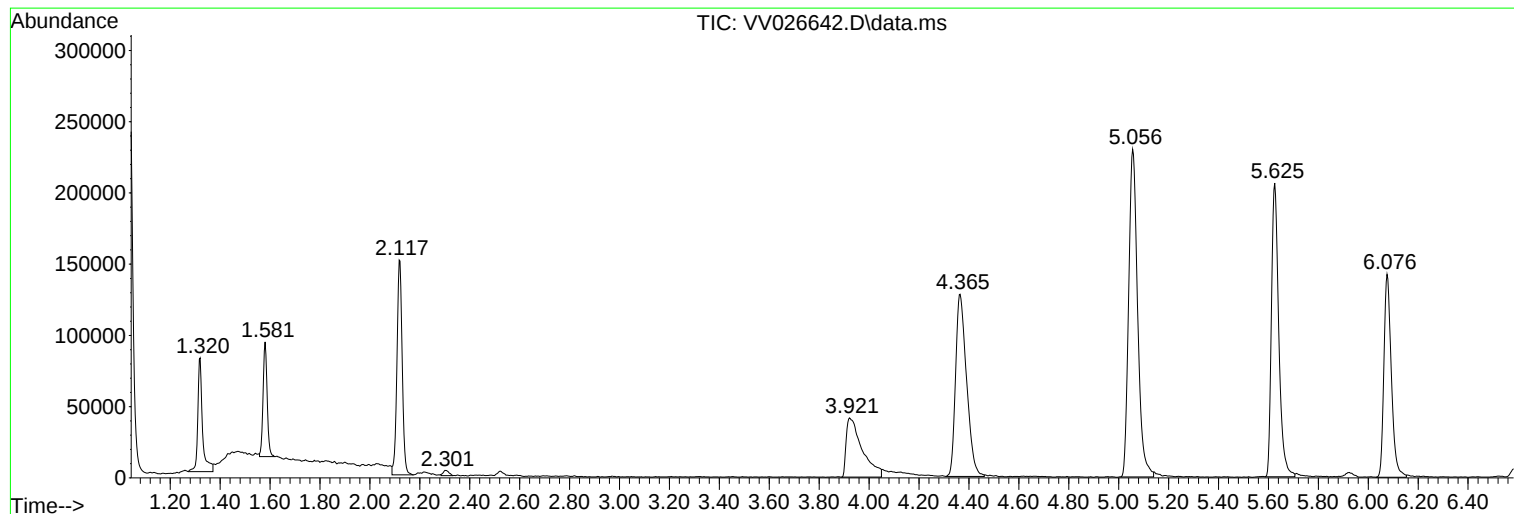

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070522\
Data File : VV026642.D
Acq On : 05 Jul 2022 14:19
Operator : SY/MD
Sample : N3506-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AM4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070522\
Data File : VV026642.D
Acq On : 05 Jul 2022 14:19
Operator : SY/MD
Sample : N3506-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AM4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
