

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070522\
 Data File : VV026646.D
 Acq On : 05 Jul 2022 15:55
 Operator : SY/MD
 Sample : N3506-06
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK002

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV026646.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.314	78	85	102	rBV	108020	123621	21.09%	2.696%
2	1.574	159	166	181	rVB	96453	111465	19.01%	2.431%
3	2.111	324	333	353	rVB	201859	299443	51.08%	6.529%
4	2.217	358	366	377	rVB4	4618	7730	1.32%	0.169%
5	2.516	449	459	472	rBV3	9987	16263	2.77%	0.355%
6	3.924	884	897	934	rBV2	31384	134488	22.94%	2.933%
7	4.359	1015	1032	1063	rBV	109210	279377	47.66%	6.092%
8	5.053	1232	1248	1277	rBV2	239999	586205	100.00%	12.782%
9	5.622	1412	1425	1462	rBV	194891	402901	68.73%	8.785%
10	6.075	1553	1566	1593	rBV2	133712	278564	47.52%	6.074%
11	6.992	1838	1851	1870	rBV	44586	84697	14.45%	1.847%
12	7.317	1941	1952	1975	rBV	256901	460545	78.56%	10.042%
13	7.628	2039	2049	2068	rBV2	23455	45031	7.68%	0.982%
14	7.944	2136	2147	2159	rVB4	5115	8974	1.53%	0.196%
15	8.095	2184	2194	2227	rBV2	164536	342528	58.43%	7.469%
16	8.854	2419	2430	2455	rBV	301532	493329	84.16%	10.757%
17	10.217	2842	2854	2870	rBV	88696	143346	24.45%	3.126%
18	10.381	2896	2905	2919	rBV2	9288	14658	2.50%	0.320%
19	11.249	3163	3175	3192	rBV	261104	402474	68.66%	8.776%
20	11.625	3279	3292	3310	rBV	219785	350399	59.77%	7.641%




Sum of corrected areas: 4586038

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070522\
Data File : VV026646.D
Acq On : 05 Jul 2022 15:55
Operator : SY/MD
Sample : N3506-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

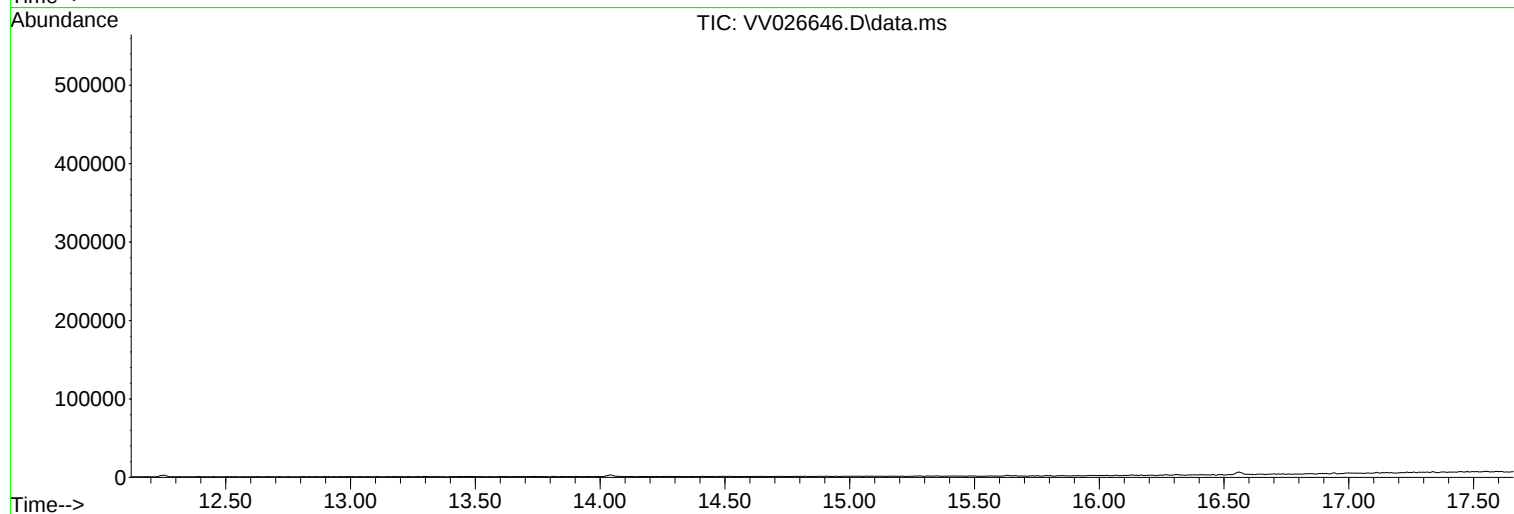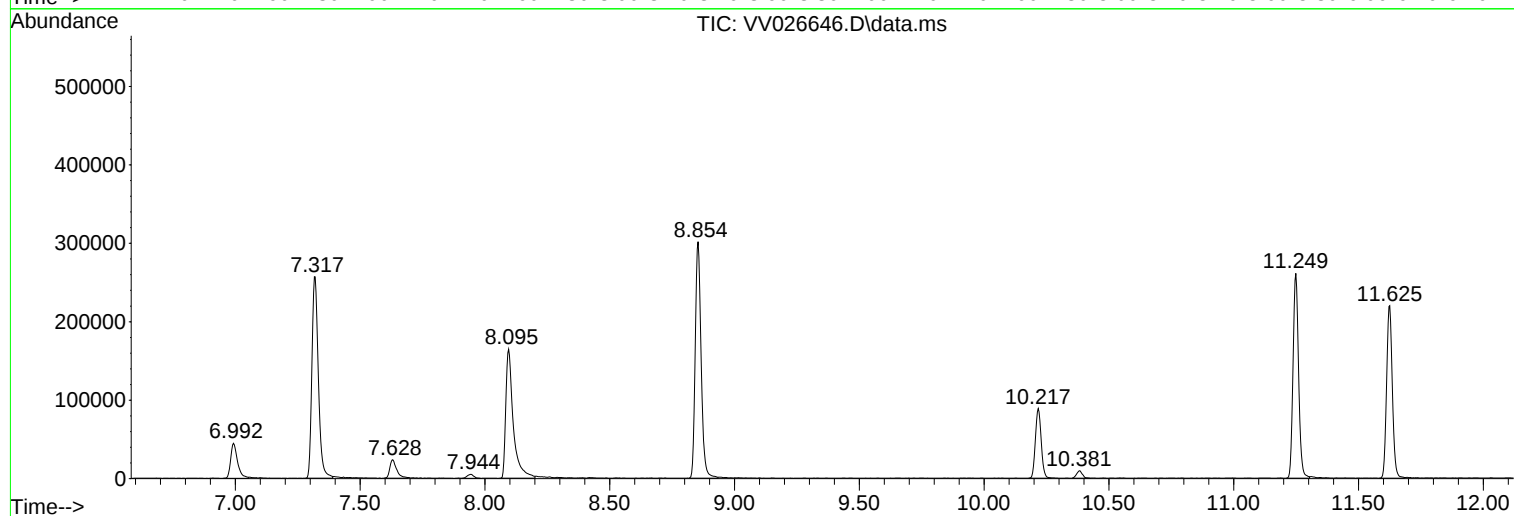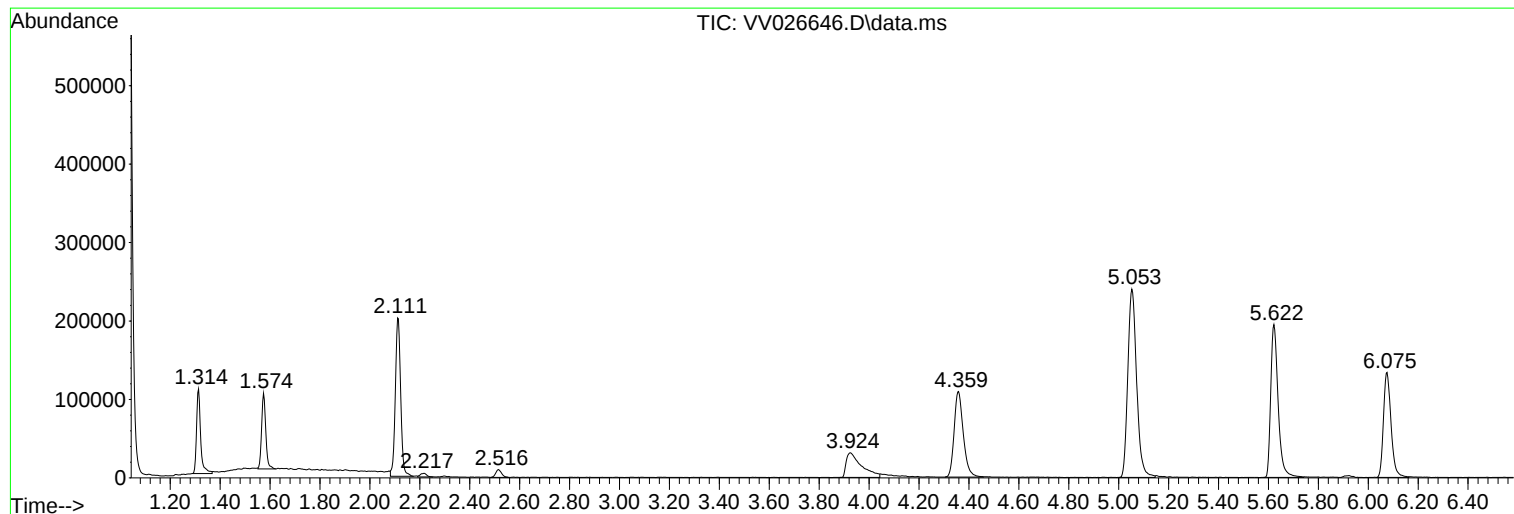

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070522\
Data File : VV026646.D
Acq On : 05 Jul 2022 15:55
Operator : SY/MD
Sample : N3506-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070522\
Data File : VV026646.D
Acq On : 05 Jul 2022 15:55
Operator : SY/MD
Sample : N3506-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
