

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070522\
 Data File : VV026647.D
 Acq On : 05 Jul 2022 16:44
 Operator : SY/MD
 Sample : N3555-02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AA9

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV026647.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.111	17	22	30	rVB	19866	18106	3.26%	0.386%
2	1.259	54	68	69	rBV9	5244	7658	1.38%	0.163%
3	1.317	80	86	107	rVB	73087	83458	15.04%	1.780%
4	1.577	161	167	179	rVB	72406	84534	15.23%	1.803%
5	2.118	325	335	355	rVB	144545	218798	39.42%	4.666%
6	2.520	450	460	479	rVB2	21304	35360	6.37%	0.754%
7	3.925	887	897	927	rBV2	42045	169595	30.56%	3.617%
8	4.362	1016	1033	1068	rBV2	111604	282729	50.94%	6.030%
9	5.056	1234	1249	1286	rBV2	224179	555029	100.00%	11.837%
10	5.626	1412	1426	1445	rBV	206181	419460	75.57%	8.946%
11	5.925	1509	1519	1529	rVB10	2777	5870	1.06%	0.125%
12	6.076	1553	1566	1589	rBV	135694	279076	50.28%	5.952%
13	6.992	1841	1851	1873	rBV	45667	88492	15.94%	1.887%
14	7.320	1942	1953	1975	rBV	228945	406497	73.24%	8.670%
15	7.629	2040	2049	2071	rBV2	25307	46728	8.42%	0.997%
16	8.095	2183	2194	2235	rBV2	219424	460440	82.96%	9.820%
17	8.854	2418	2430	2458	rBV	313275	514074	92.62%	10.964%
18	10.217	2841	2854	2871	rBV	103708	164589	29.65%	3.510%
19	10.384	2895	2906	2917	rVB4	5793	9951	1.79%	0.212%
20	11.249	3164	3175	3194	rBV	276769	433984	78.19%	9.256%
21	11.625	3280	3292	3308	rBV	229973	364851	65.74%	7.781%
22	12.645	3602	3609	3618	rBV3	5964	7963	1.43%	0.170%
23	13.265	3795	3802	3815	rVB4	5731	8794	1.58%	0.188%
24	13.506	3867	3877	3889	rBV2	4903	8043	1.45%	0.172%
25	13.744	3944	3951	3960	rBV5	5630	8294	1.49%	0.177%
26	16.558	4818	4826	4833	rBV6	3741	6392	1.15%	0.136%




Sum of corrected areas: 4688765

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070522\
Data File : VV026647.D
Acq On : 05 Jul 2022 16:44
Operator : SY/MD
Sample : N3555-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AA9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

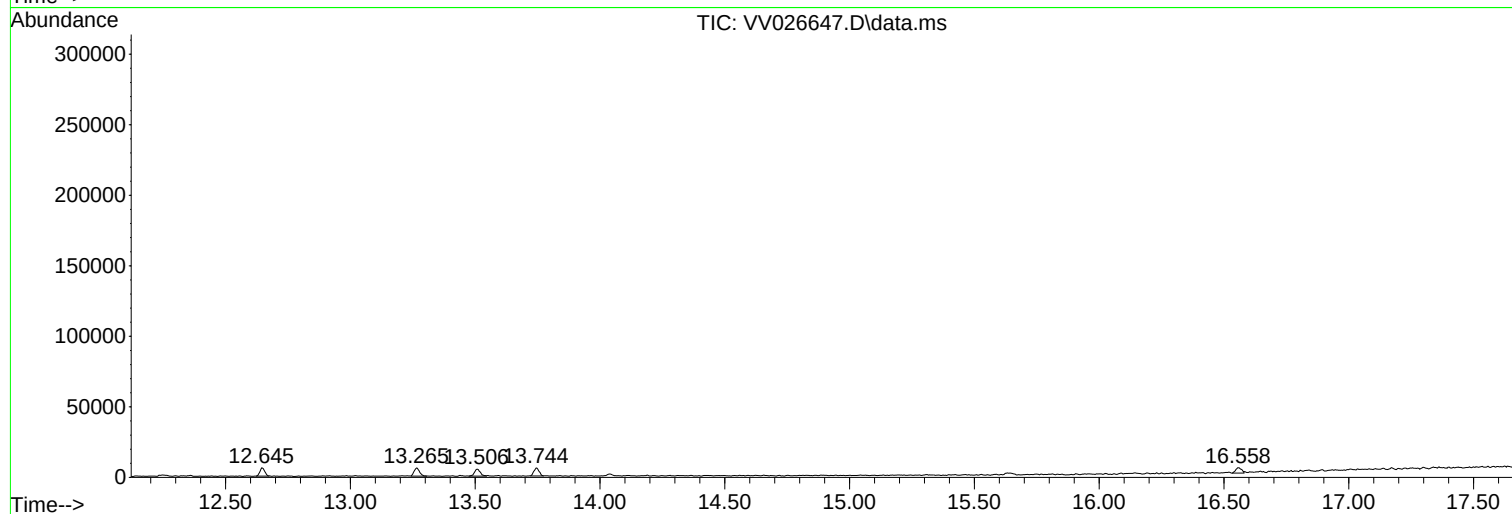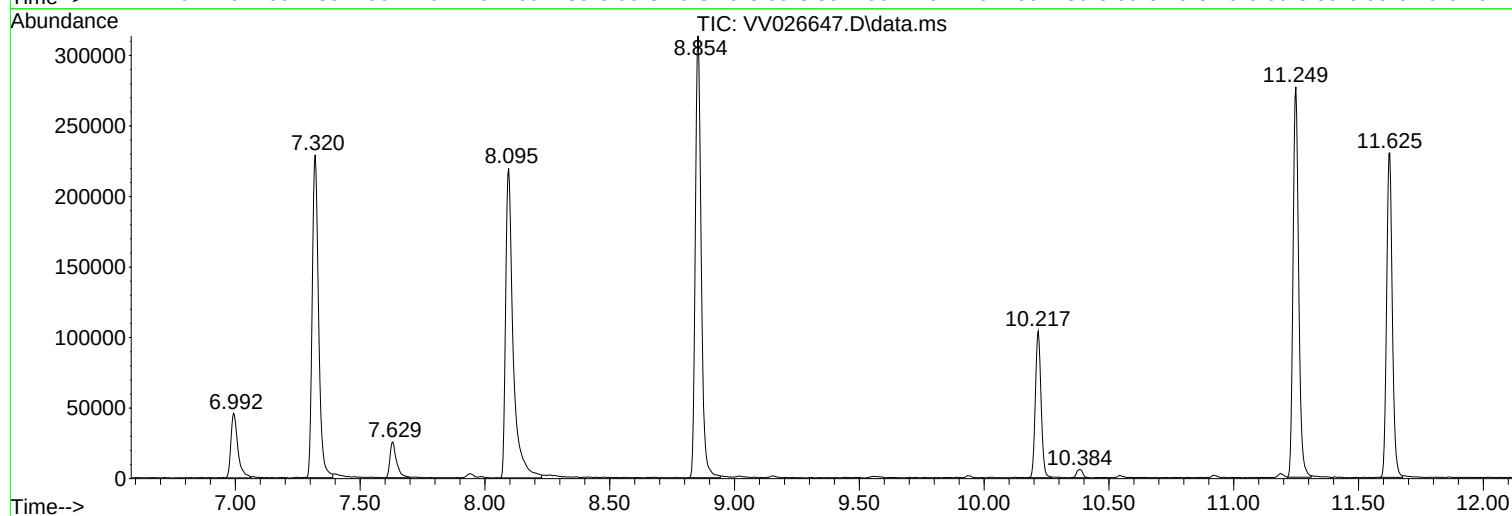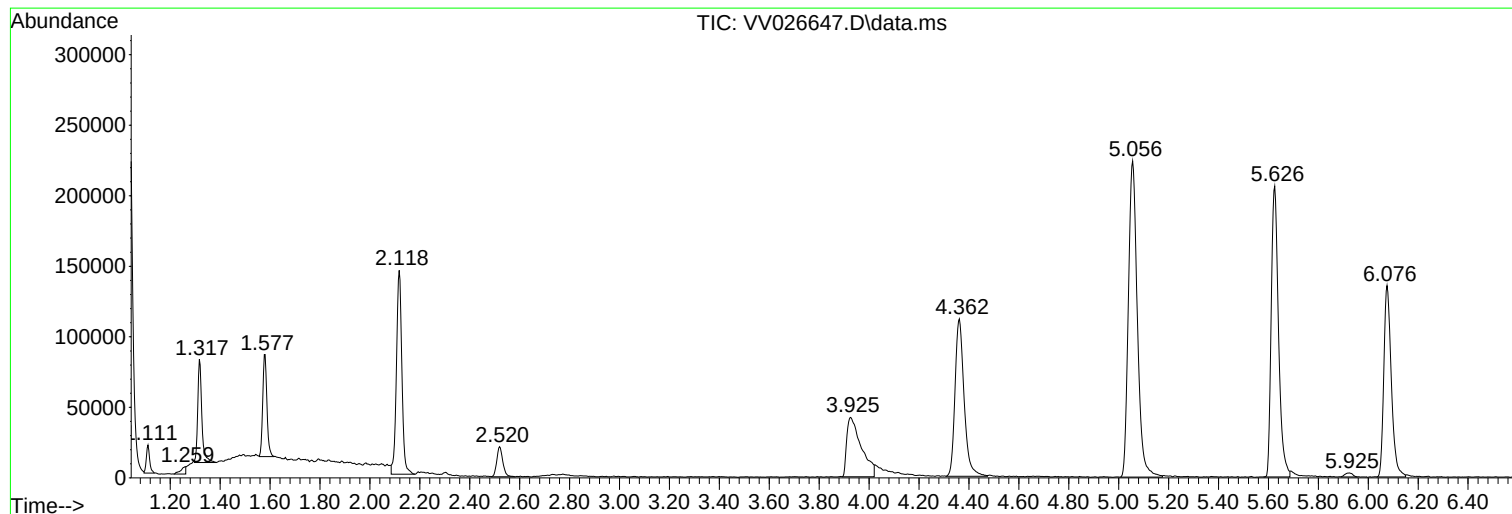

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070522\
Data File : VV026647.D
Acq On : 05 Jul 2022 16:44
Operator : SY/MD
Sample : N3555-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AA9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070522\
Data File : VV026647.D
Acq On : 05 Jul 2022 16:44
Operator : SY/MD
Sample : N3555-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AA9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
