

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070522\
 Data File : VV026648.D
 Acq On : 05 Jul 2022 17:08
 Operator : SY/MD
 Sample : N3555-03
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV026648.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.320	78	87	102	rBV	114619	131679	21.19%	2.699%
2	1.581	161	168	187	rVB	100297	121039	19.47%	2.481%
3	2.118	325	335	354	rVB	212640	314834	50.65%	6.453%
4	2.523	450	461	473	rBV2	11172	18500	2.98%	0.379%
5	3.931	889	899	948	rBV2	32622	152319	24.51%	3.122%
6	4.362	1017	1033	1060	rBV2	113261	289030	46.50%	5.924%
7	5.056	1231	1249	1288	rBV2	254099	621530	100.00%	12.740%
8	5.625	1412	1426	1452	rBV	208135	426259	68.58%	8.737%
9	6.076	1552	1566	1591	rBV	141726	293619	47.24%	6.018%
10	6.992	1842	1851	1877	rBV2	46672	90464	14.56%	1.854%
11	7.320	1942	1953	1975	rBV	281900	496064	79.81%	10.168%
12	7.632	2040	2050	2074	rBV2	26276	50104	8.06%	1.027%
13	7.940	2135	2146	2159	rBV4	6085	11232	1.81%	0.230%
14	8.095	2184	2194	2230	rBV2	175510	367624	59.15%	7.535%
15	8.854	2419	2430	2454	rBV	314254	518978	83.50%	10.638%
16	10.217	2843	2854	2872	rBV	95729	150314	24.18%	3.081%
17	10.384	2896	2906	2919	rVB2	10999	17597	2.83%	0.361%
18	11.249	3164	3175	3193	rBV	273270	431087	69.36%	8.836%
19	11.625	3280	3292	3315	rBV	229973	376345	60.55%	7.714%




Sum of corrected areas: 4878618

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070522\
Data File : VV026648.D
Acq On : 05 Jul 2022 17:08
Operator : SY/MD
Sample : N3555-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

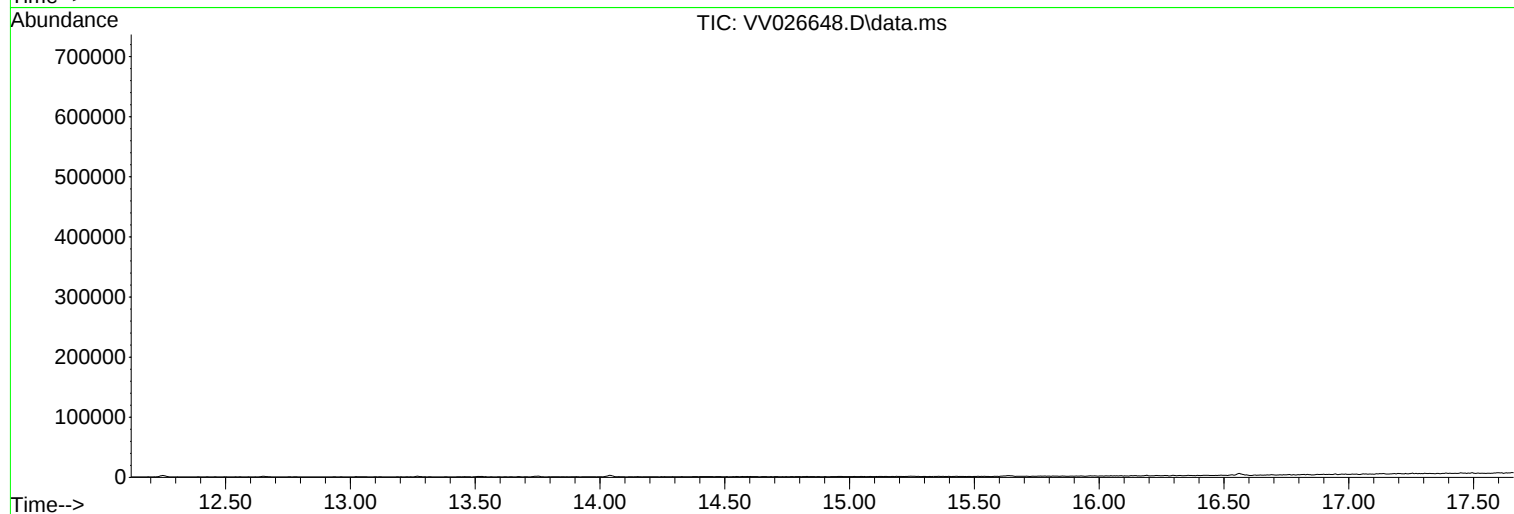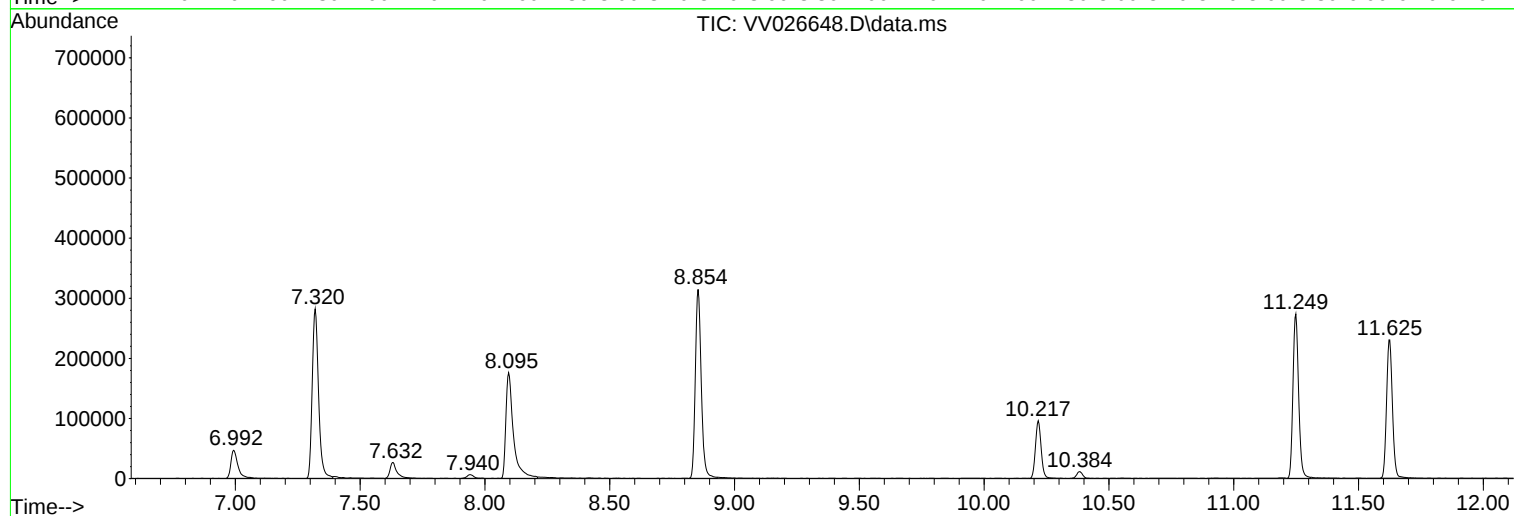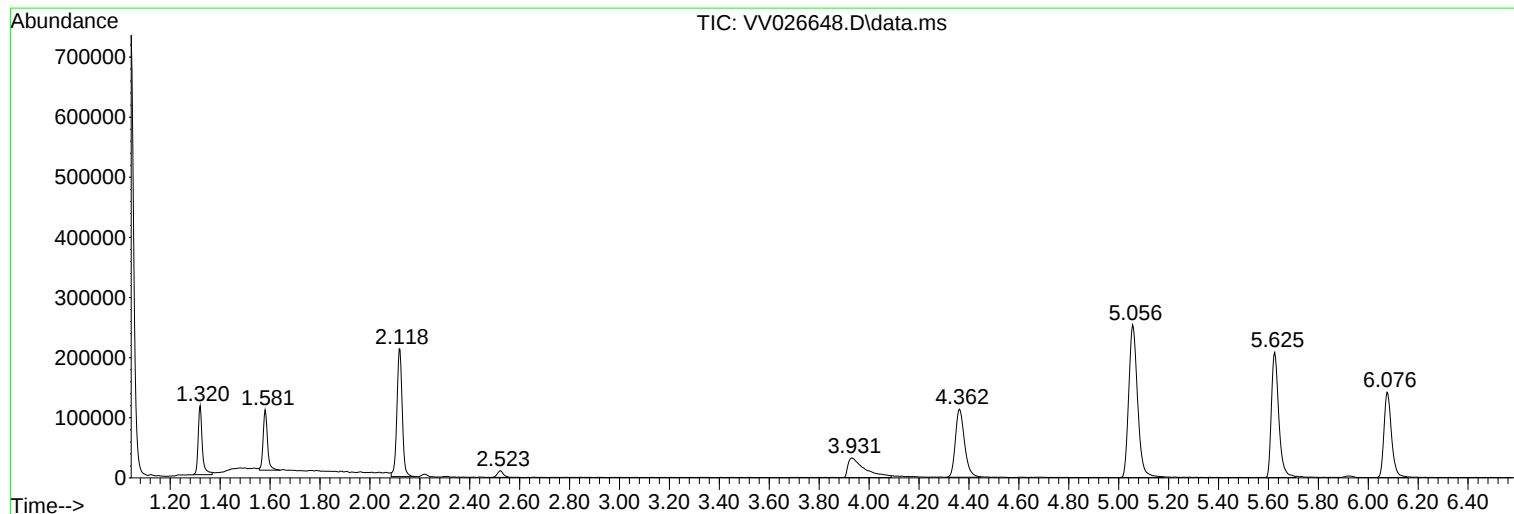

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070522\
Data File : VV026648.D
Acq On : 05 Jul 2022 17:08
Operator : SY/MD
Sample : N3555-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070522\
Data File : VV026648.D
Acq On : 05 Jul 2022 17:08
Operator : SY/MD
Sample : N3555-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc