

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070522\
 Data File : VV026649.D
 Acq On : 05 Jul 2022 17:33
 Operator : SY/MD
 Sample : N3553-04
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AM8

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV026649.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.288	60	77	78	rBV8	8310	17361	3.08%	0.360%
2	1.317	79	86	101	rVV	103574	122042	21.69%	2.533%
3	1.580	161	168	180	rVB	86665	100228	17.81%	2.080%
4	2.117	325	335	354	rVB	192945	283325	50.34%	5.881%
5	2.304	384	393	404	rVB	11478	16649	2.96%	0.346%
6	2.519	449	460	472	rBV3	12435	22434	3.99%	0.466%
7	2.587	472	481	490	rVB3	5583	9628	1.71%	0.200%
8	3.931	886	899	923	rBV3	33499	138374	24.59%	2.872%
9	4.375	1015	1037	1069	rBV3	155293	541346	96.19%	11.237%
10	5.056	1233	1249	1280	rBV2	229982	562771	100.00%	11.681%
11	5.625	1414	1426	1447	rBV	203201	415360	73.81%	8.621%
12	6.075	1553	1566	1594	rBV2	127972	266790	47.41%	5.538%
13	6.992	1840	1851	1870	rBV2	42835	81772	14.53%	1.697%
14	7.320	1942	1953	1973	rBV	250359	442348	78.60%	9.182%
15	7.628	2040	2049	2065	rBV3	22726	42257	7.51%	0.877%
16	8.095	2184	2194	2237	rBV2	161971	336507	59.79%	6.985%
17	8.853	2418	2430	2466	rBV	310315	509942	90.61%	10.585%
18	10.217	2842	2854	2869	rBV	87563	138696	24.65%	2.879%
19	10.381	2895	2905	2916	rBV3	8450	13126	2.33%	0.272%
20	11.249	3163	3175	3197	rBV	277820	426677	75.82%	8.856%
21	11.625	3280	3292	3307	rBV	206388	330109	58.66%	6.852%




Sum of corrected areas: 4817742

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070522\
Data File : VV026649.D
Acq On : 05 Jul 2022 17:33
Operator : SY/MD
Sample : N3553-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AM8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

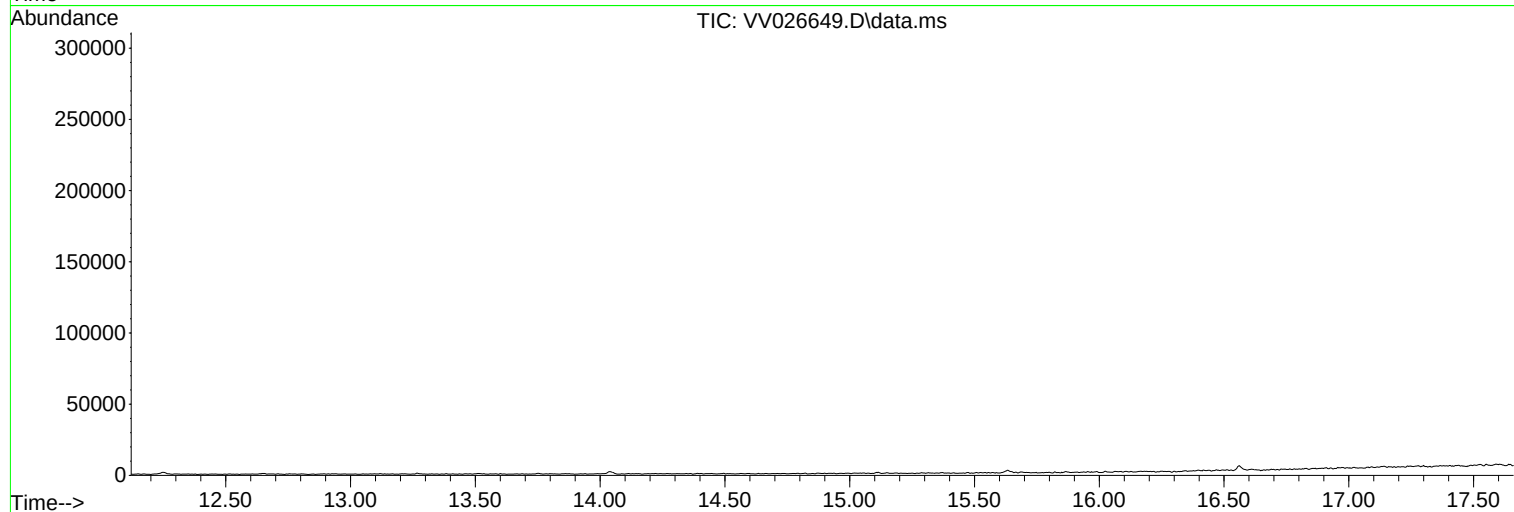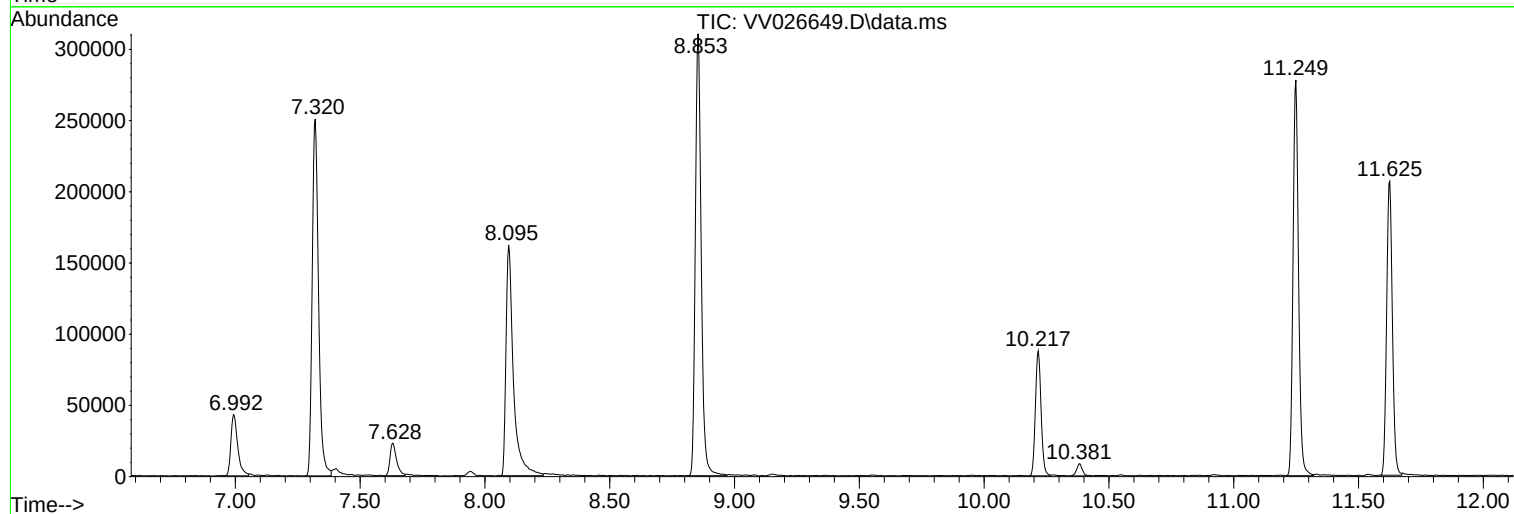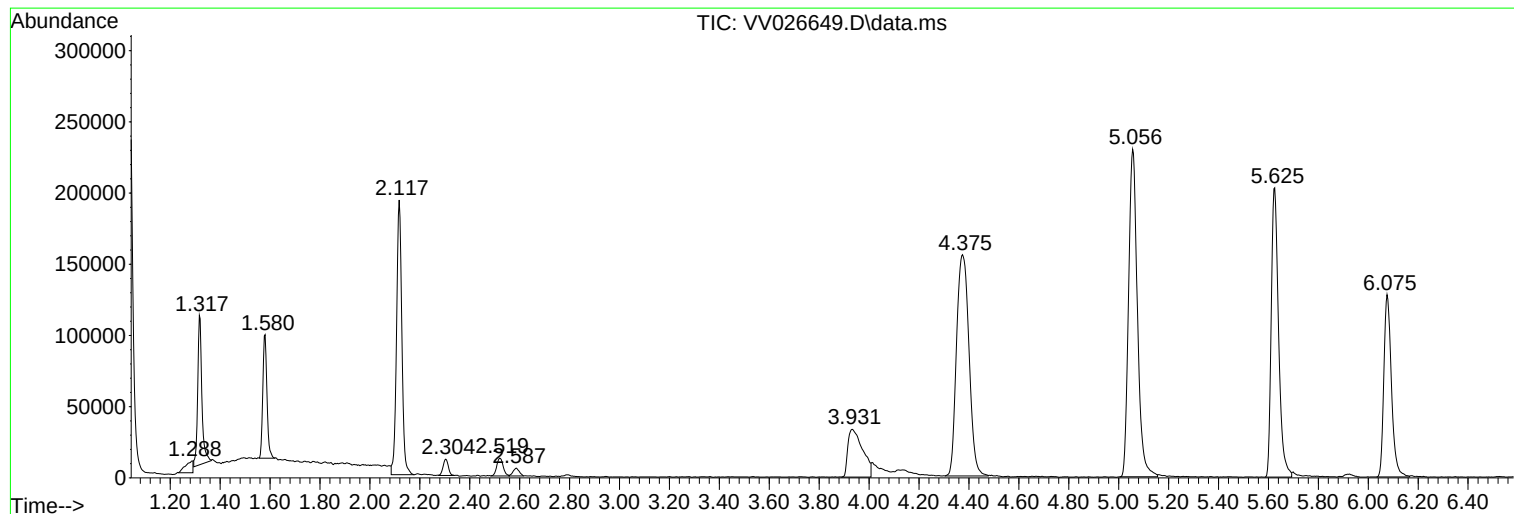

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070522\
Data File : VV026649.D
Acq On : 05 Jul 2022 17:33
Operator : SY/MD
Sample : N3553-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AM8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070522\
Data File : VV026649.D
Acq On : 05 Jul 2022 17:33
Operator : SY/MD
Sample : N3553-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AM8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc