

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070522\
 Data File : VV026653.D
 Acq On : 05 Jul 2022 19:10
 Operator : SY/MD
 Sample : N3553-06
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV026653.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.320	80	87	100	rBV	109684	117214	20.35%	2.568%
2	1.580	161	168	183	rVB	93366	109761	19.06%	2.404%
3	2.121	326	336	354	rVB	198483	290132	50.37%	6.355%
4	2.523	448	461	474	rBV2	13011	21238	3.69%	0.465%
5	3.940	889	902	939	rBV2	29275	140060	24.32%	3.068%
6	4.362	1015	1033	1065	rBV2	107584	272453	47.31%	5.968%
7	5.056	1232	1249	1279	rBV2	236388	575949	100.00%	12.616%
8	5.625	1413	1426	1452	rBV	197043	406751	70.62%	8.910%
9	6.075	1553	1566	1591	rBV	131466	274990	47.75%	6.024%
10	6.992	1839	1851	1873	rBV2	41540	81249	14.11%	1.780%
11	7.320	1940	1953	1977	rBV	257146	454763	78.96%	9.962%
12	7.632	2040	2050	2069	rBV3	22827	42734	7.42%	0.936%
13	7.937	2136	2145	2161	rBV3	6700	12055	2.09%	0.264%
14	8.095	2184	2194	2225	rBV2	160784	339085	58.87%	7.428%
15	8.853	2419	2430	2461	rBV	304999	502883	87.31%	11.016%
16	10.217	2843	2854	2868	rBV	87427	137272	23.83%	3.007%
17	10.384	2892	2906	2920	rBV2	12476	20230	3.51%	0.443%
18	11.249	3162	3175	3198	rBV	264147	412662	71.65%	9.039%
19	11.622	3279	3291	3311	rBV2	215005	343091	59.57%	7.515%
20	16.557	4819	4826	4835	rBV2	7412	10571	1.84%	0.232%




Sum of corrected areas: 4565143

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070522\
Data File : VV026653.D
Acq On : 05 Jul 2022 19:10
Operator : SY/MD
Sample : N3553-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

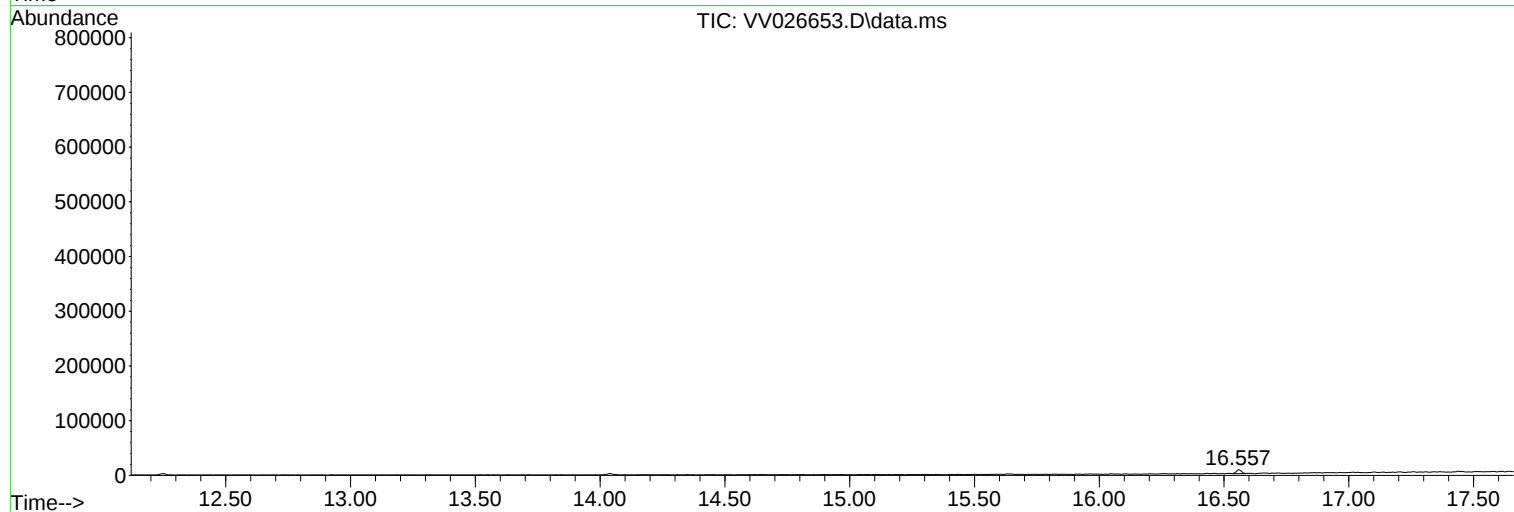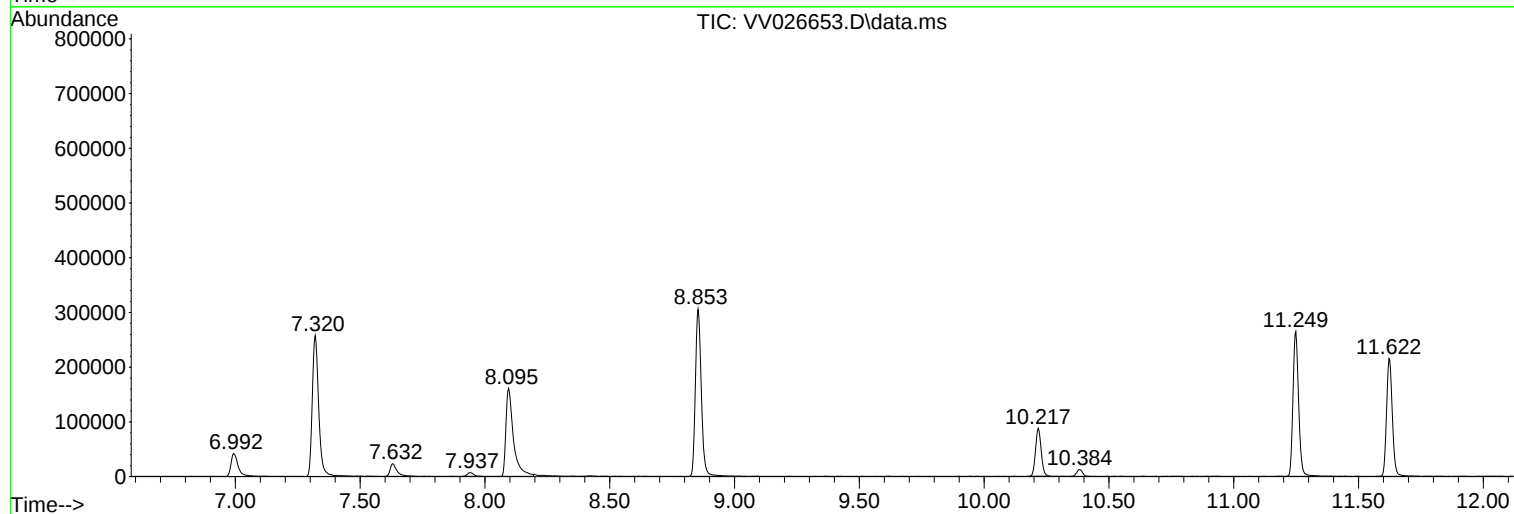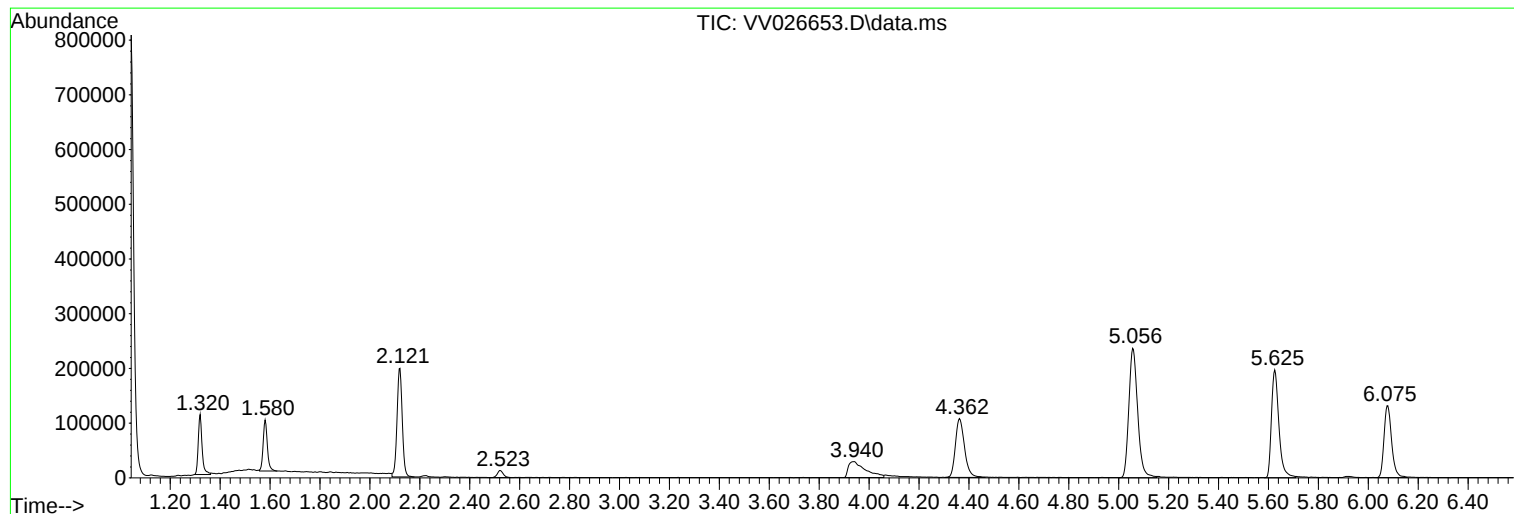

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070522\
Data File : VV026653.D
Acq On : 05 Jul 2022 19:10
Operator : SY/MD
Sample : N3553-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070522\
Data File : VV026653.D
Acq On : 05 Jul 2022 19:10
Operator : SY/MD
Sample : N3553-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc