
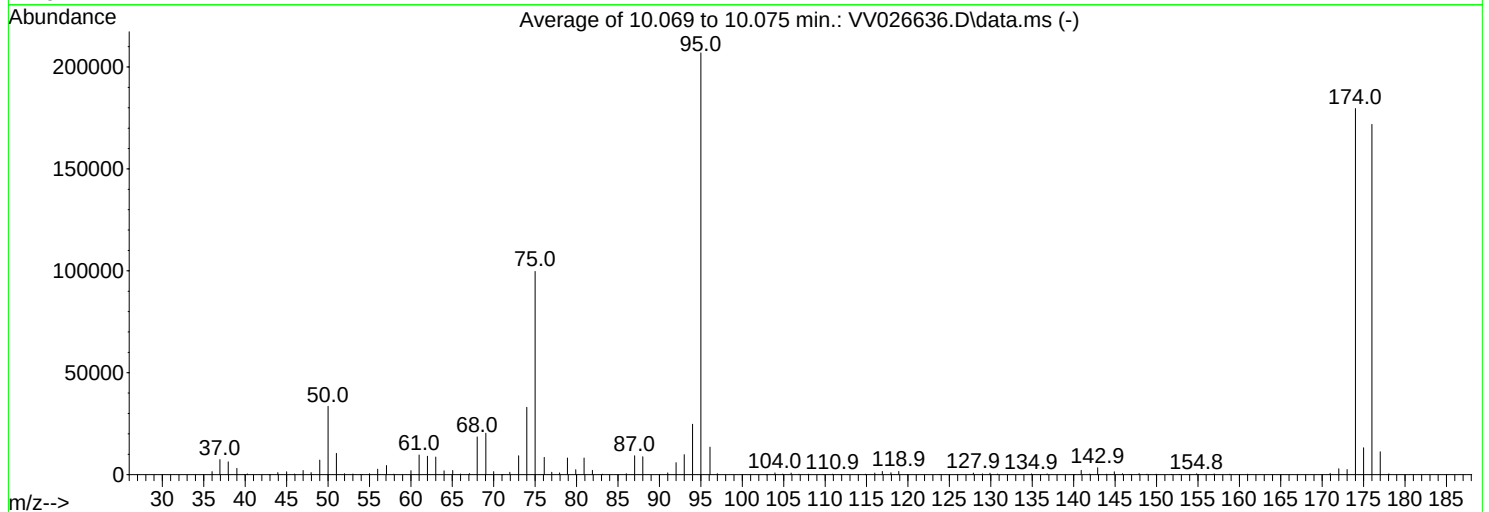


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070522\
 Data File : VV026636.D
 Acq On : 05 Jul 2022 08:58
 Operator : SY/MD
 Sample : BFB338
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB338

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Wed Jul 06 00:22:14 2022

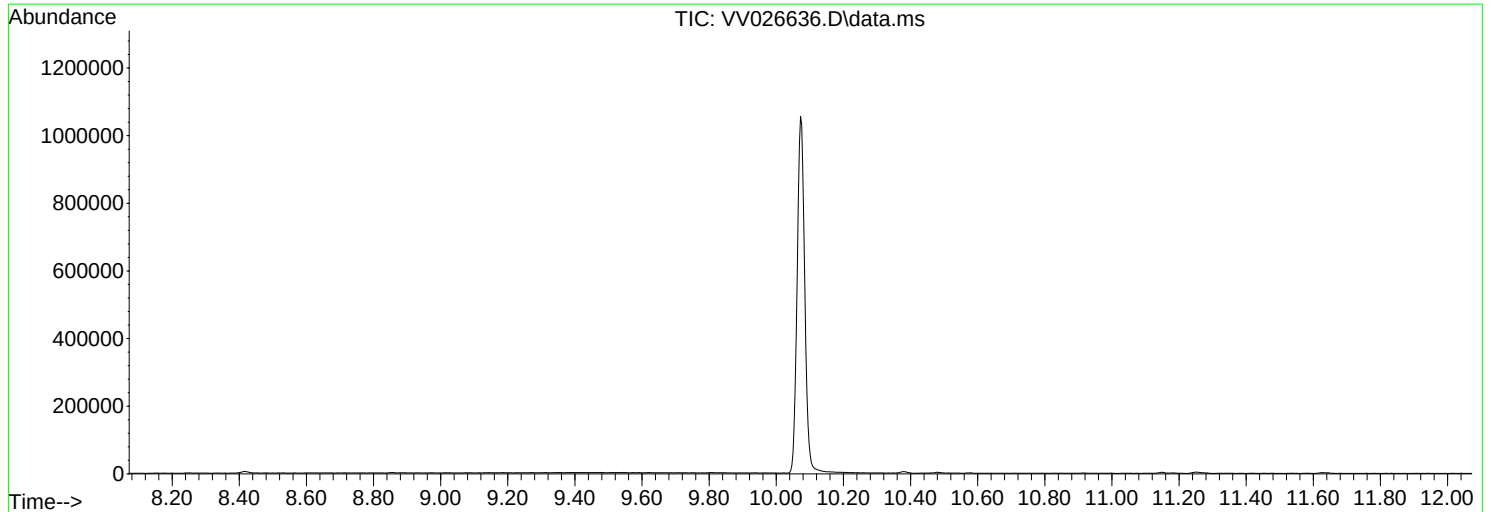

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2795

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.2	33488	PASS
75	95	30	80	48.2	99709	PASS
95	95	100	100	100.0	206955	PASS
96	95	5	9	6.5	13524	PASS
173	174	0.00	2	1.4	2511	PASS
174	95	50	120	86.8	179605	PASS
175	174	5	9	7.4	13202	PASS
176	174	95	105	95.7	171840	PASS
177	176	5	10	6.5	11248	PASS

m/z	Abundance
36.00	1410.0
36.90	142.0
37.90	506.0
39.90	260.0
43.90	298.0

Instrument :
MSVOA_V
ClientSampleId :
BFB338

m/z	Abundance
36.00	2796.0
37.00	7290.0
38.00	6797.0
39.00	2960.0
39.90	321.0
40.30	446.0
42.90	105.0
44.00	1281.0
45.00	1437.0
45.90	387.0
47.00	2111.0
48.00	1048.0
49.00	6732.0
50.00	32648.0
51.00	10110.0
52.00	464.0
53.00	308.0
53.90	150.0
55.00	461.0
56.00	2498.0
57.10	4411.0
57.90	194.0
60.00	1910.0
61.00	9704.0
62.00	8855.0
63.00	8337.0
64.00	1885.0
65.10	1858.0
66.00	308.0
67.10	528.0
68.00	17696.0
69.00	19568.0
70.00	1459.0
72.00	1047.0
73.00	8885.0
74.00	31304.0
75.00	95888.0
76.10	8580.0
77.00	1061.0
78.00	766.0
78.90	7849.0
79.90	2423.0
80.90	8111.0
81.90	2022.0
83.10	187.0
86.00	448.0
87.00	8950.0
88.00	8549.0
91.00	775.0
92.00	5516.0
93.00	9299.0
94.00	23584.0
95.00	198016.0
96.10	13350.0
97.00	486.0
103.90	872.0
104.90	309.0
105.90	683.0
106.80	180.0
108.00	187.0
109.80	106.0
110.90	214.0
112.70	139.0
114.80	288.0
116.00	699.0
116.90	1484.0
117.90	851.0
118.90	1500.0
123.80	124.0
127.90	777.0
129.00	358.0
129.90	635.0
130.80	262.0
135.00	379.0
136.80	391.0
140.00	117.0
140.90	1971.0
142.00	292.0
142.90	3444.0
144.00	244.0
144.90	1479.0
145.90	432.0
146.80	138.0
147.90	626.0
148.80	216.0
150.00	224.0
151.80	167.0
152.80	162.0
154.00	144.0
154.90	428.0
156.90	339.0
158.90	229.0

Instrument :
MSVOA_V
ClientSampleId :
BFB338

161.00	210.0
171.00	665.0
172.00	2697.0
173.00	2438.0
174.00	169536.0
175.00	12647.0
176.00	160896.0
177.00	11023.0
178.10	374.0

Instrument :
MSVOA_V
ClientSampleId :
BFB338

m/z	Abundance
36.00	2949.0
37.00	7808.0
38.00	6923.0
39.00	3152.0
39.90	327.0
40.30	405.0
44.00	1325.0
45.00	1493.0
45.90	331.0
47.00	2121.0
48.00	1076.0
49.00	7411.0
50.00	34656.0
51.00	10793.0
52.00	482.0
53.00	374.0
54.10	164.0
55.00	446.0
56.00	2779.0
57.00	4588.0
58.00	203.0
60.00	2071.0
61.00	9920.0
62.00	9338.0
63.00	8985.0
64.00	2011.0
65.00	2064.0
66.00	288.0
67.10	573.0
68.00	19232.0
69.10	21144.0
70.00	1517.0
71.00	105.0
71.90	1207.0
73.00	9648.0
74.00	34112.0
75.00	103344.0
76.10	8765.0
77.00	1236.0
77.90	915.0
78.90	8456.0
79.90	2460.0
80.90	8466.0
81.90	2179.0
83.10	205.0
86.00	537.0
87.00	9581.0
88.00	9140.0
91.00	891.0
92.00	6068.0
93.00	10275.0
94.00	25552.0
95.00	214400.0
96.10	13930.0
97.00	524.0
104.00	931.0
104.90	332.0
105.90	763.0
106.90	216.0
108.00	232.0
109.90	137.0
110.90	218.0
112.80	138.0
114.80	262.0
116.00	780.0
116.90	1637.0
117.90	965.0
118.90	1633.0
123.80	116.0
127.90	856.0
129.00	433.0
129.90	770.0
130.80	318.0
134.90	355.0
136.80	399.0
140.90	2171.0
142.00	318.0
142.90	3490.0
144.00	229.0
144.90	1518.0
145.90	469.0
146.80	140.0
147.90	590.0
148.80	239.0
149.90	289.0
151.80	187.0
152.80	192.0
154.00	167.0
154.90	497.0
155.80	103.0
157.00	421.0
158.80	226.0

Instrument :
MSVOA_V
ClientSampleId :
BFB338

161.00	264.0
170.90	690.0
172.00	3030.0
173.00	2590.0
174.00	185664.0
175.00	13671.0
176.00	177728.0
177.00	11676.0
178.00	382.0

Instrument :
MSVOA_V
ClientSampleId :
BFB338

m/z	Abundance
36.00	2887.0
37.00	7407.0
38.00	6570.0
39.00	3044.0
39.90	330.0
40.20	351.0
44.00	1383.0
45.00	1351.0
46.00	275.0
47.00	1992.0
47.90	1010.0
49.00	7340.0
50.00	33160.0
51.00	10329.0
52.00	509.0
53.00	378.0
54.20	192.0
55.00	453.0
56.00	2743.0
57.00	4496.0
58.00	204.0
60.00	1949.0
61.00	9370.0
62.00	9016.0
63.00	8654.0
64.00	1839.0
65.00	2183.0
66.00	255.0
67.00	639.0
68.00	18664.0
69.10	20280.0
70.00	1469.0
71.90	1227.0
73.00	9361.0
74.00	33664.0
75.00	99896.0
76.10	8144.0
77.00	1295.0
77.90	993.0
78.90	8202.0
79.90	2351.0
80.90	7942.0
81.90	2070.0
83.10	213.0
86.00	514.0
87.00	9359.0
88.00	8757.0
91.00	848.0
92.00	6053.0
93.00	9784.0
94.00	25128.0
95.00	208448.0
96.10	13291.0
97.00	477.0
102.90	103.0
104.00	895.0
104.90	317.0
105.90	814.0
106.90	219.0
108.00	232.0
109.90	126.0
110.90	229.0
111.90	136.0
112.80	153.0
114.90	231.0
116.00	795.0
116.90	1608.0
118.00	963.0
118.90	1675.0
123.90	120.0
127.90	796.0
129.00	451.0
129.90	841.0
130.80	389.0
134.80	345.0
136.80	409.0
140.90	2125.0
141.90	295.0
142.90	3174.0
143.90	209.0
144.90	1365.0
145.90	462.0
146.80	141.0
147.90	474.0
148.90	220.0
149.90	300.0
151.80	154.0
152.80	206.0
154.00	156.0
154.80	580.0
155.80	105.0
157.00	454.0

Instrument :
MSVOA_V
ClientSampleId :
BFB338

158.80	219.0
161.00	237.0
170.90	624.0
172.00	3057.0
173.00	2506.0
174.00	183616.0
175.00	13288.0
176.00	176896.0
177.00	11045.0
178.00	374.0

Instrument :
MSVOA_V
ClientSampleId :
BFB338