


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV070620\
Data File : VV017351.D
Acq On : 06 Jul 2020 14:53
Operator : SY/MD
Sample : L3154-18
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H4298

Manual Integrations
APPROVED

MMDadoda
7/8/2020 12:26:15 PM

Quant Time: Jul 07 03:01:21 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR061720WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Jul 07 01:14:17 2020
Response via : Initial Calibration

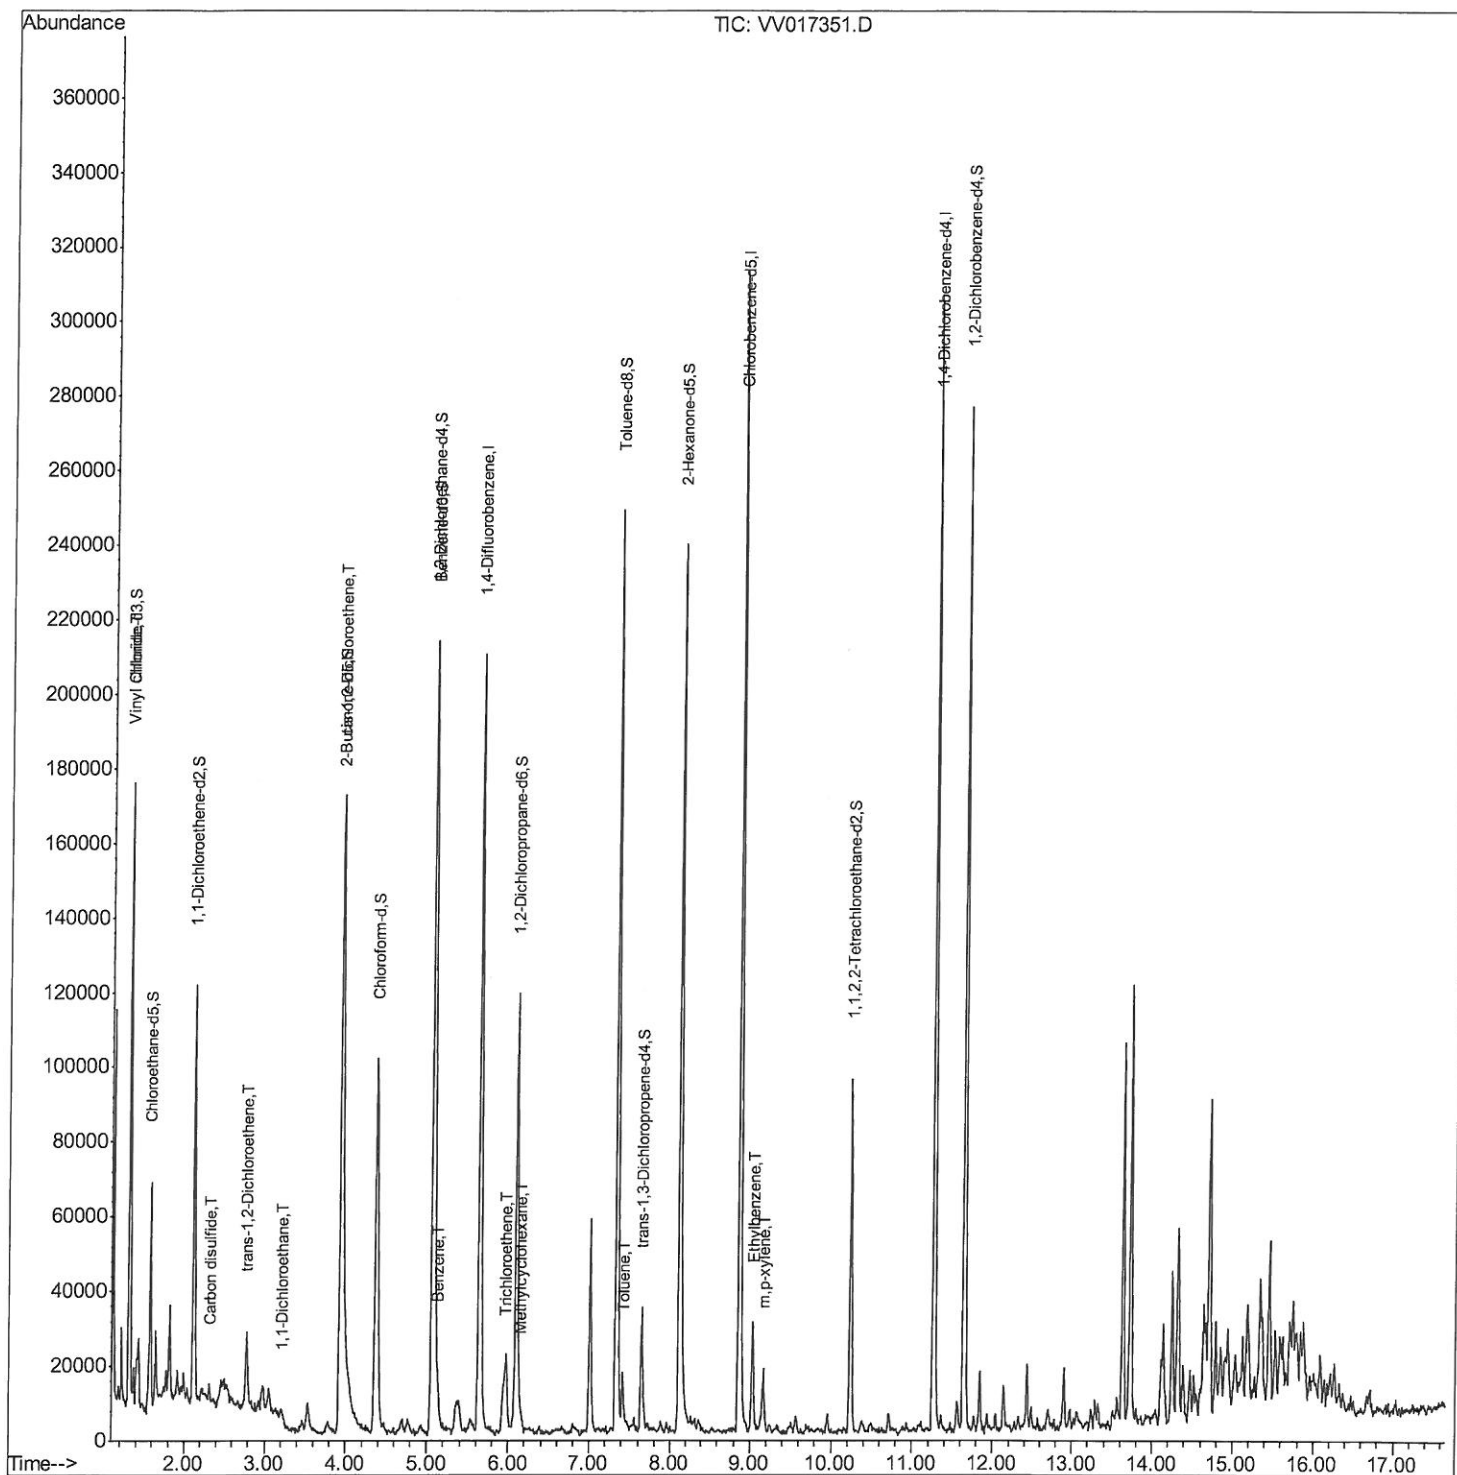

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV070620\
 Data File : VV017351.D
 Acq On : 06 Jul 2020 14:53
 Operator : SY/MD
 Sample : L3154-18
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H4298

Manual Integrations
 APPROVED

MMDadoda
 7/8/2020 12:26:15 PM

Quant Time: Jul 07 01:18:45 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR061720WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Jul 07 01:14:17 2020
 Response via : Initial Calibration

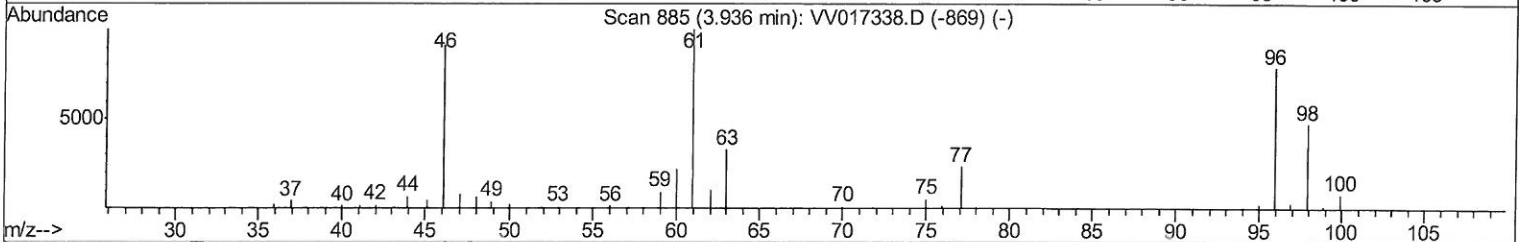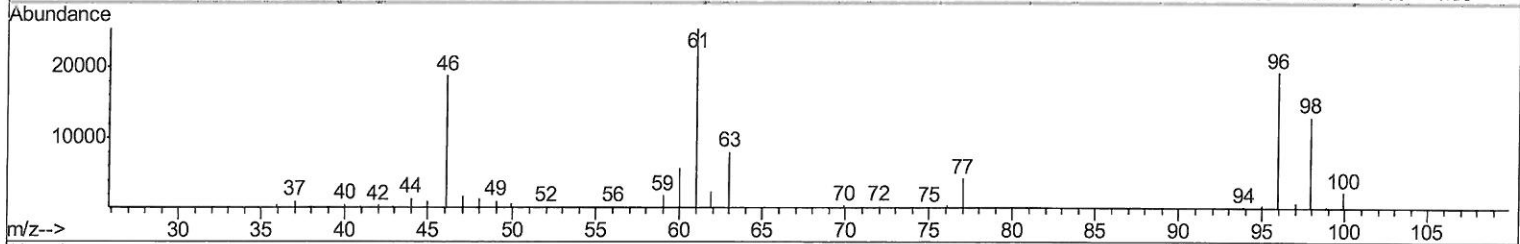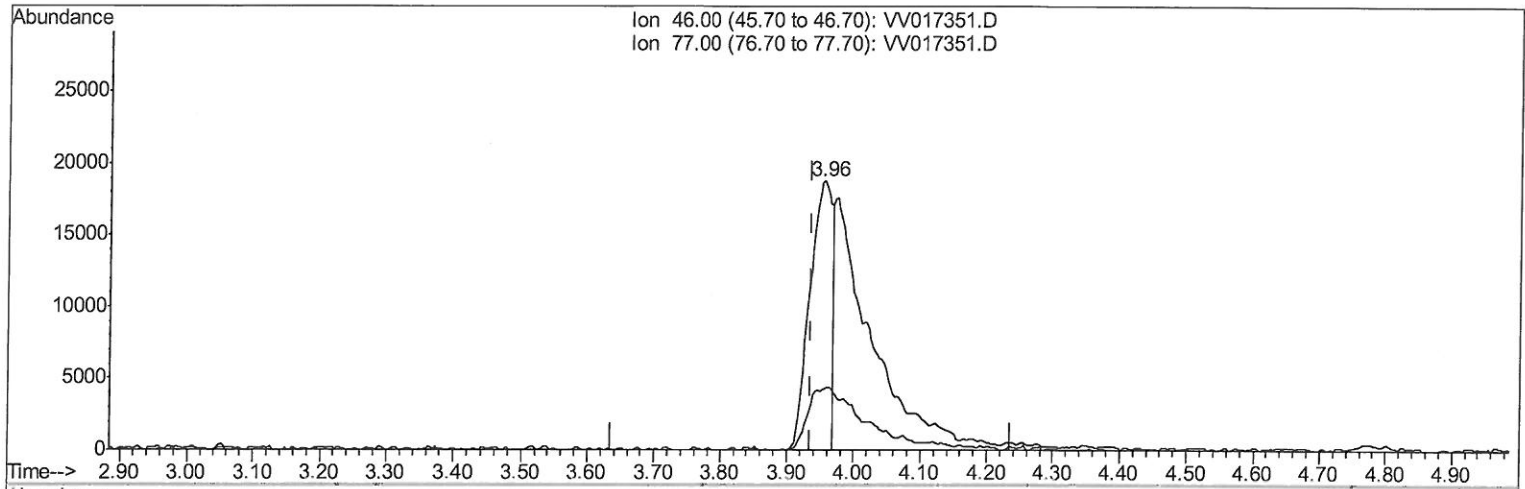

TIC: VV017351.D

(20) 2-Butanone-d5 (S)

3.955min (+0.019) 16.70ug/L

response 43787

Ion	Exp%	Act%
46.00	100	100
77.00	24.20	29.15
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV070620\
Data File : VV017351.D
Acq On : 06 Jul 2020 14:53
Operator : SY/MD
Sample : L3154-18
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
H4298

Manual Integrations
APPROVED

MMDadoda
7/8/2020 12:26:15 PM

Quant Time: Jul 07 01:18:45 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR061720WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Jul 07 01:14:17 2020
Response via : Initial Calibration

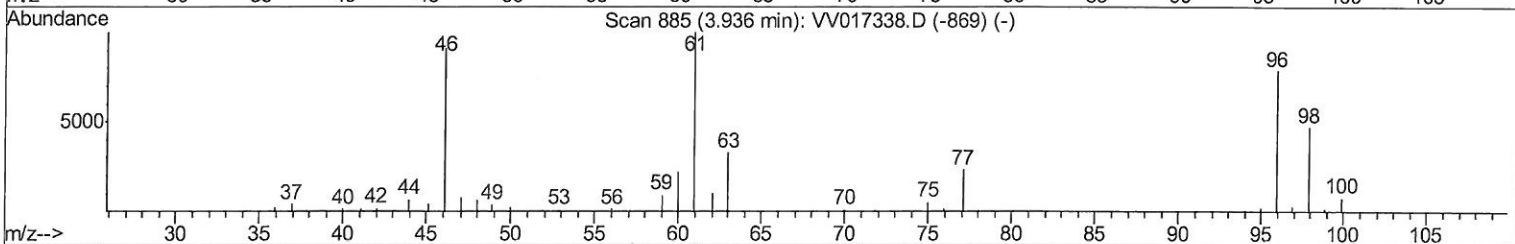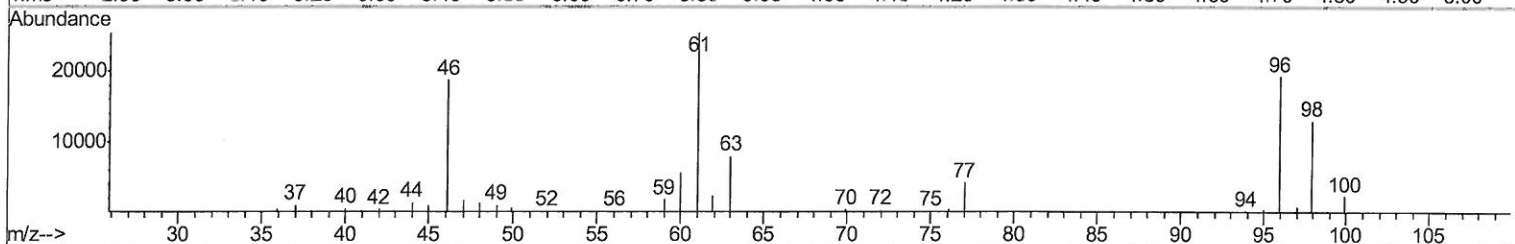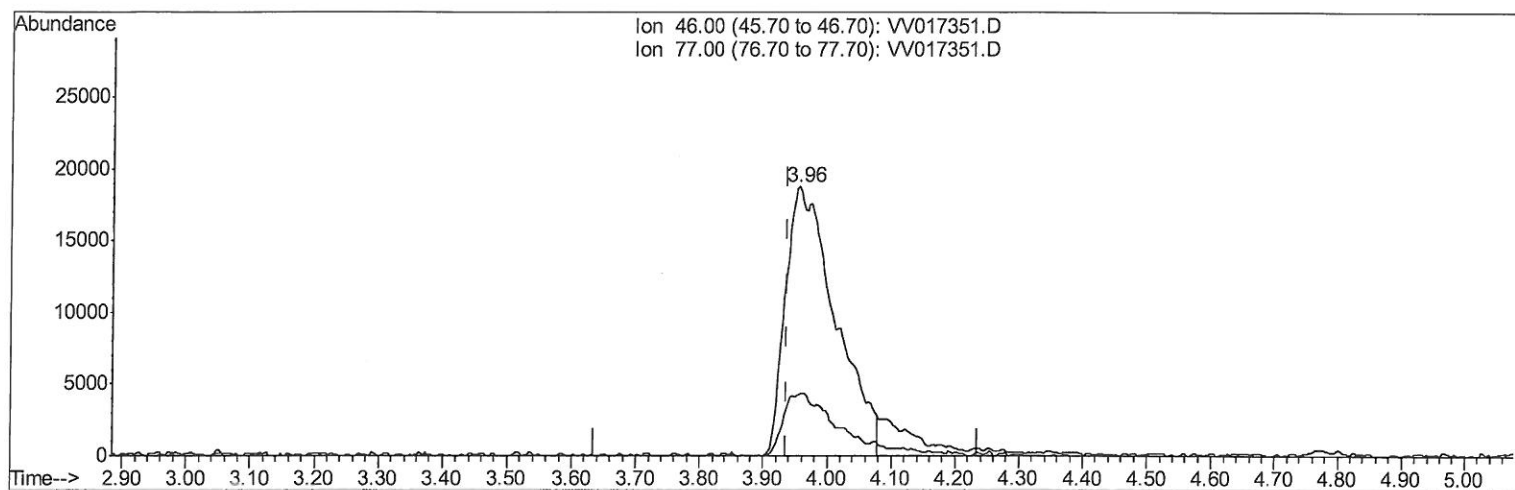

TIC: VV017351.D

(20) 2-Butanone-d5 (S)

3.955min (+0.019) 38.75ug/L m

response 101565

Ion	Exp%	Act%
46.00	100	100
77.00	24.20	12.57#
0.00	0.00	0.00
0.00	0.00	0.00

MD
7/13/20

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV070620\
 Data File : VV017351.D
 Acq On : 06 Jul 2020 14:53
 Operator : SY/MD
 Sample : L3154-18
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H4298

Manual Integrations
 APPROVED

MMDadoda
 7/8/2020 12:26:15 PM

Quant Time: Jul 07 01:18:45 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR061720WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Jul 07 01:14:17 2020
 Response via : Initial Calibration

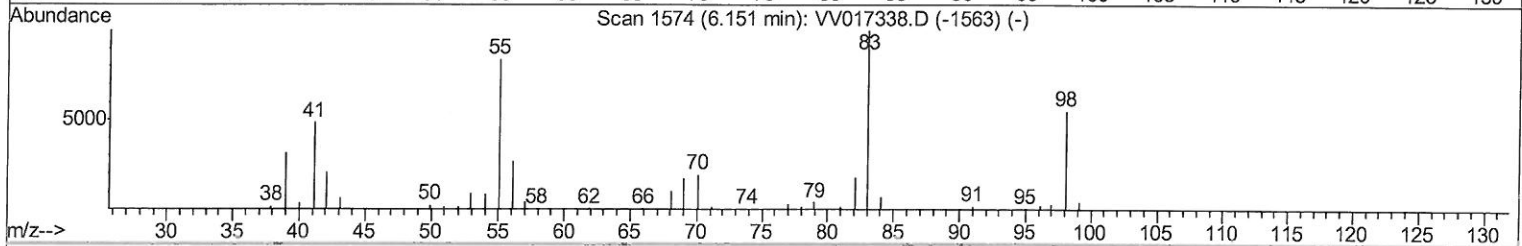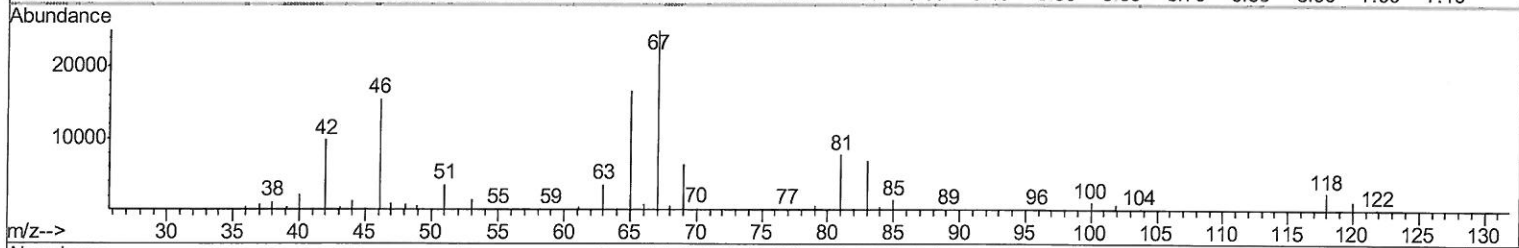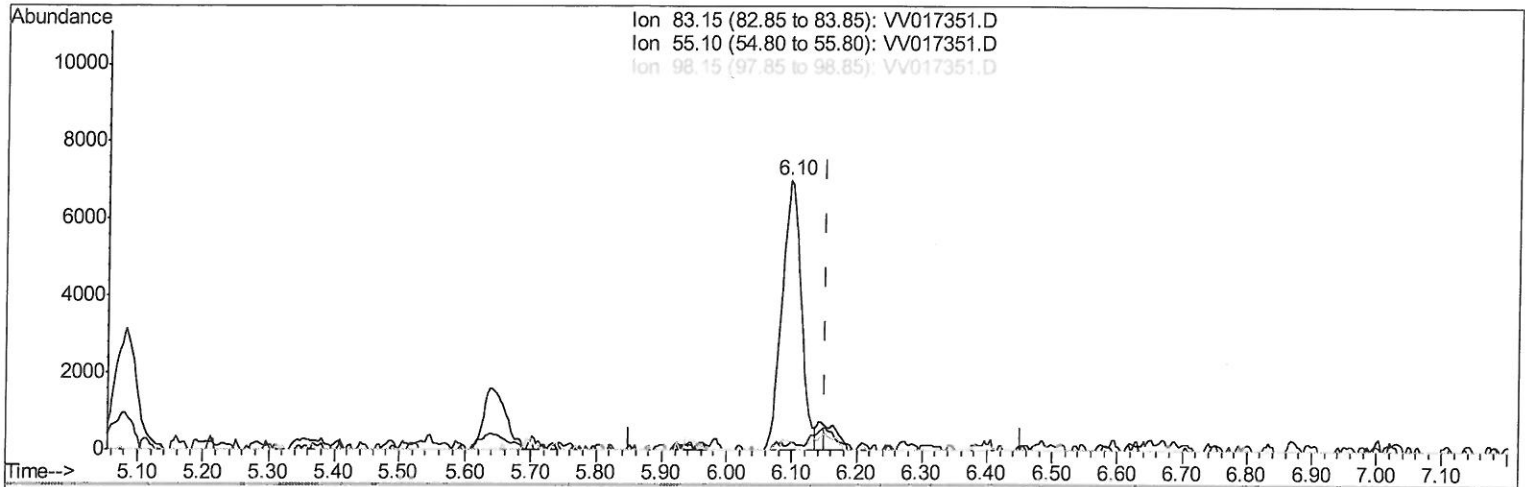

TIC: VV017351.D

(35) Methylcyclohexane (T)

6.096min (-0.055) 0.74ug/L

response 14214

Ion	Exp%	Act%
83.15	100	100
55.10	79.50	1.74#
98.15	48.50	2.05#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV070620\
 Data File : VV017351.D
 Acq On : 06 Jul 2020 14:53
 Operator : SY/MD
 Sample : L3154-18
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H4298

Manual Integrations
 APPROVED

MMDadoda
 7/8/2020 12:26:15 PM

Quant Time: Jul 07 01:18:45 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR061720WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Jul 07 01:14:17 2020
 Response via : Initial Calibration

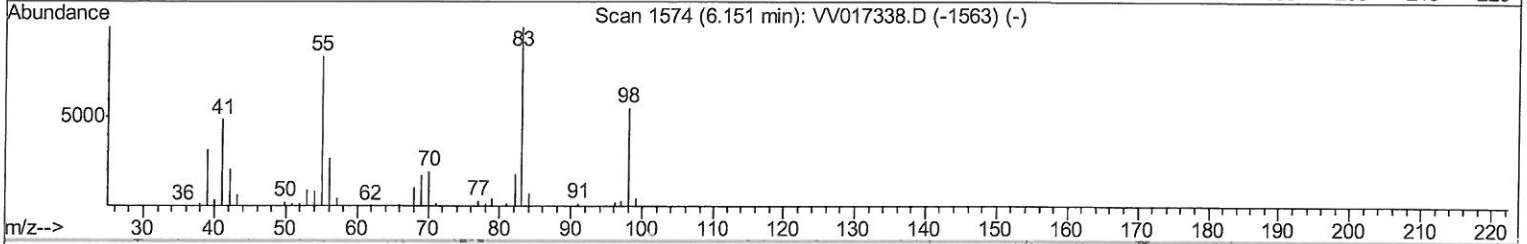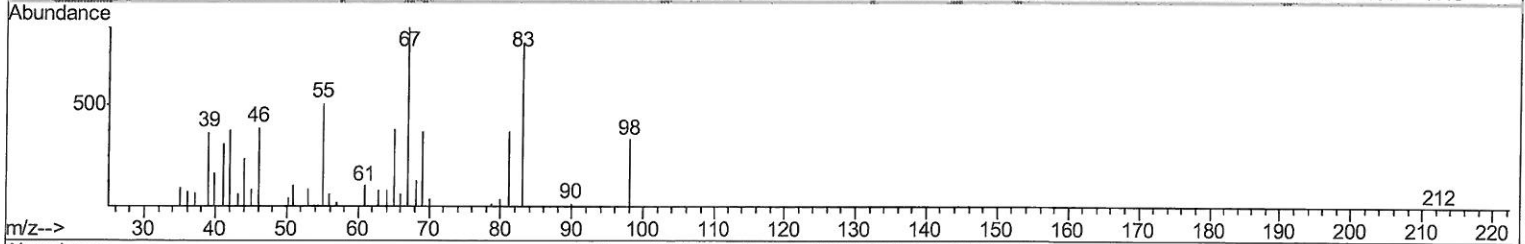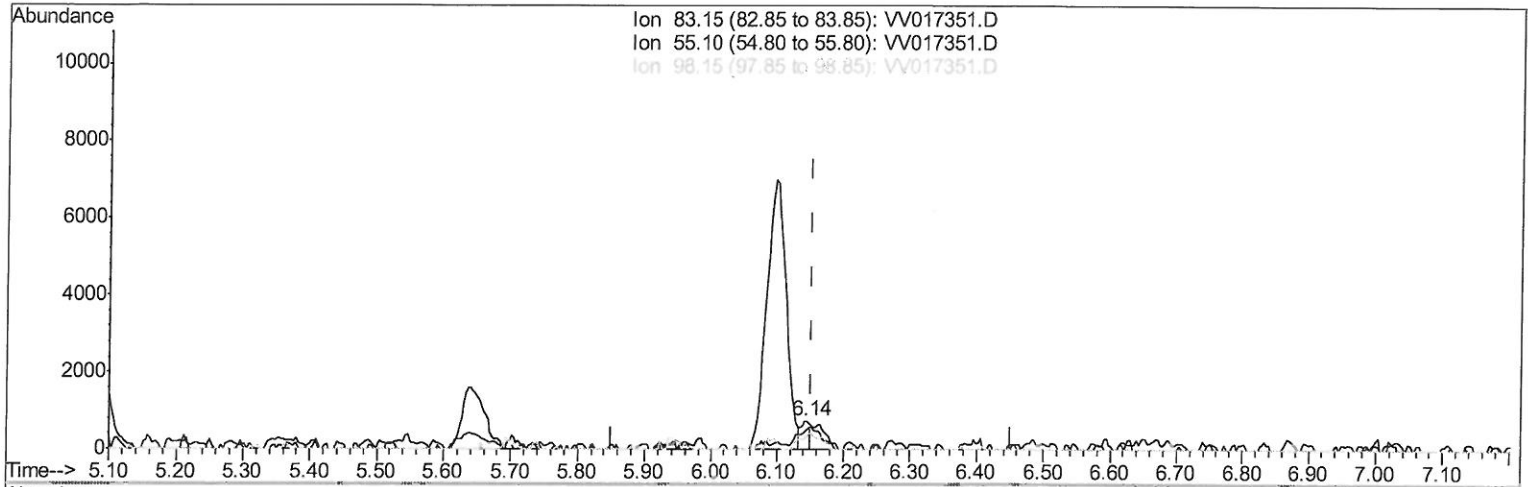

TIC: VV017351.D

(35) Methylcyclohexane (T)

6.145min (-0.006) 0.08ug/L m

response 1628

Ion	Exp%	Act%
83.15	100	100
55.10	79.50	15.23#
98.15	48.50	17.94#
0.00	0.00	0.00

MD
7/13/20

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV070620\
 Data File : VV017351.D
 Acq On : 06 Jul 2020 14:53
 Operator : SY/MD
 Sample : L3154-18
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H4298

Manual Integrations
 APPROVED

MMDadoda
 7/8/2020 12:26:15 PM

Quant Time: Jul 07 03:01:21 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR061720WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Jul 07 01:14:17 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	171372	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	160751	5.00	ug/L	0.00
61) 1,4-Dichlorobenzene-d4	11.27	152	78150	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	34769	3.38	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	67.60%
7) Chloroethane-d5	1.58	69	34527	4.62	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	92.40%
11) 1,1-Dichloroethene-d2	2.12	63	60011	3.07	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	61.40%
20) 2-Butanone-d5	3.96	46	101565m	38.75	ug/L	0.027 <i>md</i>
Spiked Amount	50.000	Range	40 - 130	Recovery	=	77.50%
24) Chloroform-d	4.38	84	100608	4.57	ug/L	0.00 <i>7/13/20</i>
Spiked Amount	5.000	Range	70 - 125	Recovery	=	91.40%
26) 1,2-Dichloroethane-d4	5.06	65	56455	4.84	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	96.80%
32) Benzene-d6	5.08	84	176092	4.22	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	84.40%
36) 1,2-Dichloropropane-d6	6.10	67	52868	4.23	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	84.60%
41) Toluene-d8	7.34	98	155106	3.96	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	79.20%
45) trans-1,3-Dichloropropene-	7.65	79	18174	3.50	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	70.00%
48) 2-Hexanone-d5	8.12	63	79297	40.02	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	80.04%
59) 1,1,2,2-Tetrachloroethane-	10.24	84	38783	4.67	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	93.40%
65) 1,2-Dichlorobenzene-d4	11.65	152	67839	4.70	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	94.00%

Target Compounds

						Ovalue
5) Vinyl chloride	1.32	62	31917	2.838	ug/L	95
14) Carbon disulfide	2.31	76	3544	0.144	ug/L #	76
18) trans-1,2-Dichloroethene	2.78	96	4638	0.532	ug/L	96
19) 1,1-Dichloroethane	3.22	63	3140	0.160	ug/L #	86
22) cis-1,2-Dichloroethene	3.94	96	79846	6.699	ug/L	96
33) Benzene	5.13	78	11985	0.285	ug/L	100
34) Trichloroethene	5.95	95	3616	0.293	ug/L	88
35) Methylcyclohexane	6.14	83	1628m	0.085	ug/L	
42) Toluene	7.41	91	10042	0.205	ug/L	97 <i>md</i>
54) Ethylbenzene	9.04	91	19815	0.379	ug/L	99 <i>7/13/20</i>
55) m,p-xylene	9.16	106	4383	0.214	ug/L	85

(#) = qualifier out of range (m) = manual integration (+) = signals summed