

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV070620\
 Data File : VV017361.D
 Acq On : 06 Jul 2020 19:16
 Operator : SY/MD
 Sample : L3168-10DL 200X
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AJ6DL

Quant Time: Jul 07 03:53:12 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR061720WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Jul 07 01:14:17 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	156246	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	150979	5.00	ug/L	0.00
61) 1,4-Dichlorobenzene-d4	11.27	152	73698	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.31	65	38589	4.11	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	82.20%
7) Chloroethane-d5	1.58	69	33125	4.86	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	97.20%
11) 1,1-Dichloroethene-d2	2.12	63	67316	3.77	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	75.40%
20) 2-Butanone-d5	3.96	46	92646	38.76	ug/L	0.03
Spiked Amount	50.000	Range	40 - 130	Recovery	=	77.52%
24) Chloroform-d	4.38	84	97069	4.84	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	96.80%
26) 1,2-Dichloroethane-d4	5.06	65	54688	5.14	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	102.80%
32) Benzene-d6	5.07	84	174679	4.46	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	89.20%
36) 1,2-Dichloropropane-d6	6.10	67	49075	4.18	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	83.60%
41) Toluene-d8	7.34	98	158498	4.31	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	86.20%
45) trans-1,3-Dichloropropene-	7.65	79	20356	4.17	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	83.40%
48) 2-Hexanone-d5	8.12	63	67313	36.17	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	72.34%
59) 1,1,2,2-Tetrachloroethane-	10.24	84	34967	4.49	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	89.80%
65) 1,2-Dichlorobenzene-d4	11.65	152	62442	4.58	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	91.60%


Target Compounds					Ovalue
49) Tetrachloroethene	8.00	164	103034	11.057 ug/L	98




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV070620\
Data File : VV017361.D
Acq On : 06 Jul 2020 19:16
Operator : SY/MD
Sample : L3168-10DL 200X
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AJ6DL

Quant Time: Jul 07 03:53:12 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR061720WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Jul 07 01:14:17 2020
Response via : Initial Calibration

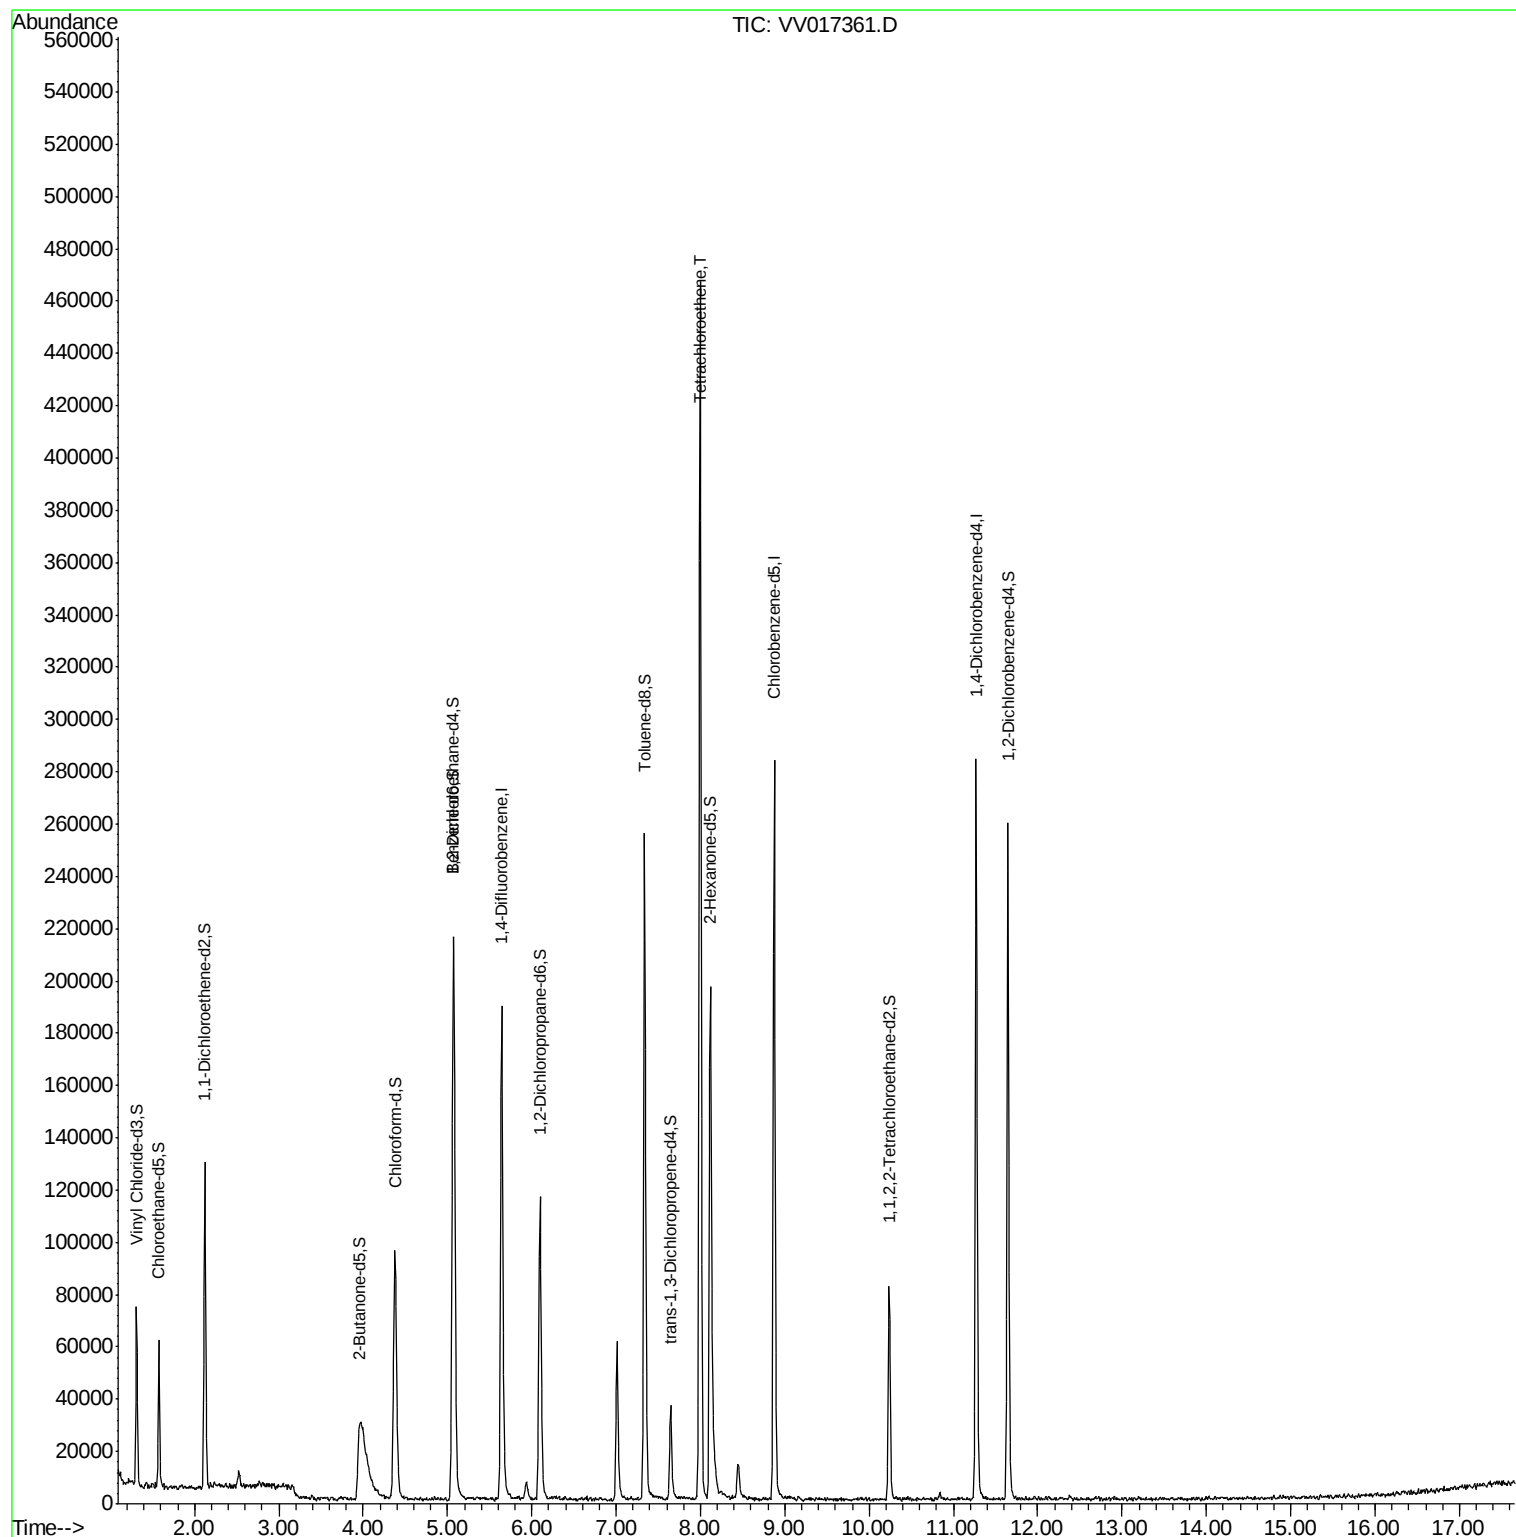

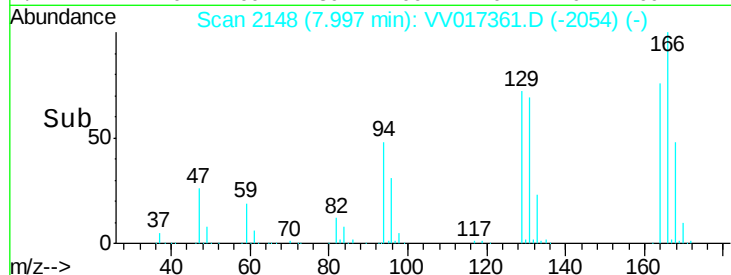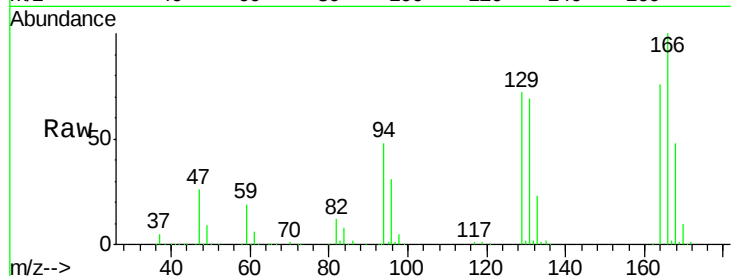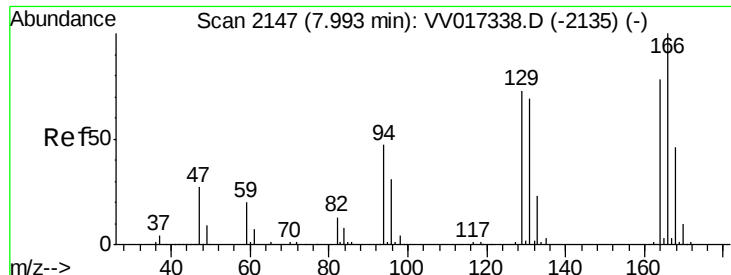

#49

Tetrachloroethene

Concen: 11.057 ug/L

RT: 8.00 min Scan# 2148

Delta R.T. 0.00 min

Lab File: VV017361.D

Acq: 06 Jul 2020 19:16

Instrument :
MSVOA_V
ClientSampleId :
C0AJ6DL

Tot Ion:164 Resp: 103034

Ion Ratio Lower Upper

164 100

129 95.0 65.2 121.0

131 90.4 64.1 119.1

166 131.6 90.2 167.4

Abundance Ion 163.90 (163.60 to 164.60): V

Ion 128.95 (128.65 to 129.65): V

Ion 130.95 (130.65 to 131.65): V

Ion 165.90 (165.60 to 166.60): V

