


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV070620\
 Data File : VV017337.D
 Acq On : 06 Jul 2020 08:51
 Operator : SY/MD
 Sample : BFB47
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB47

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR061720WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Tue Jul 07 01:14:17 2020

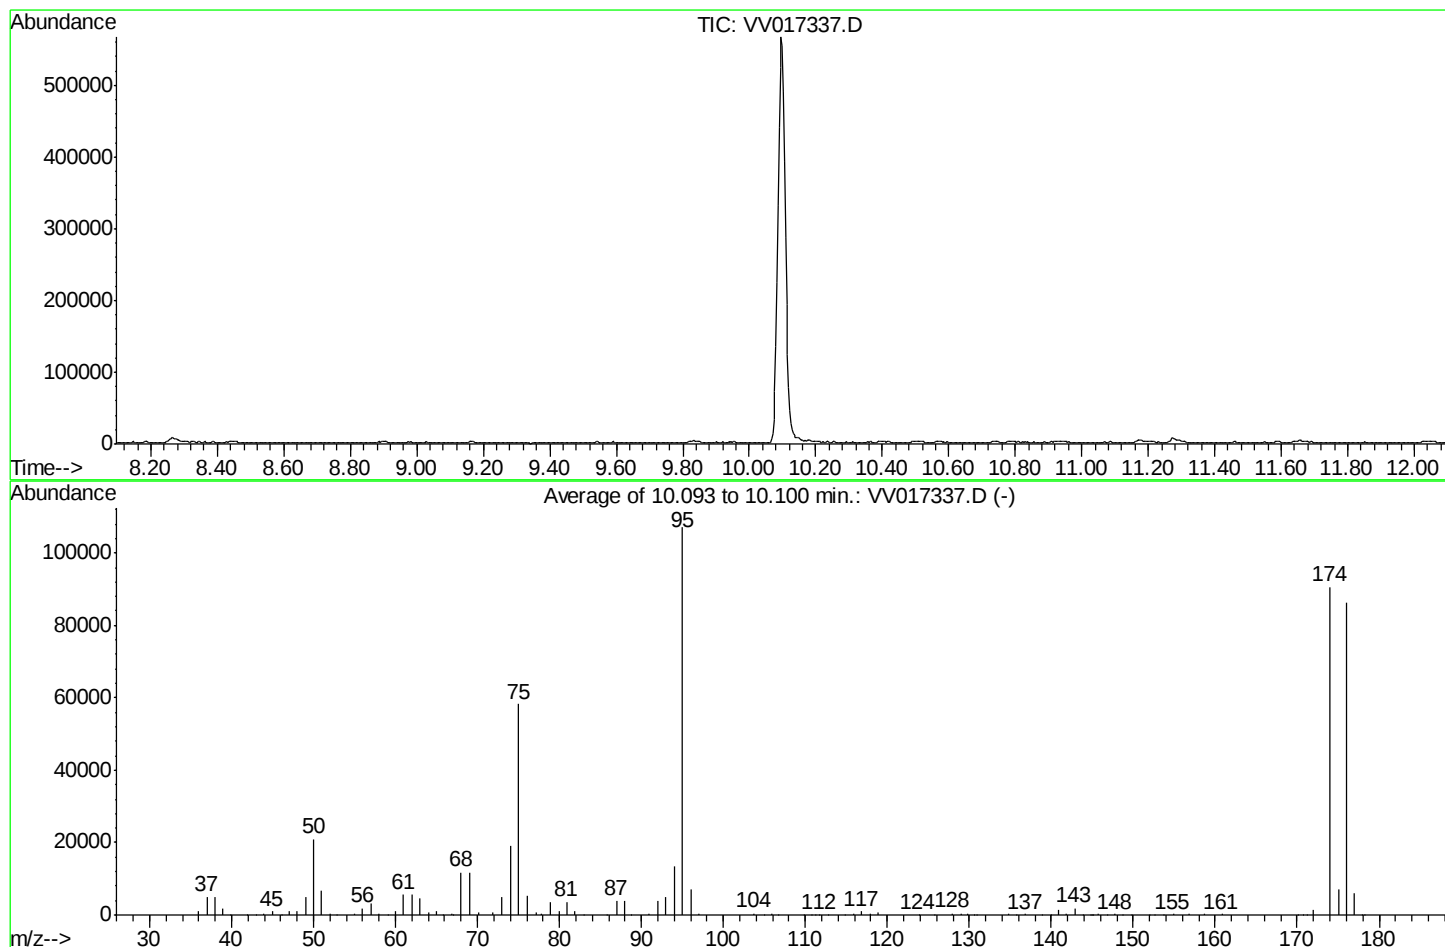

AutoFind: Scans 2800, 2801, 2802; Background Corrected with Scan 2787

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.7	21045	PASS
75	95	30	80	54.4	58288	PASS
95	95	100	100	100.0	107098	PASS
96	95	5	9	6.5	6944	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	84.7	90706	PASS
175	174	5	9	8.0	7255	PASS
176	174	95	101	95.0	86208	PASS
177	176	5	9	6.8	5878	PASS

m/z	Abundance
35.90	1122.0
37.00	5045.0
38.00	4881.0
39.00	2001.0
40.00	262.0
41.00	117.0
42.00	160.0
43.00	229.0
44.00	878.0
45.00	925.0
46.10	147.0
47.00	1103.0
47.90	947.0
49.00	4900.0
50.00	20696.0
51.00	6438.0
51.90	253.0
55.00	401.0
56.00	1930.0
57.00	3368.0
58.00	219.0
60.00	1037.0
61.00	5369.0
62.00	5663.0
63.00	4485.0
64.00	928.0
65.00	1103.0
65.90	169.0
66.80	319.0
68.00	11407.0
69.00	11439.0
70.10	953.0
71.90	697.0
73.00	4763.0
74.00	18320.0
75.00	56352.0
76.00	5090.0
77.10	553.0
77.80	480.0
78.90	3442.0
79.90	963.0
80.90	3604.0
81.90	1006.0
83.00	118.0
85.80	155.0
87.00	3975.0
88.00	3539.0
88.70	133.0
90.80	506.0
92.00	3689.0
93.00	4765.0
94.00	12229.0
95.00	102848.0
96.00	6544.0
97.20	144.0
103.80	553.0
104.90	169.0
105.90	457.0
106.70	122.0
110.70	130.0
111.20	146.0
112.70	106.0
114.90	185.0
115.90	487.0
116.80	861.0
117.90	516.0
118.90	675.0
123.80	143.0
125.70	104.0
128.00	486.0
129.00	143.0
129.80	451.0
130.60	149.0
130.90	129.0
134.80	221.0
135.80	142.0
136.80	326.0
139.90	133.0
140.90	1395.0
141.90	181.0
142.90	1684.0
143.90	163.0
144.80	280.0
145.00	267.0
145.70	183.0
146.80	133.0
147.80	281.0
148.80	103.0
149.80	145.0
151.90	158.0
154.90	290.0
156.80	297.0

Instrument :
MSVOA_V
ClientSampleId :
BFB47

158.70	141.0
160.80	183.0
170.70	147.0
171.90	1285.0
174.00	84984.0
175.00	6830.0
176.00	80760.0
176.90	5629.0
178.00	201.0

Instrument :
MSVOA_V
ClientSampleId :
BFB47

m/z	Abundance
35.90	1127.0
37.00	5176.0
38.00	5188.0
39.00	2175.0
40.00	315.0
41.10	138.0
42.00	137.0
43.00	170.0
44.00	896.0
45.00	977.0
46.00	158.0
47.00	1195.0
47.90	960.0
49.00	5052.0
50.00	21808.0
51.00	6793.0
51.90	322.0
52.70	166.0
55.00	409.0
56.00	2007.0
57.00	3443.0
57.90	240.0
59.10	101.0
60.00	1128.0
61.00	5666.0
62.00	5855.0
63.00	4734.0
64.00	768.0
65.00	1103.0
65.80	179.0
66.80	330.0
68.00	12279.0
69.00	12103.0
70.10	938.0
71.90	806.0
73.00	4997.0
74.00	19688.0
75.00	60304.0
76.00	5353.0
77.10	691.0
77.80	525.0
78.90	3636.0
79.90	922.0
80.90	3767.0
81.90	1010.0
83.00	162.0
85.80	140.0
87.00	4132.0
88.00	4043.0
88.80	156.0
90.80	542.0
91.90	3931.0
93.00	4889.0
94.00	13973.0
95.00	110680.0
96.10	7240.0
97.00	178.0
103.70	518.0
104.90	167.0
105.90	495.0
106.80	179.0
109.80	112.0
110.70	111.0
111.20	114.0
111.80	163.0
112.70	120.0
114.80	162.0
115.90	520.0
116.90	939.0
117.90	493.0
118.80	738.0
123.90	164.0
125.70	136.0
128.00	517.0
128.90	197.0
129.80	438.0
130.70	172.0
134.70	256.0
135.80	134.0
136.90	360.0
139.90	111.0
140.90	1632.0
141.90	219.0
142.90	1852.0
143.80	193.0
145.10	294.0
145.70	193.0
146.90	170.0
147.80	349.0
148.80	126.0
149.70	150.0
151.90	138.0

Instrument :
MSVOA_V
ClientSampleId :
BFB47

152.60	110.0
154.90	362.0
156.80	283.0
158.70	204.0
160.90	222.0
170.70	180.0
172.00	1381.0
174.00	93192.0
175.00	7465.0
176.00	89200.0
176.90	6126.0
177.90	152.0

Instrument :
MSVOA_V
ClientSampleId :
BFB47

m/z	Abundance
36.00	1036.0
37.00	4900.0
38.00	5047.0
39.00	2052.0
39.90	338.0
41.10	136.0
41.90	124.0
42.80	145.0
43.90	829.0
45.00	970.0
46.00	207.0
47.00	1172.0
48.00	964.0
49.00	4650.0
50.00	20632.0
51.00	6442.0
52.00	334.0
52.80	165.0
55.00	309.0
56.00	1770.0
57.00	3066.0
57.90	277.0
60.00	1188.0
61.00	5721.0
62.00	5510.0
63.00	4558.0
64.00	577.0
65.00	854.0
65.70	168.0
67.00	336.0
68.00	11517.0
69.00	11582.0
70.10	791.0
71.90	824.0
73.00	4931.0
74.00	19608.0
75.00	58208.0
76.00	5099.0
77.10	723.0
77.80	517.0
78.90	3382.0
79.90	830.0
80.90	3550.0
81.90	983.0
83.00	177.0
85.80	108.0
86.90	3775.0
87.90	4115.0
88.80	168.0
90.90	497.0
92.00	3762.0
93.00	4879.0
94.00	14268.0
95.00	107768.0
96.00	7049.0
96.90	300.0
103.80	477.0
104.90	155.0
105.90	507.0
106.80	201.0
109.80	132.0
110.70	104.0
111.70	191.0
112.70	119.0
114.70	160.0
115.80	483.0
116.90	1027.0
117.90	387.0
118.80	724.0
123.90	188.0
125.70	127.0
127.90	484.0
128.90	251.0
129.90	408.0
130.80	183.0
134.80	258.0
136.90	327.0
138.80	105.0
140.90	1606.0
141.80	236.0
142.90	1825.0
143.80	161.0
144.90	305.0
145.70	228.0
146.90	208.0
147.80	345.0
148.70	126.0
149.80	133.0
152.60	125.0
153.70	101.0
154.90	382.0
156.90	257.0

Instrument :
MSVOA_V
ClientSampleId :
BFB47

158.70	223.0
160.80	238.0
170.10	141.0
170.70	165.0
171.10	169.0
171.90	1328.0
174.00	93944.0
175.00	7471.0
176.00	88664.0
176.90	5880.0
177.90	103.0
178.20	110.0

Instrument :
MSVOA_V
ClientSampleId :
BFB47

Scan 2787 (10.051 min): VV017337.D
BFB47

m/z	Abundance
35.40	123.0
38.80	121.0
39.90	204.0
40.90	140.0
42.00	100.0
43.90	341.0
46.10	132.0
53.00	113.0
62.20	103.0
67.50	106.0
72.20	100.0

Instrument :
MSVOA_V
ClientSampleId :
BFB47