

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070621\
 Data File : VV021607.D
 Acq On : 06 Jul 2021 10:04
 Operator : SY/MD
 Sample : VV0706WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK200

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M

Title : VOC Analysis

Signal : TIC: VV021607.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	96	rVB	184670	188477	11.54%	1.449%
2	1.564	156	163	177	rVB	159638	179159	10.97%	1.377%
3	2.105	322	331	355	rVB	340569	511584	31.32%	3.932%
4	2.654	500	502	503	rBV	280	69	0.00%	0.001%
5	2.876	568	571	574	rBV	365	225	0.01%	0.002%
6	2.899	574	578	580	rBV2	393	326	0.02%	0.003%
7	2.912	580	582	587	rVB	372	231	0.01%	0.002%
8	2.934	587	589	592	rBV2	350	261	0.02%	0.002%
9	3.043	619	623	625	rBV4	527	451	0.03%	0.003%
10	3.108	639	643	646	rBV3	450	350	0.02%	0.003%
11	3.124	646	648	649	rBV	179	69	0.00%	0.001%
12	3.188	665	668	670	rBV	444	229	0.01%	0.002%
13	3.224	676	679	680	rBV	261	179	0.01%	0.001%
14	3.285	694	698	701	rBV3	553	346	0.02%	0.003%
15	3.323	707	710	712	rBV2	305	188	0.01%	0.001%
16	3.346	715	717	719	rBV	218	120	0.01%	0.001%
17	3.426	741	742	745	rBV2	369	173	0.01%	0.001%
18	3.490	758	762	764	rBV	270	202	0.01%	0.002%
19	3.539	775	777	780	rBV	211	169	0.01%	0.001%
20	3.571	785	787	791	rVB2	271	120	0.01%	0.001%
21	3.609	793	799	800	rBV4	213	215	0.01%	0.002%
22	3.638	805	808	810	rBV	276	178	0.01%	0.001%
23	3.664	814	816	817	rBV	279	121	0.01%	0.001%
24	3.748	841	842	844	rBV	175	49	0.00%	0.000%
25	3.764	844	847	851	rBV2	438	251	0.02%	0.002%
26	3.812	855	862	865	rBV3	454	474	0.03%	0.004%
27	3.873	870	881	930	rBV	144312	399178	24.44%	3.068%
28	4.346	1014	1028	1055	rBV	258794	639491	39.15%	4.915%
29	4.783	1160	1164	1165	rBV2	382	205	0.01%	0.002%
30	4.818	1173	1175	1179	rBB3	240	127	0.01%	0.001%
31	4.883	1190	1195	1198	rBV2	441	482	0.03%	0.004%
32	4.918	1205	1206	1209	rVB	220	80	0.00%	0.001%
33	4.937	1210	1212	1213	rBV	135	37	0.00%	0.000%
34	4.950	1213	1216	1222	rVB2	489	534	0.03%	0.004%
35	4.976	1222	1224	1227	rBV2	396	212	0.01%	0.002%
36	5.043	1228	1245	1282	rBV2	630211	1633505	100.00%	12.555%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070621\
 Data File : VV021607.D
 Acq On : 06 Jul 2021 10:04
 Operator : SY/MD
 Sample : VV0706WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK200

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M
 Title : VOC Analysis

37	5.474	1376	1379	1381	rBV3	745	540	0.03%	0.004%
38	5.535	1396	1398	1399	rBV3	297	100	0.01%	0.001%
39	5.616	1410	1423	1454	rBV	549944	1109495	67.92%	8.527%
40	5.908	1502	1514	1534	rVB2	17486	38246	2.34%	0.294%
41	6.069	1550	1564	1593	rBV	362330	743311	45.50%	5.713%
42	6.420	1671	1673	1676	rBV2	267	135	0.01%	0.001%
43	6.474	1687	1690	1691	rBV2	291	160	0.01%	0.001%
44	6.526	1704	1706	1708	rVB	323	99	0.01%	0.001%
45	6.622	1727	1736	1737	rBV3	4148	5153	0.32%	0.040%
46	6.776	1780	1784	1786	rBV3	530	356	0.02%	0.003%
47	6.828	1796	1800	1806	rVB3	703	731	0.04%	0.006%
48	6.857	1806	1809	1810	rBV2	472	320	0.02%	0.002%
49	6.918	1825	1828	1831	rBV2	399	288	0.02%	0.002%
50	6.985	1838	1849	1875	rBV	211920	385208	23.58%	2.961%
51	7.317	1940	1952	1973	rBV	774776	1337390	81.87%	10.279%
52	7.622	2036	2047	2075	rBV	145055	258323	15.81%	1.985%
53	7.899	2130	2133	2134	rBV	499	265	0.02%	0.002%
54	8.088	2181	2192	2221	rBV	463168	852949	52.22%	6.556%
55	8.583	2343	2346	2350	rVB4	381	206	0.01%	0.002%
56	8.606	2351	2353	2355	rBV3	462	206	0.01%	0.002%
57	8.657	2367	2369	2371	rVB	322	124	0.01%	0.001%
58	8.709	2383	2385	2386	rBV2	256	71	0.00%	0.001%
59	8.747	2396	2397	2399	rBV2	213	87	0.01%	0.001%
60	8.773	2404	2405	2407	rVB	431	101	0.01%	0.001%
61	8.783	2407	2408	2410	rBV	254	94	0.01%	0.001%
62	8.796	2410	2412	2414	rBV2	262	152	0.01%	0.001%
63	8.854	2417	2430	2458	rBV	783841	1308606	80.11%	10.058%
64	9.120	2511	2513	2515	rBV2	268	131	0.01%	0.001%
65	9.153	2515	2523	2533	rVV5	1292	2507	0.15%	0.019%
66	9.210	2539	2541	2543	rVB2	443	164	0.01%	0.001%
67	9.246	2549	2552	2556	rVB2	515	412	0.03%	0.003%
68	9.265	2556	2558	2560	rBV	290	137	0.01%	0.001%
69	9.310	2567	2572	2578	rBV4	268	404	0.02%	0.003%
70	9.429	2606	2609	2610	rBV	160	71	0.00%	0.001%
71	9.439	2610	2612	2613	rBV	202	69	0.00%	0.001%
72	9.477	2621	2624	2626	rBV4	413	245	0.01%	0.002%
73	9.490	2626	2628	2634	rVB3	437	417	0.03%	0.003%
74	9.709	2694	2696	2698	rBV3	354	150	0.01%	0.001%
75	9.754	2706	2710	2717	rBV2	476	456	0.03%	0.004%
76	9.828	2730	2733	2736	rVB	506	256	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070621\
 Data File : VV021607.D
 Acq On : 06 Jul 2021 10:04
 Operator : SY/MD
 Sample : VV0706WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK200

Integration Parameters: LSCINT.P

Integrator: RTE

Smoother: OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M

Title : VOC Analysis

77	9.982	2779	2781	2786	rBV	211	178	0.01%	0.001%
78	10.079	2806	2811	2813	rBV	438	343	0.02%	0.003%
79	10.127	2819	2826	2837	rVB4	2151	3550	0.22%	0.027%
80	10.217	2842	2854	2875	rBV	520655	817884	50.07%	6.286%
81	10.429	2918	2920	2925	rBV2	469	279	0.02%	0.002%
82	10.480	2934	2936	2939	rVB	296	131	0.01%	0.001%
83	10.548	2949	2957	2961	rBV5	1329	1844	0.11%	0.014%
84	10.699	3002	3004	3007	rBV3	413	144	0.01%	0.001%
85	10.876	3057	3059	3061	rBV3	408	241	0.01%	0.002%
86	10.921	3066	3073	3081	rVB5	3757	5532	0.34%	0.043%
87	11.079	3120	3122	3124	rBV	268	113	0.01%	0.001%
88	11.146	3138	3143	3150	rBV5	1439	1914	0.12%	0.015%
89	11.249	3164	3175	3203	rBV	839556	1319857	80.80%	10.144%
90	11.519	3257	3259	3260	rBV	326	162	0.01%	0.001%
91	11.625	3280	3292	3314	rBV	781393	1230699	75.34%	9.459%
92	12.030	3416	3418	3421	rBV	314	124	0.01%	0.001%
93	12.651	3605	3611	3618	rBV6	3451	4183	0.26%	0.032%
94	13.265	3796	3802	3811	rBV5	5439	8085	0.49%	0.062%
95	13.750	3946	3953	3964	rVB3	6561	9359	0.57%	0.072%




Sum of corrected areas: 13010824

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070621\
Data File : VV021607.D
Acq On : 06 Jul 2021 10:04
Operator : SY/MD
Sample : VV0706WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK200

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

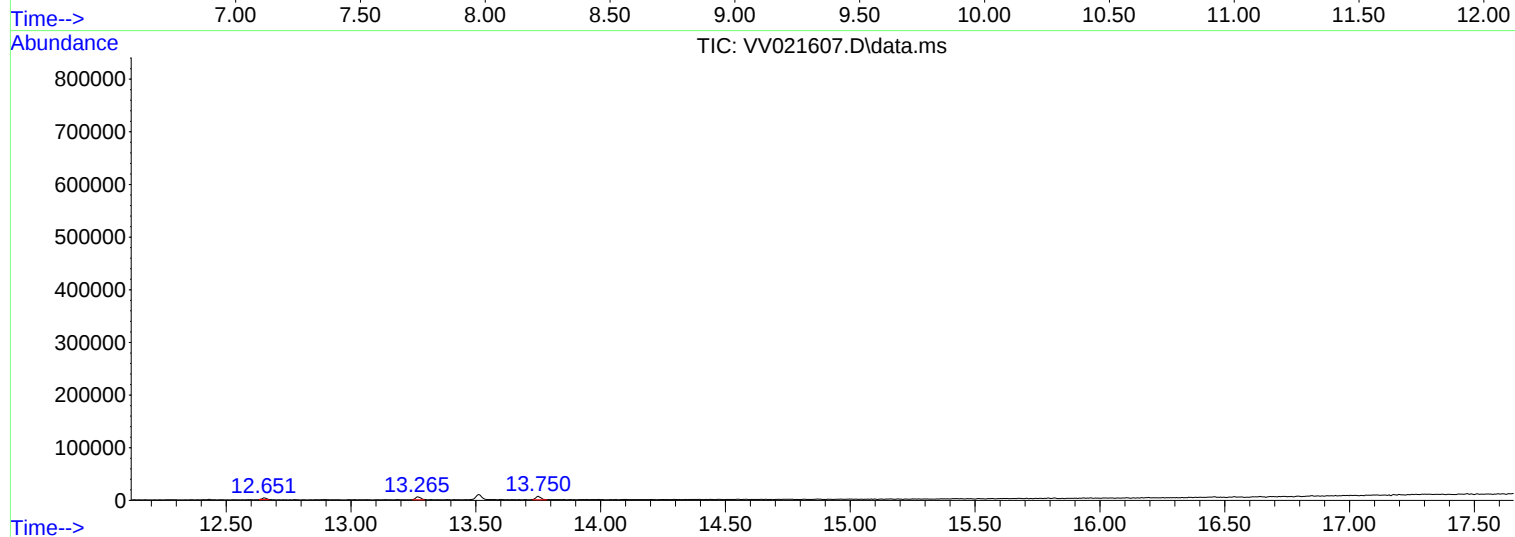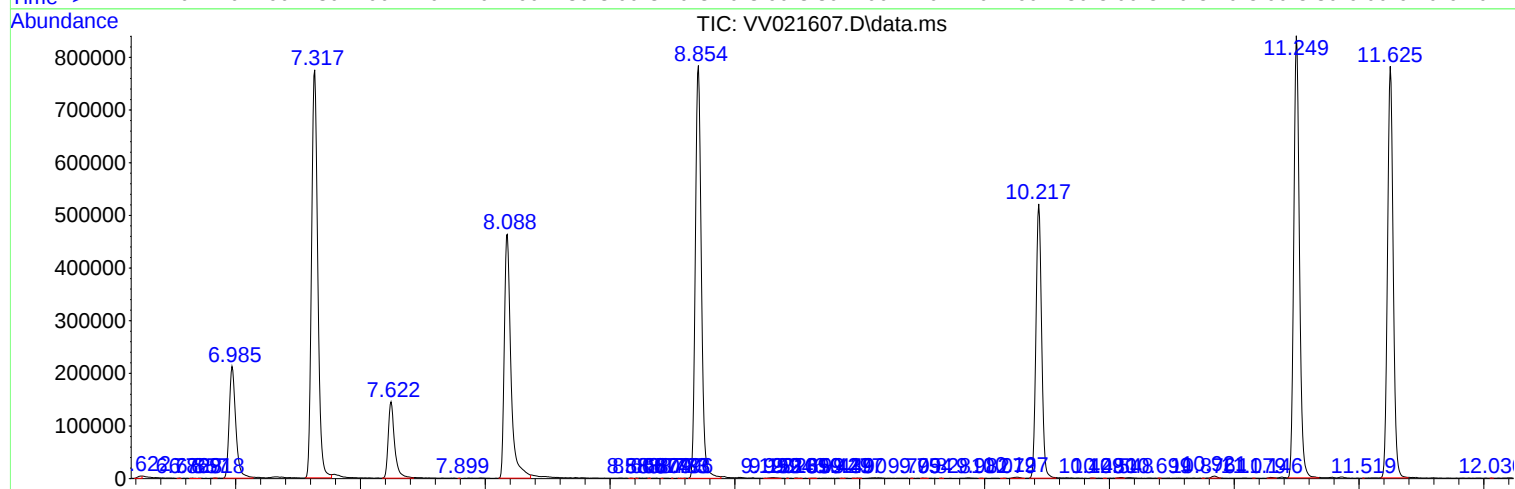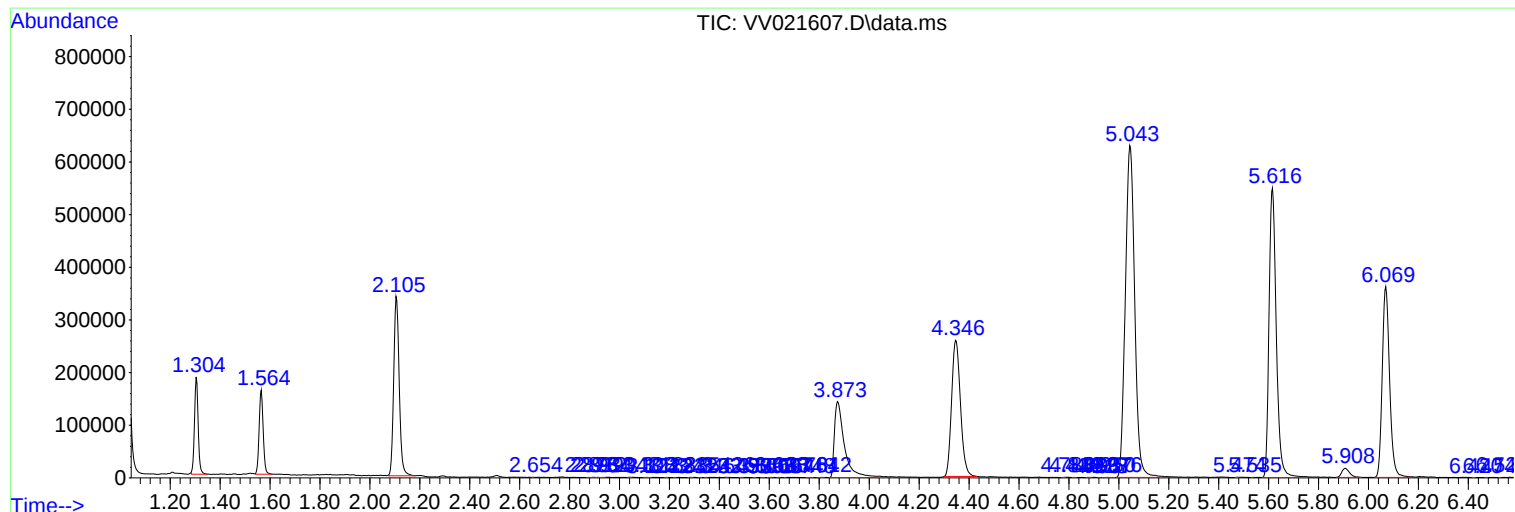

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070621\
Data File : VV021607.D
Acq On : 06 Jul 2021 10:04
Operator : SY/MD
Sample : VV0706WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK200

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070621\
Data File : VV021607.D
Acq On : 06 Jul 2021 10:04
Operator : SY/MD
Sample : VV0706WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK200

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
