
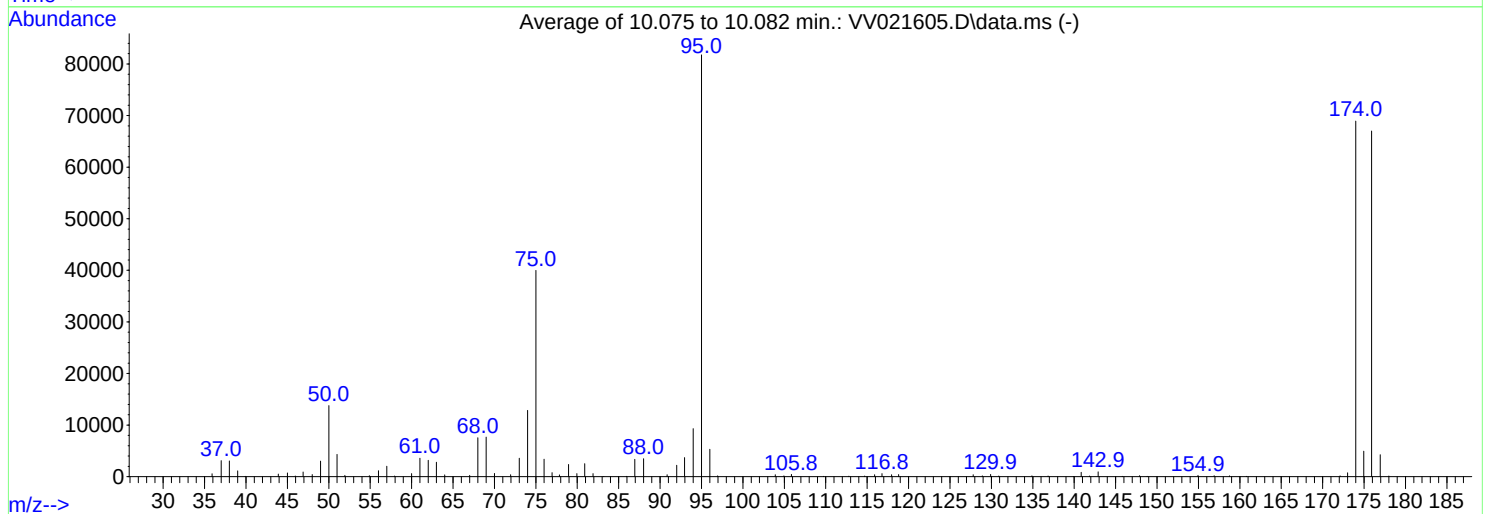


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VV070621\  
 Data File : VV021605.D  
 Acq On : 06 Jul 2021 09:05  
 Operator : SY/MD  
 Sample : BFB200  
 Misc : 5.0mL/MSVOA\_V/WATER  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 MSVOA\_V  
 ClientSampleId :  
 BFB200

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVLM062921WMA.M  
 Title : VOC Analysis  
 Last Update : Wed Jul 07 01:00:10 2021

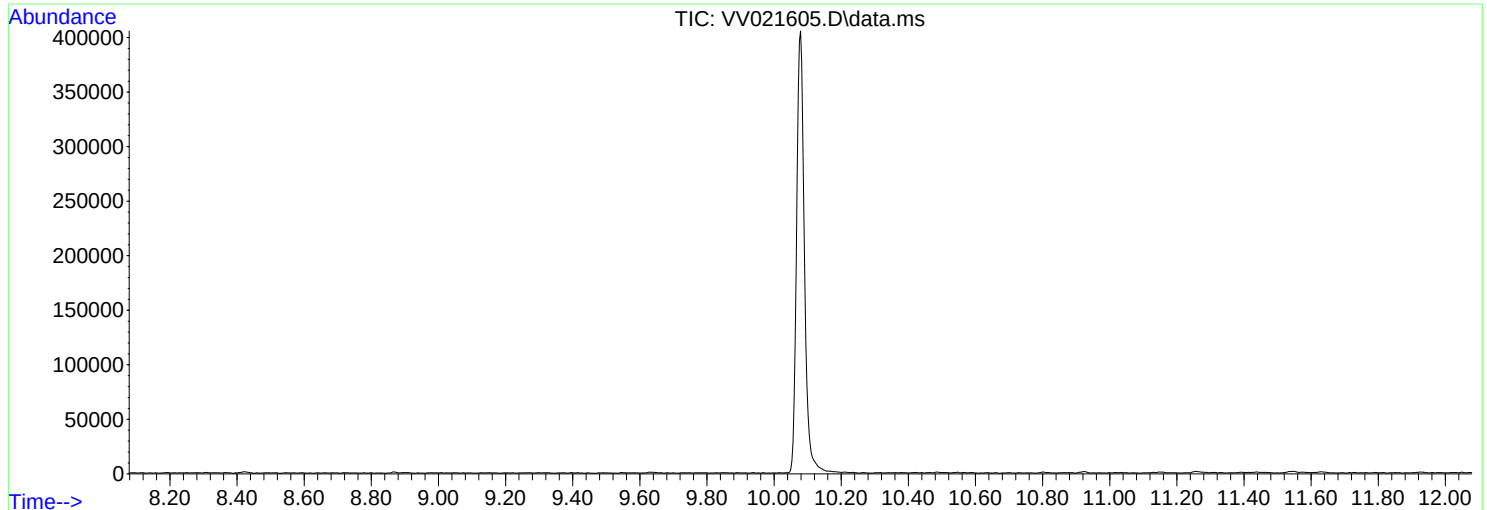

AutoFind: Scans 2810, 2811, 2812; Background Corrected with Scan 2798

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 50             | 95              | 15              | 40              | 16.9         | 13781      | PASS                |
| 75             | 95              | 30              | 80              | 48.9         | 39973      | PASS                |
| 95             | 95              | 100             | 100             | 100.0        | 81768      | PASS                |
| 96             | 95              | 5               | 9               | 6.5          | 5315       | PASS                |
| 173            | 174             | 0.00            | 2               | 1.1          | 745        | PASS                |
| 174            | 95              | 50              | 120             | 84.3         | 68936      | PASS                |
| 175            | 174             | 5               | 9               | 7.2          | 4943       | PASS                |
| 176            | 174             | 95              | 105             | 97.2         | 67003      | PASS                |
| 177            | 176             | 5               | 10              | 6.3          | 4242       | PASS                |

| m/z    | Abundance |
|--------|-----------|
| 35.90  | 560.0     |
| 37.00  | 3178.0    |
| 38.00  | 3157.0    |
| 39.00  | 1253.0    |
| 39.90  | 307.0     |
| 43.90  | 1063.0    |
| 45.00  | 737.0     |
| 46.00  | 130.0     |
| 46.90  | 908.0     |
| 48.00  | 435.0     |
| 49.00  | 3146.0    |
| 50.00  | 14245.0   |
| 51.00  | 4411.0    |
| 52.00  | 247.0     |
| 54.90  | 295.0     |
| 56.00  | 1201.0    |
| 57.00  | 2086.0    |
| 58.00  | 145.0     |
| 60.00  | 582.0     |
| 61.00  | 3669.0    |
| 62.00  | 3225.0    |
| 63.00  | 2923.0    |
| 64.00  | 369.0     |
| 67.00  | 245.0     |
| 68.00  | 7738.0    |
| 69.00  | 7900.0    |
| 70.00  | 648.0     |
| 71.90  | 373.0     |
| 73.00  | 3652.0    |
| 74.00  | 13132.0   |
| 75.00  | 41280.0   |
| 76.00  | 3462.0    |
| 77.00  | 839.0     |
| 77.90  | 331.0     |
| 78.90  | 2430.0    |
| 79.90  | 592.0     |
| 80.90  | 2570.0    |
| 81.90  | 620.0     |
| 83.20  | 111.0     |
| 85.90  | 104.0     |
| 86.90  | 3475.0    |
| 88.00  | 3594.0    |
| 90.90  | 400.0     |
| 92.00  | 2270.0    |
| 93.00  | 3835.0    |
| 94.00  | 9594.0    |
| 95.00  | 84416.0   |
| 96.00  | 5450.0    |
| 97.00  | 174.0     |
| 103.90 | 400.0     |
| 105.00 | 162.0     |
| 105.90 | 438.0     |
| 109.80 | 109.0     |
| 112.80 | 127.0     |
| 114.70 | 136.0     |
| 115.90 | 408.0     |
| 116.80 | 614.0     |
| 118.00 | 381.0     |
| 118.80 | 423.0     |
| 127.80 | 379.0     |
| 128.90 | 157.0     |
| 129.90 | 474.0     |
| 130.90 | 141.0     |
| 134.90 | 174.0     |
| 136.80 | 139.0     |
| 140.80 | 897.0     |
| 141.80 | 136.0     |
| 142.90 | 951.0     |
| 145.80 | 102.0     |
| 147.90 | 193.0     |
| 148.80 | 108.0     |
| 154.90 | 269.0     |
| 156.90 | 192.0     |
| 158.70 | 146.0     |
| 160.80 | 112.0     |
| 172.10 | 172.0     |
| 173.00 | 778.0     |
| 174.00 | 71032.0   |
| 175.00 | 5080.0    |
| 175.90 | 69128.0   |
| 177.00 | 4392.0    |
| 178.00 | 120.0     |

Instrument :  
MSVOA\_V  
ClientSampleId :  
BFB200

| m/z    | Abundance |
|--------|-----------|
| 35.90  | 488.0     |
| 37.00  | 3001.0    |
| 38.00  | 2881.0    |
| 39.00  | 1276.0    |
| 40.00  | 323.0     |
| 44.00  | 925.0     |
| 45.00  | 683.0     |
| 46.00  | 128.0     |
| 46.90  | 795.0     |
| 48.00  | 410.0     |
| 49.00  | 2821.0    |
| 50.00  | 12978.0   |
| 51.00  | 3955.0    |
| 52.00  | 280.0     |
| 54.90  | 284.0     |
| 56.00  | 1099.0    |
| 57.00  | 1750.0    |
| 57.90  | 141.0     |
| 60.00  | 616.0     |
| 61.00  | 3391.0    |
| 62.00  | 2976.0    |
| 63.00  | 2610.0    |
| 64.00  | 307.0     |
| 67.00  | 249.0     |
| 68.00  | 7216.0    |
| 69.00  | 7423.0    |
| 70.00  | 600.0     |
| 71.90  | 410.0     |
| 73.00  | 3413.0    |
| 74.00  | 11533.0   |
| 75.00  | 37944.0   |
| 76.00  | 3196.0    |
| 76.90  | 825.0     |
| 77.80  | 343.0     |
| 79.00  | 2349.0    |
| 80.00  | 548.0     |
| 80.90  | 2551.0    |
| 81.90  | 583.0     |
| 86.90  | 3359.0    |
| 88.00  | 3246.0    |
| 90.90  | 334.0     |
| 92.00  | 2061.0    |
| 92.90  | 3478.0    |
| 94.00  | 9017.0    |
| 95.00  | 77592.0   |
| 96.00  | 5000.0    |
| 96.90  | 163.0     |
| 103.90 | 379.0     |
| 105.00 | 148.0     |
| 105.80 | 415.0     |
| 109.70 | 112.0     |
| 112.80 | 136.0     |
| 114.70 | 120.0     |
| 115.90 | 348.0     |
| 116.80 | 597.0     |
| 118.00 | 317.0     |
| 118.80 | 332.0     |
| 127.80 | 387.0     |
| 128.90 | 130.0     |
| 129.90 | 349.0     |
| 130.90 | 140.0     |
| 134.90 | 127.0     |
| 136.90 | 139.0     |
| 140.90 | 844.0     |
| 141.90 | 128.0     |
| 142.90 | 877.0     |
| 147.90 | 194.0     |
| 148.80 | 114.0     |
| 154.90 | 240.0     |
| 156.90 | 167.0     |
| 158.80 | 136.0     |
| 160.80 | 112.0     |
| 172.10 | 147.0     |
| 173.00 | 704.0     |
| 174.00 | 67544.0   |
| 175.00 | 4765.0    |
| 175.90 | 65768.0   |
| 177.00 | 4072.0    |
| 178.00 | 122.0     |

Instrument :  
MSVOA\_V  
ClientSampleId :  
BFB200

| m/z   | Abundance |
|-------|-----------|
| 39.10 | 115.0     |
| 39.90 | 222.0     |
| 41.00 | 102.0     |
| 43.90 | 527.0     |
| 55.00 | 101.0     |

Instrument :  
MSVOA\_V  
ClientSampleId :  
BFB200

| m/z    | Abundance |
|--------|-----------|
| 35.90  | 584.0     |
| 37.00  | 3130.0    |
| 38.00  | 3090.0    |
| 39.00  | 1180.0    |
| 39.90  | 267.0     |
| 43.90  | 1061.0    |
| 45.00  | 721.0     |
| 45.90  | 149.0     |
| 46.90  | 977.0     |
| 48.00  | 410.0     |
| 49.00  | 3067.0    |
| 50.00  | 14119.0   |
| 51.00  | 4580.0    |
| 51.90  | 230.0     |
| 54.90  | 292.0     |
| 56.00  | 1175.0    |
| 57.00  | 2206.0    |
| 58.00  | 135.0     |
| 60.00  | 581.0     |
| 61.00  | 3690.0    |
| 62.00  | 3321.0    |
| 63.00  | 2896.0    |
| 64.00  | 341.0     |
| 67.00  | 221.0     |
| 68.00  | 7647.0    |
| 69.00  | 7641.0    |
| 70.00  | 637.0     |
| 72.00  | 349.0     |
| 73.00  | 3685.0    |
| 74.00  | 13835.0   |
| 75.00  | 40696.0   |
| 76.00  | 3497.0    |
| 77.00  | 690.0     |
| 77.90  | 317.0     |
| 78.90  | 2311.0    |
| 79.90  | 625.0     |
| 80.90  | 2414.0    |
| 81.90  | 575.0     |
| 86.00  | 122.0     |
| 87.00  | 3260.0    |
| 88.00  | 3608.0    |
| 90.80  | 421.0     |
| 92.00  | 2304.0    |
| 93.00  | 3752.0    |
| 94.00  | 9306.0    |
| 95.00  | 83296.0   |
| 96.00  | 5496.0    |
| 97.00  | 150.0     |
| 103.90 | 393.0     |
| 104.90 | 159.0     |
| 105.90 | 425.0     |
| 114.70 | 121.0     |
| 115.90 | 358.0     |
| 116.80 | 538.0     |
| 117.90 | 414.0     |
| 118.80 | 465.0     |
| 127.80 | 322.0     |
| 128.90 | 166.0     |
| 129.90 | 505.0     |
| 130.90 | 122.0     |
| 134.90 | 199.0     |
| 136.80 | 121.0     |
| 139.90 | 105.0     |
| 140.80 | 799.0     |
| 141.80 | 130.0     |
| 142.90 | 937.0     |
| 145.80 | 124.0     |
| 147.90 | 198.0     |
| 155.00 | 237.0     |
| 156.90 | 204.0     |
| 158.70 | 158.0     |
| 172.10 | 179.0     |
| 173.00 | 754.0     |
| 174.00 | 68232.0   |
| 174.90 | 4983.0    |
| 175.90 | 66112.0   |
| 176.90 | 4261.0    |
| 178.00 | 115.0     |

Instrument :  
MSVOA\_V  
ClientSampleId :  
BFB200