

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070622\
 Data File : VV026660.D
 Acq On : 06 Jul 2022 10:18
 Operator : SY/MD
 Sample : VV0706WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK389

Quant Time: Jul 07 01:16:50 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Jul 07 01:16:16 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.622	114	183128	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	177411	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	73649	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.320	65	68983	4.684	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	93.600%
7) Chloroethane-d5	1.581	69	58133	4.913	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	98.200%
11) 1,1-Dichloroethene-d2	2.121	63	94029	3.593	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	71.800%
20) 2-Butanone-d5	3.928	46	72232	49.332	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	98.660%
24) Chloroform-d	4.359	84	113838	4.728	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.600%
26) 1,2-Dichloroethane-d4	5.043	65	46274	4.990	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	99.800%
32) Benzene-d6	5.056	84	221887	4.354	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	87.000%
36) 1,2-Dichloropropane-d6	6.076	67	66997	4.781	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	95.600%
41) Toluene-d8	7.320	98	177081	3.864	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	77.200%
43) trans-1,3-Dichloroprop...	7.629	79	14110	3.895	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	78.000%
46) 2-Hexanone-d5	8.095	63	58547	42.436	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	84.880%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	44127	4.814	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	96.200%
66) 1,2-Dichlorobenzene-d4	11.622	152	58171	4.773	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	95.400%
Target Compounds						
16) Methylene chloride	2.523	84	5415	0.412	ug/L	Qvalue 95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070622\
Data File : VV026660.D
Acq On : 06 Jul 2022 10:18
Operator : SY/MD
Sample : VV0706WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK389


Quant Time: Jul 07 01:16:50 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Jul 07 01:16:16 2022
Response via : Initial Calibration

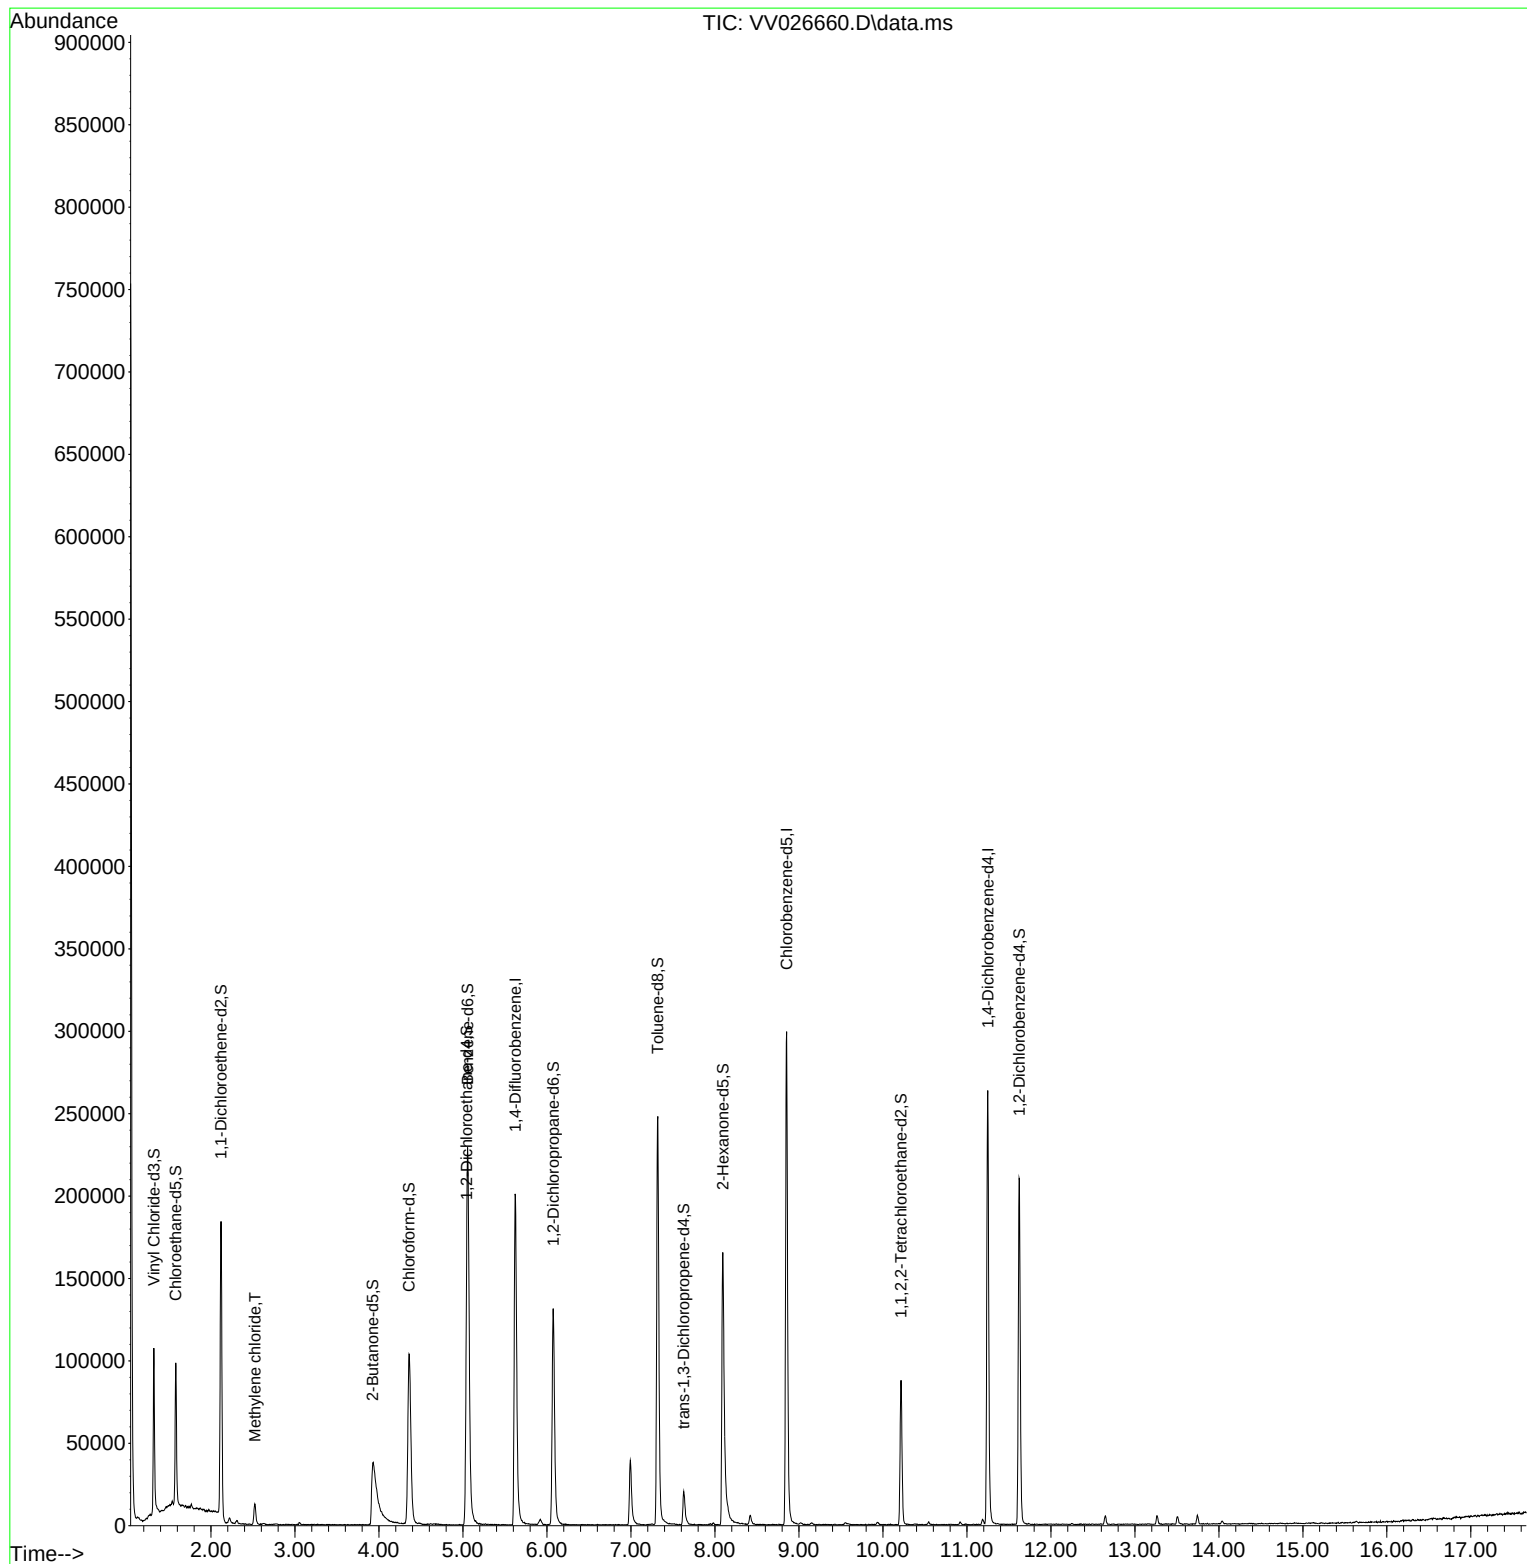

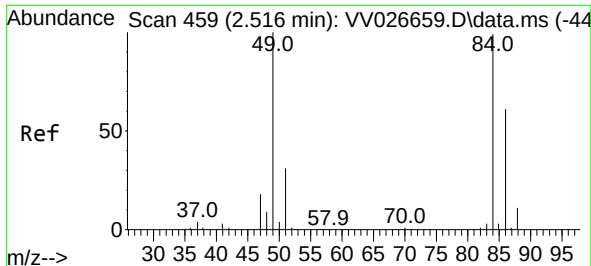

#16
Methylene chloride
Concen: 0.412 ug/L
RT: 2.523 min Scan# 41
Delta R.T. 0.006 min
Lab File: VV026660.D
Acq: 06 Jul 2022 10:18

Instrument :
MSVOA_V
ClientSampleId :
VBLK389

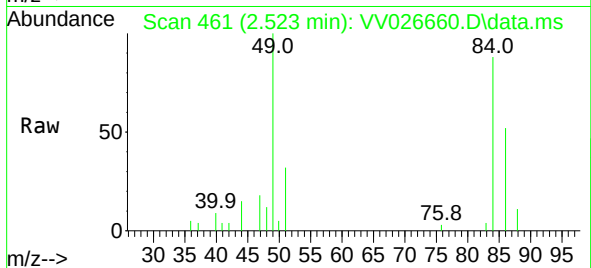

Tgt Ion: 84 Resp: 5415

Ion	Ratio	Lower	Upper
84	100		
86	59.3	46.0	85.4
49	113.9	77.7	144.3

