

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW070622\
 Data File : VW026664.D
 Acq On : 06 Jul 2022 13:42
 Operator : SY/MD
 Sample : N3598-06
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COAN5

Manual Integrations
 APPROVED

Reviewed By :Krupa Patel 07/07/2022
 Supervised By :Mahesh Dadoda 07/07/2022

Quant Time: Jul 07 01:17:41 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Jul 07 01:16:16 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.622	114	211813	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	205185	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	84704	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.317	65	68119	3.999	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	80.000%
7) Chloroethane-d5	1.580	69	57080	4.171	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	83.400%
11) 1,1-Dichloroethene-d2	2.117	63	96303	3.182	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	63.600%
20) 2-Butanone-d5	3.918	46	88865	52.473	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	104.940%
24) Chloroform-d	4.358	84	115620	4.152	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	83.000%
26) 1,2-Dichloroethane-d4	5.040	65	46080	4.296	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	86.000%
32) Benzene-d6	5.059	84	222566	3.776	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	75.600%
36) 1,2-Dichloropropane-d6	6.075	67	68221	4.209	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	84.200%
41) Toluene-d8	7.320	98	174578	3.294	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	65.800%#
43) trans-1,3-Dichloroprop...	7.628	79	17418	4.158	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	83.200%
46) 2-Hexanone-d5	8.091	63	71021	44.509	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	89.020%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	43295	4.084	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	81.600%
66) 1,2-Dichlorobenzene-d4	11.622	152	57965	4.135	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	82.800%
Target Compounds						Qvalue
3) Chloromethane	1.252	50	312436	17.713	ug/L	99
5) Vinyl chloride	1.323	62	137662	7.330	ug/L	97
6) Bromomethane	1.539	94	2602	0.256	ug/L	87
12) 1,1-Dichloroethene	2.127	96	5921	0.414	ug/L #	1
13) Acetone	2.214	43	12168m	11.326	ug/L	
14) Carbon disulfide	2.307	76	5516	0.146	ug/L	97
17) Methyl tert-butyl Ether	2.786	73	27679	1.187	ug/L #	84
18) trans-1,2-Dichloroethene	2.773	96	19268	1.320	ug/L	95
19) 1,1-Dichloroethane	3.201	63	5841	0.223	ug/L	95
22) cis-1,2-Dichloroethene	3.921	96	471120	32.506	ug/L	96
23) Bromochloromethane	4.272	128	1391	0.233	ug/L	86
25) Chloroform	4.387	83	57495	2.051	ug/L	94
33) Benzene	5.117	78	8841	0.148	ug/L	100
34) Trichloroethene	5.918	95	418496	26.571	ug/L	97
37) 1,2-Dichloropropane	6.188	63	6543	0.453	ug/L #	95
38) Bromodichloromethane	6.516	83	41251	2.420	ug/L	95
42) Toluene	7.390	91	535367	8.656	ug/L	100
47) Tetrachloroethene	7.976	164	1715659	136.818	ug/L	99
49) Dibromochloromethane	8.249	129	46033m	4.993	ug/L	

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070622\
 Data File : VV026664.D
 Acq On : 06 Jul 2022 13:42
 Operator : SY/MD
 Sample : N3598-06
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AN5


Manual Integrations
 APPROVED

Reviewed By :Krupa Patel 07/07/2022
 Supervised By :Mahesh Dadoda 07/07/2022

Quant Time: Jul 07 01:17:41 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Jul 07 01:16:16 2022
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
52) Ethylbenzene	9.017	91	18597	0.291	ug/L	97
53) m,p-Xylene	9.146	106	3004	0.120	ug/L	94
54) o-Xylene	9.545	106	2568	0.110	ug/L	97
59) Bromoform	9.731	173	17372	5.565	ug/L	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

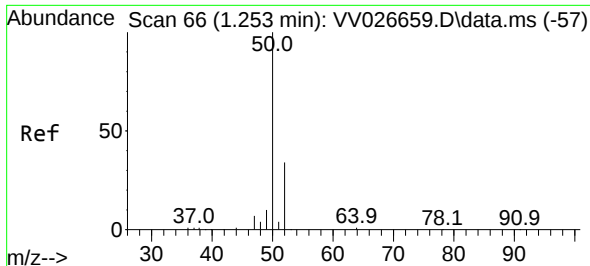

#3
Chloromethane
Concen: 17.713 ug/L
RT: 1.252 min Scan# 60
Delta R.T. -0.000 min
Lab File: VV026664.D
Acq: 06 Jul 2022 13:42




Instrument :
MSVOA_V
ClientSampleId :
COAN5

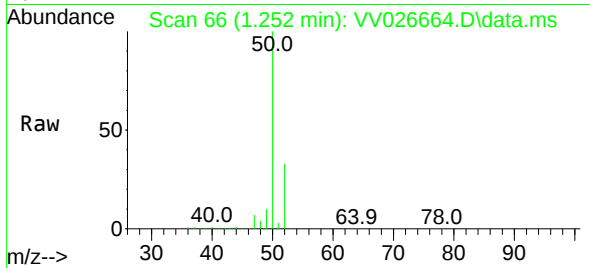


Tgt Ion: 50 Resp: 312430
Ion Ratio Lower Upper
50 100
52 33.3 23.0 42.6

Manual Integrations
APPROVED



Reviewed By :Krupa Patel 07/07/2022
Supervised By :Mahesh Dadoda 07/07/2022

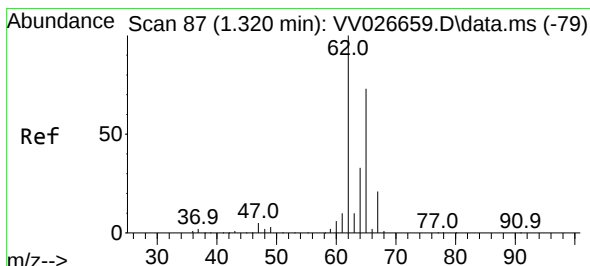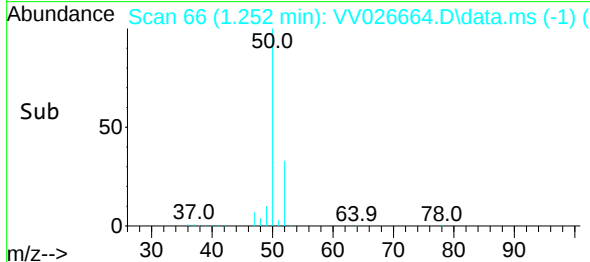


#5
Vinyl chloride
Concen: 7.330 ug/L
RT: 1.323 min Scan# 88
Delta R.T. 0.003 min
Lab File: VV026664.D
Acq: 06 Jul 2022 13:42

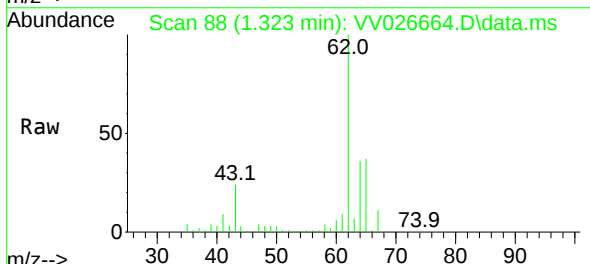


Tgt Ion: 62 Resp: 137662
Ion Ratio Lower Upper
62 100
64 35.8 26.2 48.6

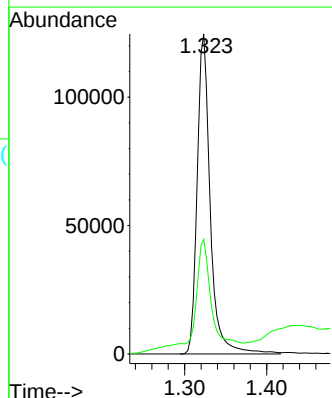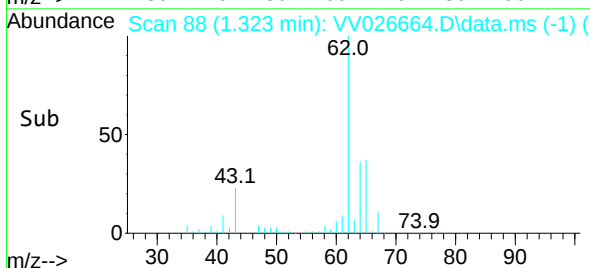

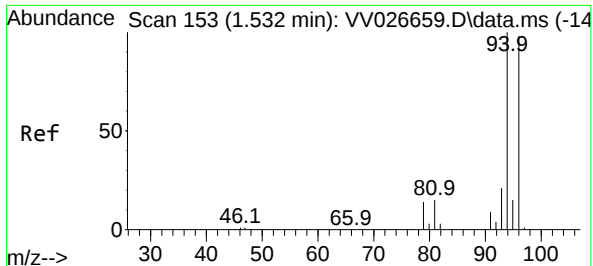

#6
Bromomethane
Concen: 0.256 ug/L
RT: 1.539 min Scan# 153
Delta R.T. 0.006 min
Lab File: VV026664.D
Acq: 06 Jul 2022 13:42




Instrument :
MSVOA_V
ClientSampleId :
COAN5

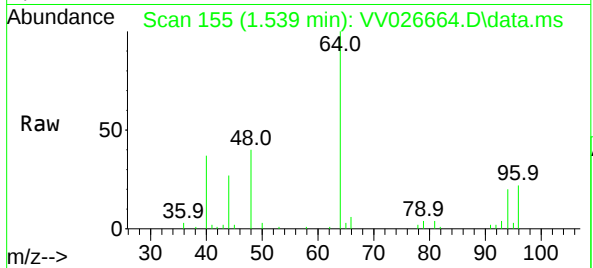

Tgt Ion: 94 Resp: 2602
Ion Ratio Lower Upper
94 100
96 109.5 68.0 126.2




Manual Integrations
APPROVED


Reviewed By :Krupa Patel 07/07/2022
Supervised By :Mahesh Dadoda 07/07/2022

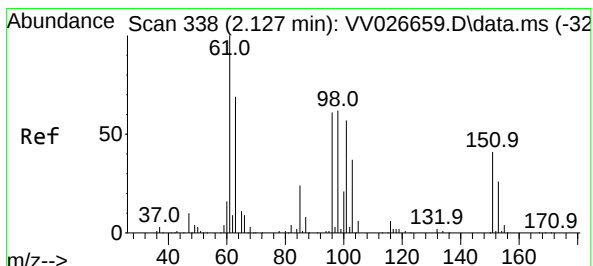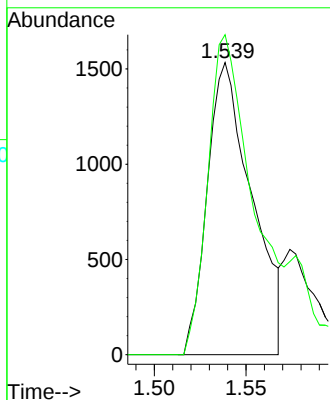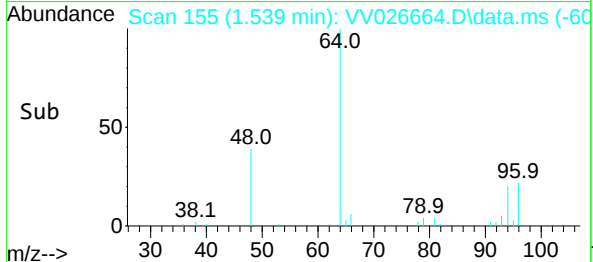

#12
1,1-Dichloroethene
Concen: 0.414 ug/L
RT: 2.127 min Scan# 338
Delta R.T. -0.000 min
Lab File: VV026664.D
Acq: 06 Jul 2022 13:42

Tgt Ion: 96 Resp: 5921
Ion Ratio Lower Upper
96 100
61 269.2 115.4 214.4#
63 1130.1 87.4 162.2#

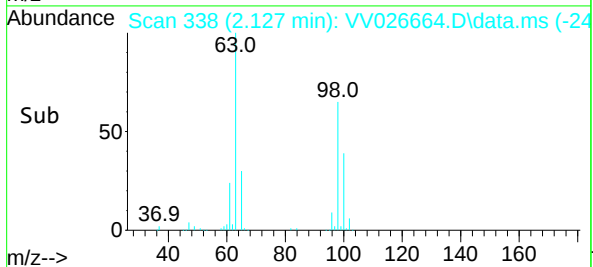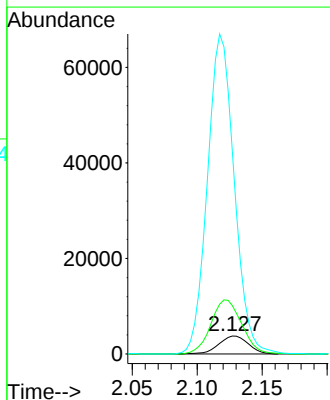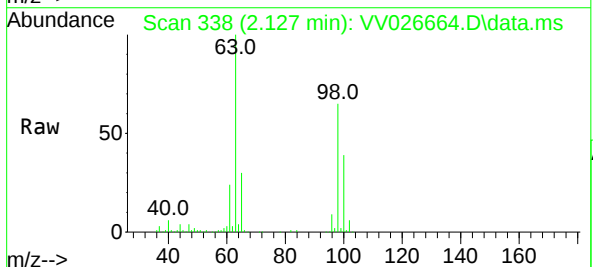



#13

Acetone

Concen: 11.326 ug/L m

RT: 2.214 min Scan# 3

Delta R.T. 0.006 min

Lab File: VV026664.D

Acq: 06 Jul 2022 13:42

Instrument :

MSVOA_V

ClientSampleId :

COAN5

Tgt Ion: 43 Resp: 1216

Ion Ratio Lower Upper

43 100





58 22.5 0.0 75.0

Manual Integrations

APPROVED

Reviewed By :Krupa Patel 07/07/2022

Supervised By :Mahesh Dadoda 07/07/2022

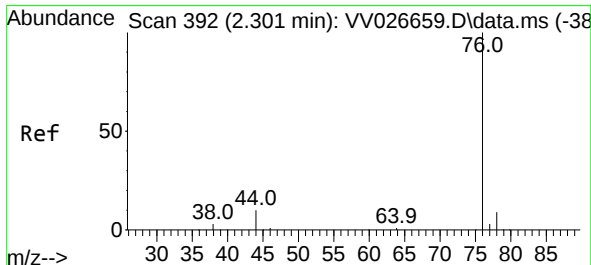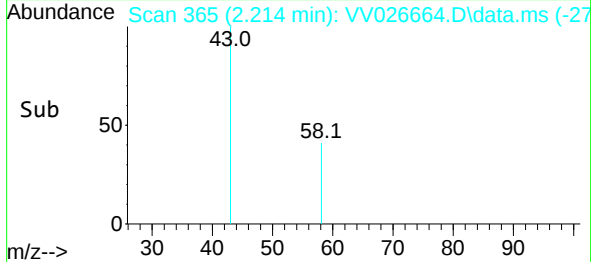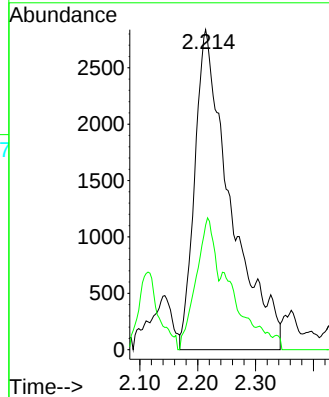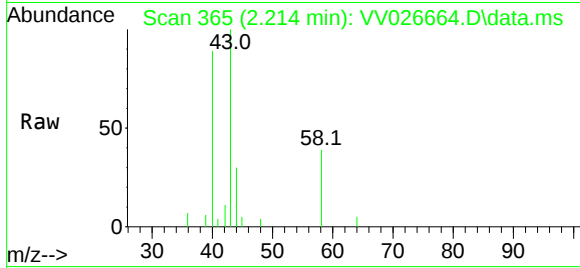

#14

Carbon disulfide

Concen: 0.146 ug/L

RT: 2.307 min Scan# 394

Delta R.T. 0.006 min

Lab File: VV026664.D




Acq: 06 Jul 2022 13:42


Tgt Ion: 76 Resp: 5516

Ion Ratio Lower Upper

76 100

78 10.7 7.8 11.6

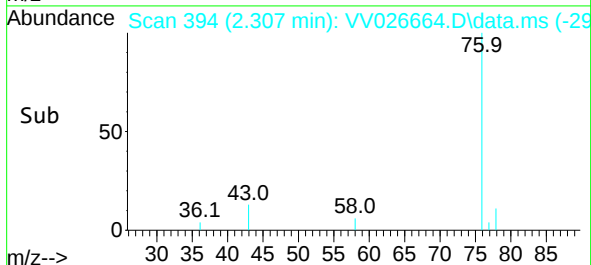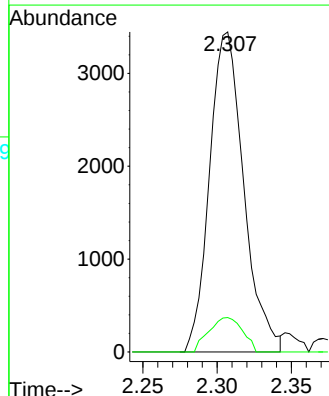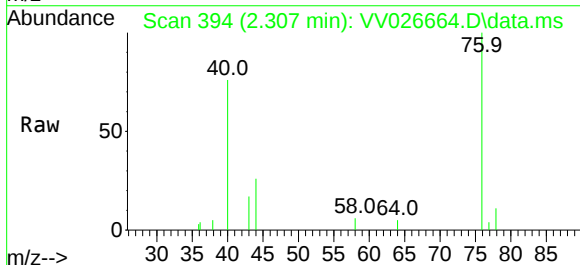







#17
Methyl tert-butyl Ether
Concen: 1.187 ug/L
RT: 2.786 min Scan# 54
Delta R.T. 0.003 min
Lab File: VV026664.D
Acq: 06 Jul 2022 13:42

Instrument :
MSVOA_V
ClientSampleId :
COAN5

Tgt Ion: 73 Resp: 27679
Ion Ratio Lower Upper
73 100
43 21.3 13.3 19.9
57 30.6 17.2 25.8




Manual Integrations
APPROVED


Reviewed By :Krupa Patel 07/07/2022
Supervised By :Mahesh Dadoda 07/07/2022

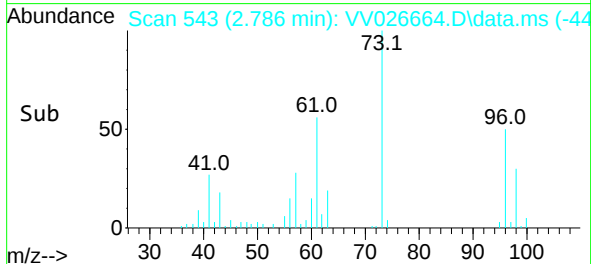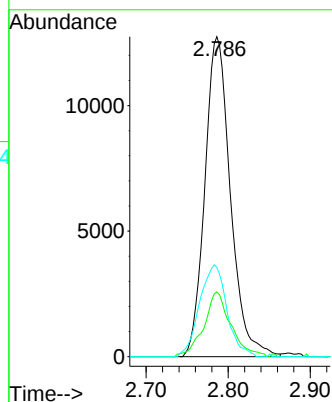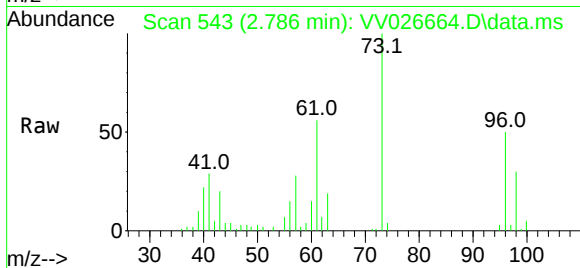

#18
trans-1,2-Dichloroethene
Concen: 1.320 ug/L
RT: 2.773 min Scan# 539
Delta R.T. 0.003 min
Lab File: VV026664.D
Acq: 06 Jul 2022 13:42

Tgt Ion: 96 Resp: 19268
Ion Ratio Lower Upper
96 100
61 121.9 90.4 167.8
98 67.2 45.6 84.8

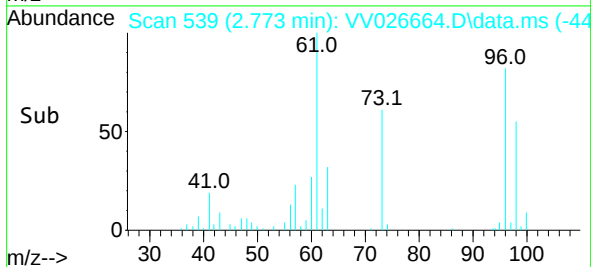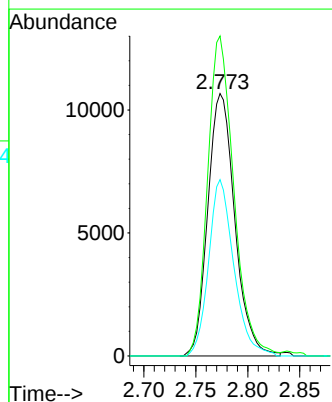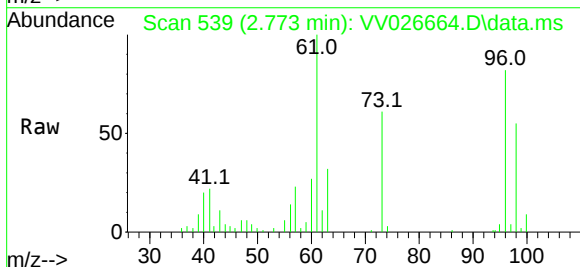

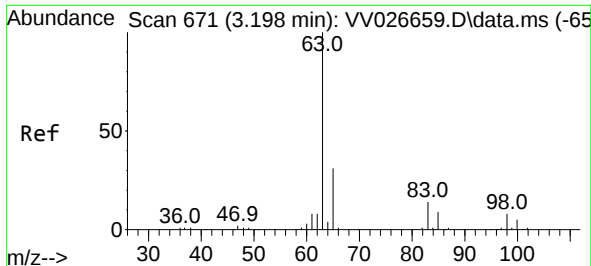





#19
1,1-Dichloroethane
Concen: 0.223 ug/L
RT: 3.201 min Scan# 61
Delta R.T. 0.003 min
Lab File: VV026664.D
Acq: 06 Jul 2022 13:42

Instrument :
MSVOA_V
ClientSampleId :
COAN5

Tgt Ion: 63 Resp: 584
Ion Ratio Lower Upper
63 100
65 29.1 23.0 42.6
83 14.4 10.2 19.0




Manual Integrations
APPROVED


Reviewed By :Krupa Patel 07/07/2022
Supervised By :Mahesh Dadoda 07/07/2022

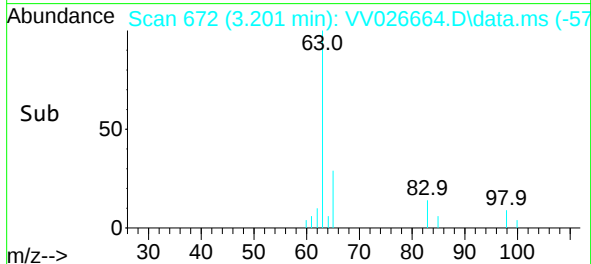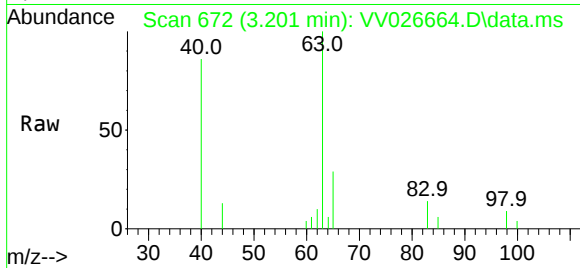

#22
cis-1,2-Dichloroethene
Concen: 32.506 ug/L
RT: 3.921 min Scan# 896
Delta R.T. -0.000 min
Lab File: VV026664.D
Acq: 06 Jul 2022 13:42


Tgt Ion: 96 Resp: 471120
Ion Ratio Lower Upper
96 100
61 113.1 82.0 152.2
68 0.0 0.0 0.0

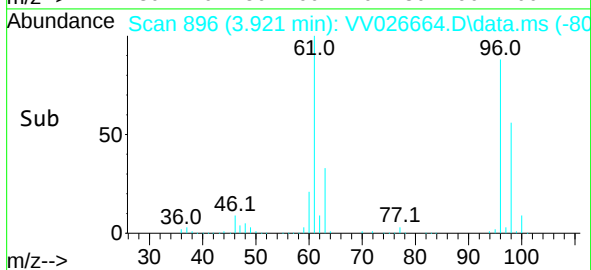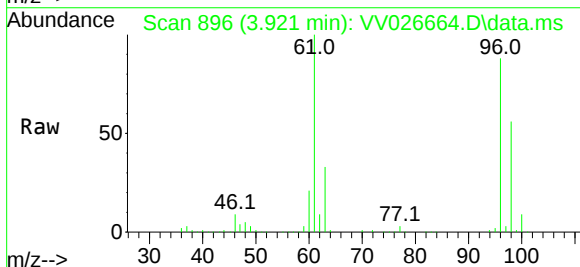

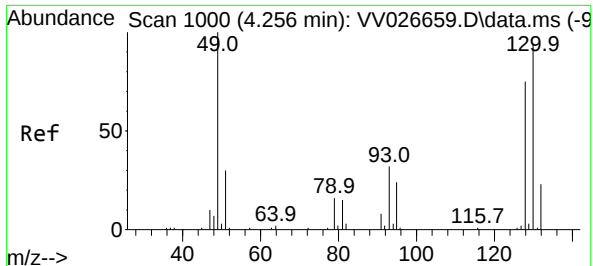

#23
Bromochloromethane
Concen: 0.233 ug/L
RT: 4.272 min Scan# 1005
Delta R.T. 0.016 min
Lab File: VV026664.D
Acq: 06 Jul 2022 13:42




Instrument :
MSVOA_V
ClientSampleId :
COAN5

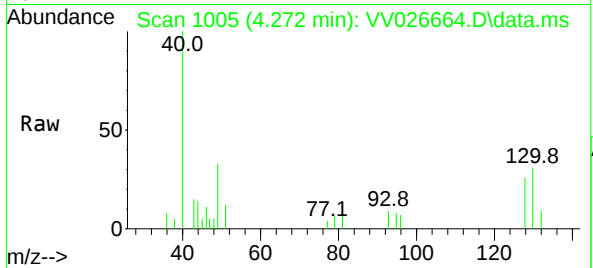

Tgt Ion:128 Resp: 139
Ion Ratio Lower Upper
128 100
49 124.1 104.0 193.1
130 119.3 93.4 173.6
51 46.8 38.4 57.6




Manual Integrations
APPROVED


Reviewed By :Krupa Patel 07/07/2022
Supervised By :Mahesh Dadoda 07/07/2022

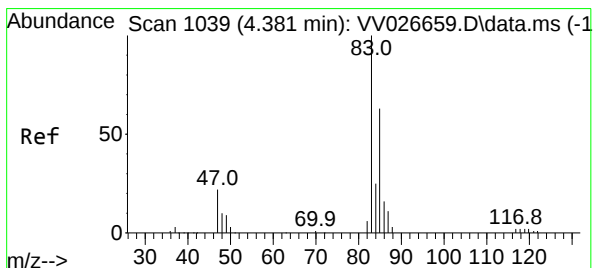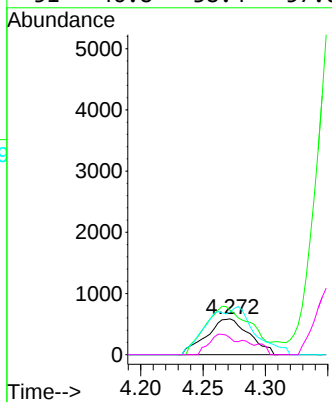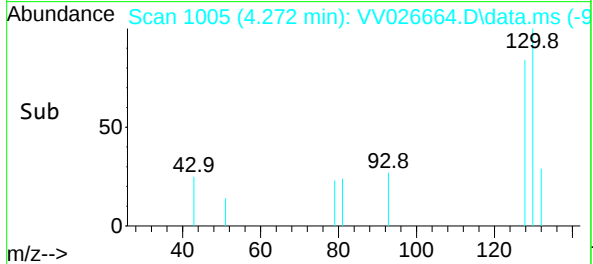

#25
Chloroform
Concen: 2.051 ug/L
RT: 4.387 min Scan# 1041
Delta R.T. 0.006 min
Lab File: VV026664.D
Acq: 06 Jul 2022 13:42

Tgt Ion: 83 Resp: 57495
Ion Ratio Lower Upper
83 100
85 67.8 44.0 81.8

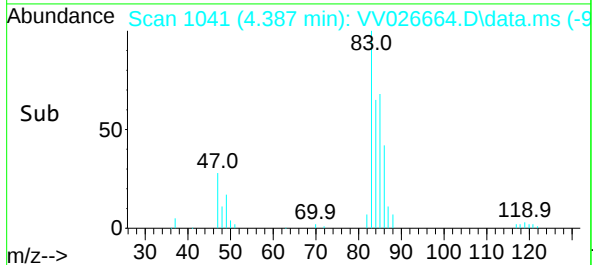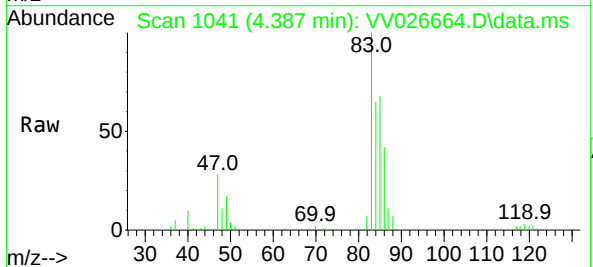







#33
Benzene
Concen: 0.148 ug/L
RT: 5.117 min Scan# 11
Delta R.T. 0.013 min
Lab File: VV026664.D
Acq: 06 Jul 2022 13:42

Instrument :
MSVOA_V
ClientSampleId :
COAN5

Tgt Ion: 78 Resp: 884

Manual Integrations
APPROVED




Reviewed By :Krupa Patel 07/07/2022
Supervised By :Mahesh Dadoda 07/07/2022

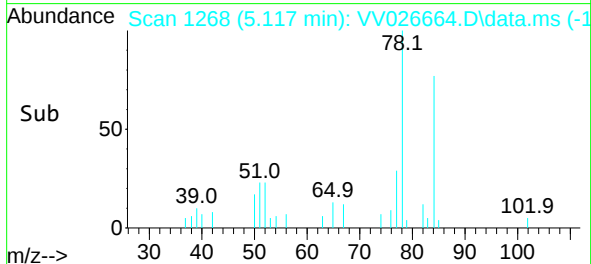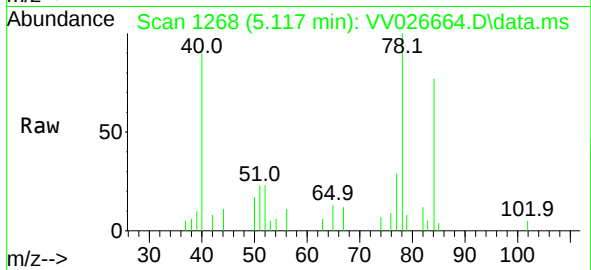


#34
Trichloroethene
Concen: 26.571 ug/L
RT: 5.918 min Scan# 1517
Delta R.T. 0.003 min
Lab File: VV026664.D
Acq: 06 Jul 2022 13:42

Tgt Ion: 95 Resp: 418496

Ion	Ratio	Lower	Upper
95	100		
97	63.8	46.8	87.0
132	101.5	69.9	129.7
130	106.0	72.0	133.8

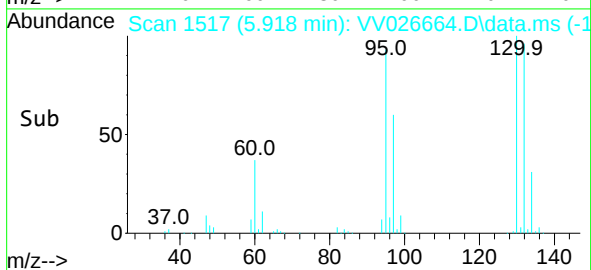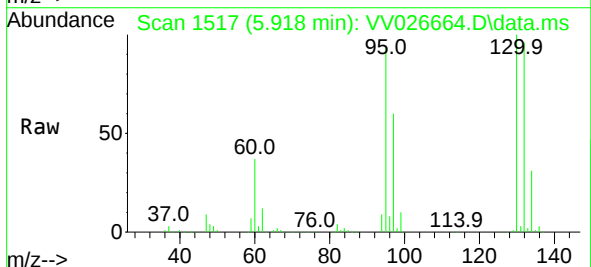







#37
1,2-Dichloropropane
Concen: 0.453 ug/L
RT: 6.188 min Scan# 1103
Delta R.T. 0.013 min
Lab File: VV026664.D
Acq: 06 Jul 2022 13:42

Instrument :
MSVOA_V
ClientSampleId :
COAN5

Tgt Ion: 63 Resp: 654
Ion Ratio Lower Upper
63 100
112 3.7 4.2 6.4




Manual Integrations
APPROVED


Reviewed By :Krupa Patel 07/07/2022
Supervised By :Mahesh Dadoda 07/07/2022

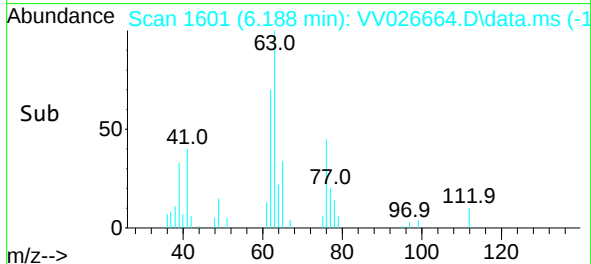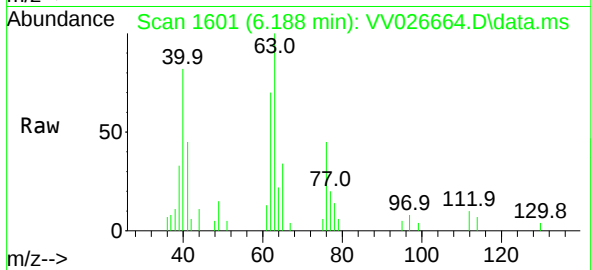

#38
Bromodichloromethane
Concen: 2.420 ug/L
RT: 6.516 min Scan# 1703
Delta R.T. 0.003 min
Lab File: VV026664.D
Acq: 06 Jul 2022 13:42


Tgt Ion: 83 Resp: 41251
Ion Ratio Lower Upper
83 100
85 67.1 44.0 81.8
127 9.0 6.6 10.0

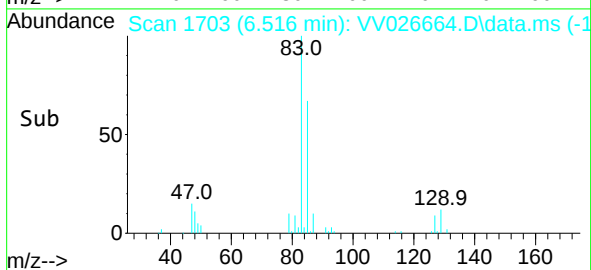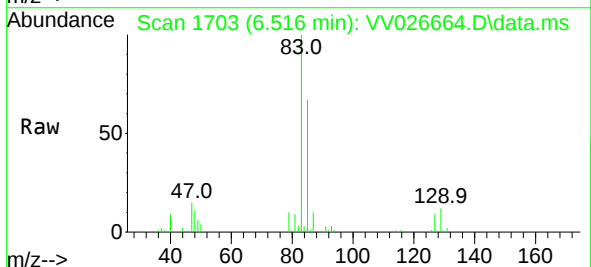

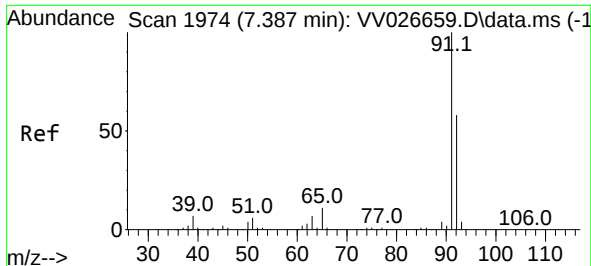

#42
Toluene
Concen: 8.656 ug/L
RT: 7.390 min Scan# 1974
Delta R.T. 0.003 min
Lab File: VV026664.D
Acq: 06 Jul 2022 13:42




Instrument :
MSVOA_V
ClientSampleId :
C0AN5



Tgt Ion: 91 Resp: 53536
Ion Ratio Lower Upper
91 100
92 57.9 40.3 74.9




Manual Integrations
APPROVED


Reviewed By :Krupa Patel 07/07/2022
Supervised By :Mahesh Dadoda 07/07/2022

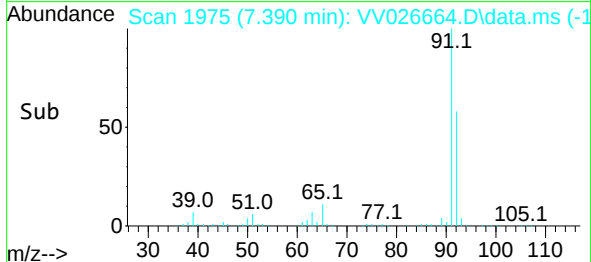

#47
Tetrachloroethene
Concen: 136.818 ug/L
RT: 7.976 min Scan# 2157
Delta R.T. -0.000 min
Lab File: VV026664.D
Acq: 06 Jul 2022 13:42


Tgt Ion:164 Resp: 1715659
Ion Ratio Lower Upper
164 100
129 96.5 66.4 123.2
131 92.6 64.4 119.6
166 126.2 88.1 163.7

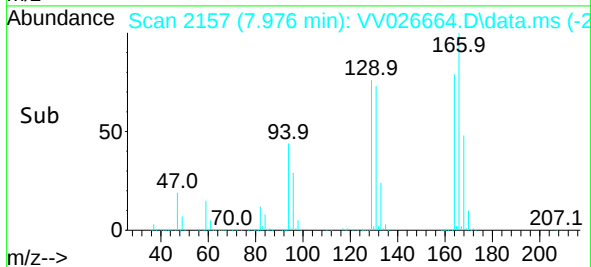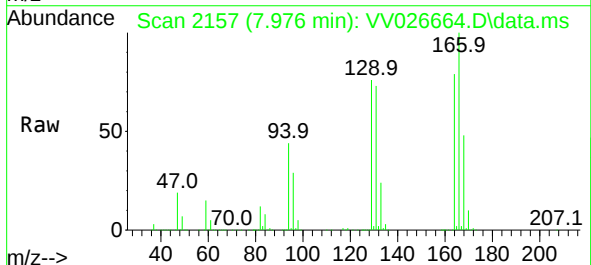

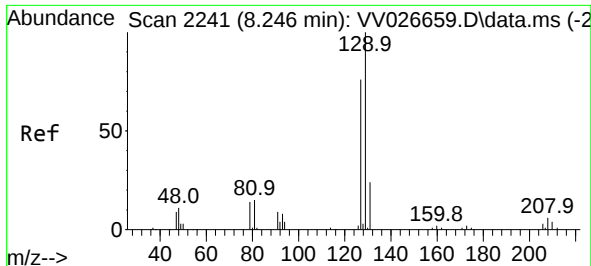

#49
Dibromochloromethane
Concen: 4.993 ug/L m
RT: 8.249 min Scan# 21
Delta R.T. 0.003 min
Lab File: VV026664.D
Acq: 06 Jul 2022 13:42




Instrument :
MSVOA_V
ClientSampleId :
COAN5




Tgt Ion:129 Resp: 4603
Ion Ratio Lower Upper
129 100
127 80.0 54.2 100.6

Manual Integrations
APPROVED



Reviewed By :Krupa Patel 07/07/2022
Supervised By :Mahesh Dadoda 07/07/2022

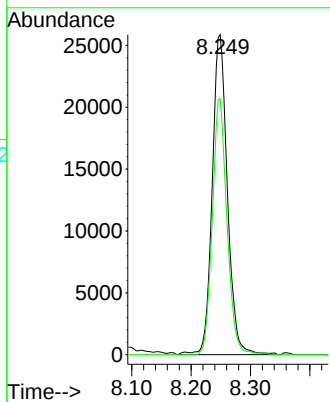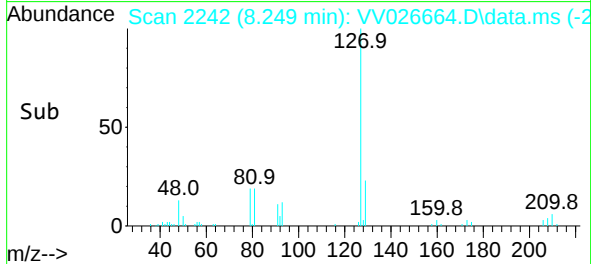


#52
Ethylbenzene
Concen: 0.291 ug/L
RT: 9.017 min Scan# 2481
Delta R.T. 0.006 min
Lab File: VV026664.D
Acq: 06 Jul 2022 13:42

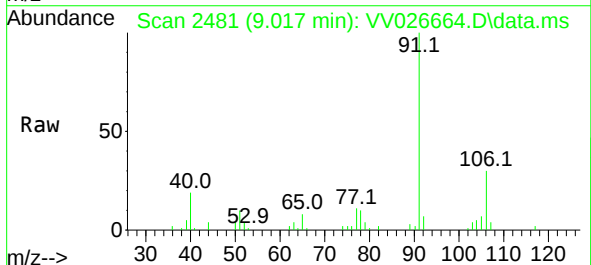


Tgt Ion: 91 Resp: 18597
Ion Ratio Lower Upper
91 100
106 29.9 22.1 41.1

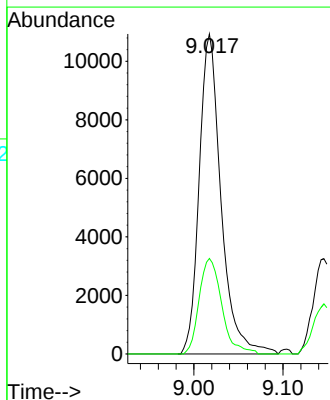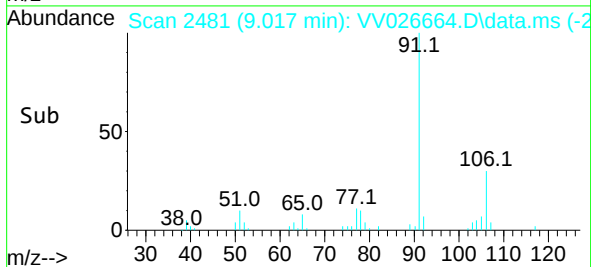



#53
m,p-Xylene
Concen: 0.120 ug/L
RT: 9.146 min Scan# 21
Delta R.T. 0.009 min
Lab File: VV026664.D
Acq: 06 Jul 2022 13:42




Instrument :
MSVOA_V
ClientSampleId :
C0AN5



Tgt Ion:106 Resp: 3004
Ion Ratio Lower Upper
106 100
91 190.2 139.9 259.9




Manual Integrations
APPROVED


Reviewed By :Krupa Patel 07/07/2022
Supervised By :Mahesh Dadoda 07/07/2022

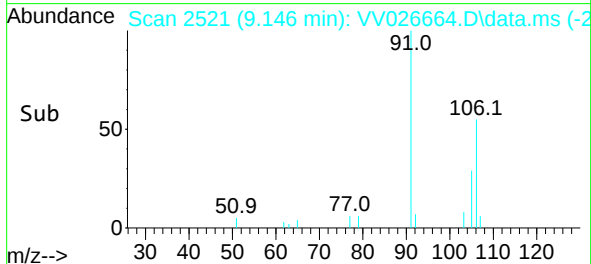

#54
o-Xylene
Concen: 0.110 ug/L
RT: 9.545 min Scan# 2645
Delta R.T. 0.003 min
Lab File: VV026664.D
Acq: 06 Jul 2022 13:42

Tgt Ion:106 Resp: 2568
Ion Ratio Lower Upper
106 100
91 206.1 147.5 273.9

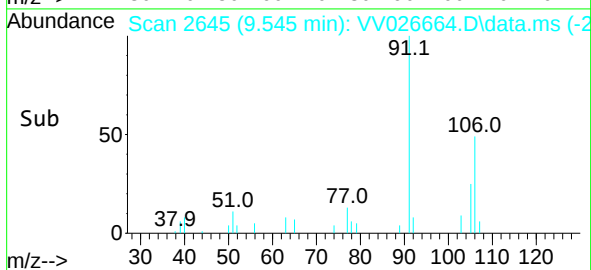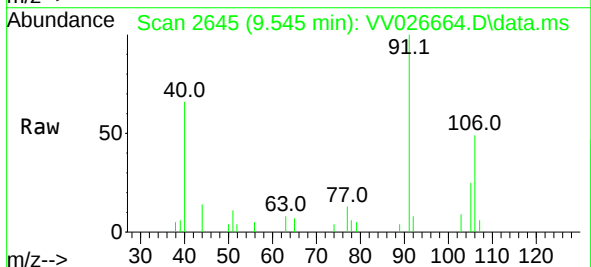

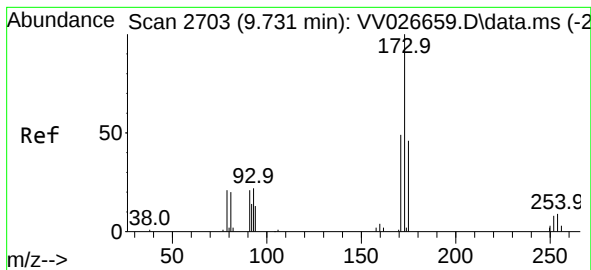

#59

Bromoform

Concen: 5.565 ug/L

RT: 9.731 min Scan# 21

Delta R.T. -0.000 min

Lab File: VV026664.D

Acq: 06 Jul 2022 13:42

Instrument :

MSVOA_V

ClientSampleId :

C0AN5

Tgt Ion:173 Resp: 1737

Ion Ratio Lower Upper

173 100

175 49.6 37.9 56.9

254 7.9 6.3 9.5

Manual Integrations

APPROVED

Reviewed By :Krupa Patel 07/07/2022

Supervised By :Mahesh Dadoda 07/07/2022

