

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070622\
 Data File : VV026666.D
 Acq On : 06 Jul 2022 15:19
 Operator : SY/MD
 Sample : N3598-06DL 20X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AN5DL

Quant Time: Jul 07 01:18:10 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Jul 07 01:16:16 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.622	114	181348	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	177840	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	71352	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.317	65	65824	4.513	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	90.200%
7) Chloroethane-d5	1.580	69	55244	4.715	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	94.400%
11) 1,1-Dichloroethene-d2	2.117	63	89331	3.447	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	69.000%
20) 2-Butanone-d5	3.915	46	74679	51.504	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	103.000%
24) Chloroform-d	4.358	84	111014	4.656	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	93.200%
26) 1,2-Dichloroethane-d4	5.040	65	43359	4.722	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	94.400%
32) Benzene-d6	5.056	84	209596	4.103	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	82.000%
36) 1,2-Dichloropropane-d6	6.075	67	63953	4.553	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	91.000%
41) Toluene-d8	7.316	98	161815	3.523	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	70.400%
43) trans-1,3-Dichloroprop...	7.628	79	14091	3.881	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	77.600%
46) 2-Hexanone-d5	8.091	63	53908	38.979	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	77.960%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	40585	4.417	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	88.400%
66) 1,2-Dichlorobenzene-d4	11.625	152	52273	4.427	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	88.600%
Target Compounds						
					Qvalue	
3) Chloromethane	1.252	50	1533	0.102	ug/L #	65
5) Vinyl chloride	1.323	62	4779	0.297	ug/L #	1
16) Methylene chloride	2.519	84	18506	1.423	ug/L	96
18) trans-1,2-Dichloroethene	2.783	96	682	0.055	ug/L #	66
22) cis-1,2-Dichloroethene	3.928	96	13645	1.100	ug/L	98
25) Chloroform	4.384	83	6191	0.258	ug/L	100
34) Trichloroethene	5.924	95	12740	0.933	ug/L	93
38) Bromodichloromethane	6.519	83	1794	0.121	ug/L #	95
42) Toluene	7.397	91	18267	0.341	ug/L	90
47) Tetrachloroethene	7.976	164	49225	4.529	ug/L	98
49) Dibromochloromethane	8.249	129	2193	0.274	ug/L	80
59) Bromoform	9.734	173	722	0.275	ug/L #	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070622\
Data File : VV026666.D
Acq On : 06 Jul 2022 15:19
Operator : SY/MD
Sample : N3598-06DL 20X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AN5DL

Quant Time: Jul 07 01:18:10 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Jul 07 01:16:16 2022
Response via : Initial Calibration




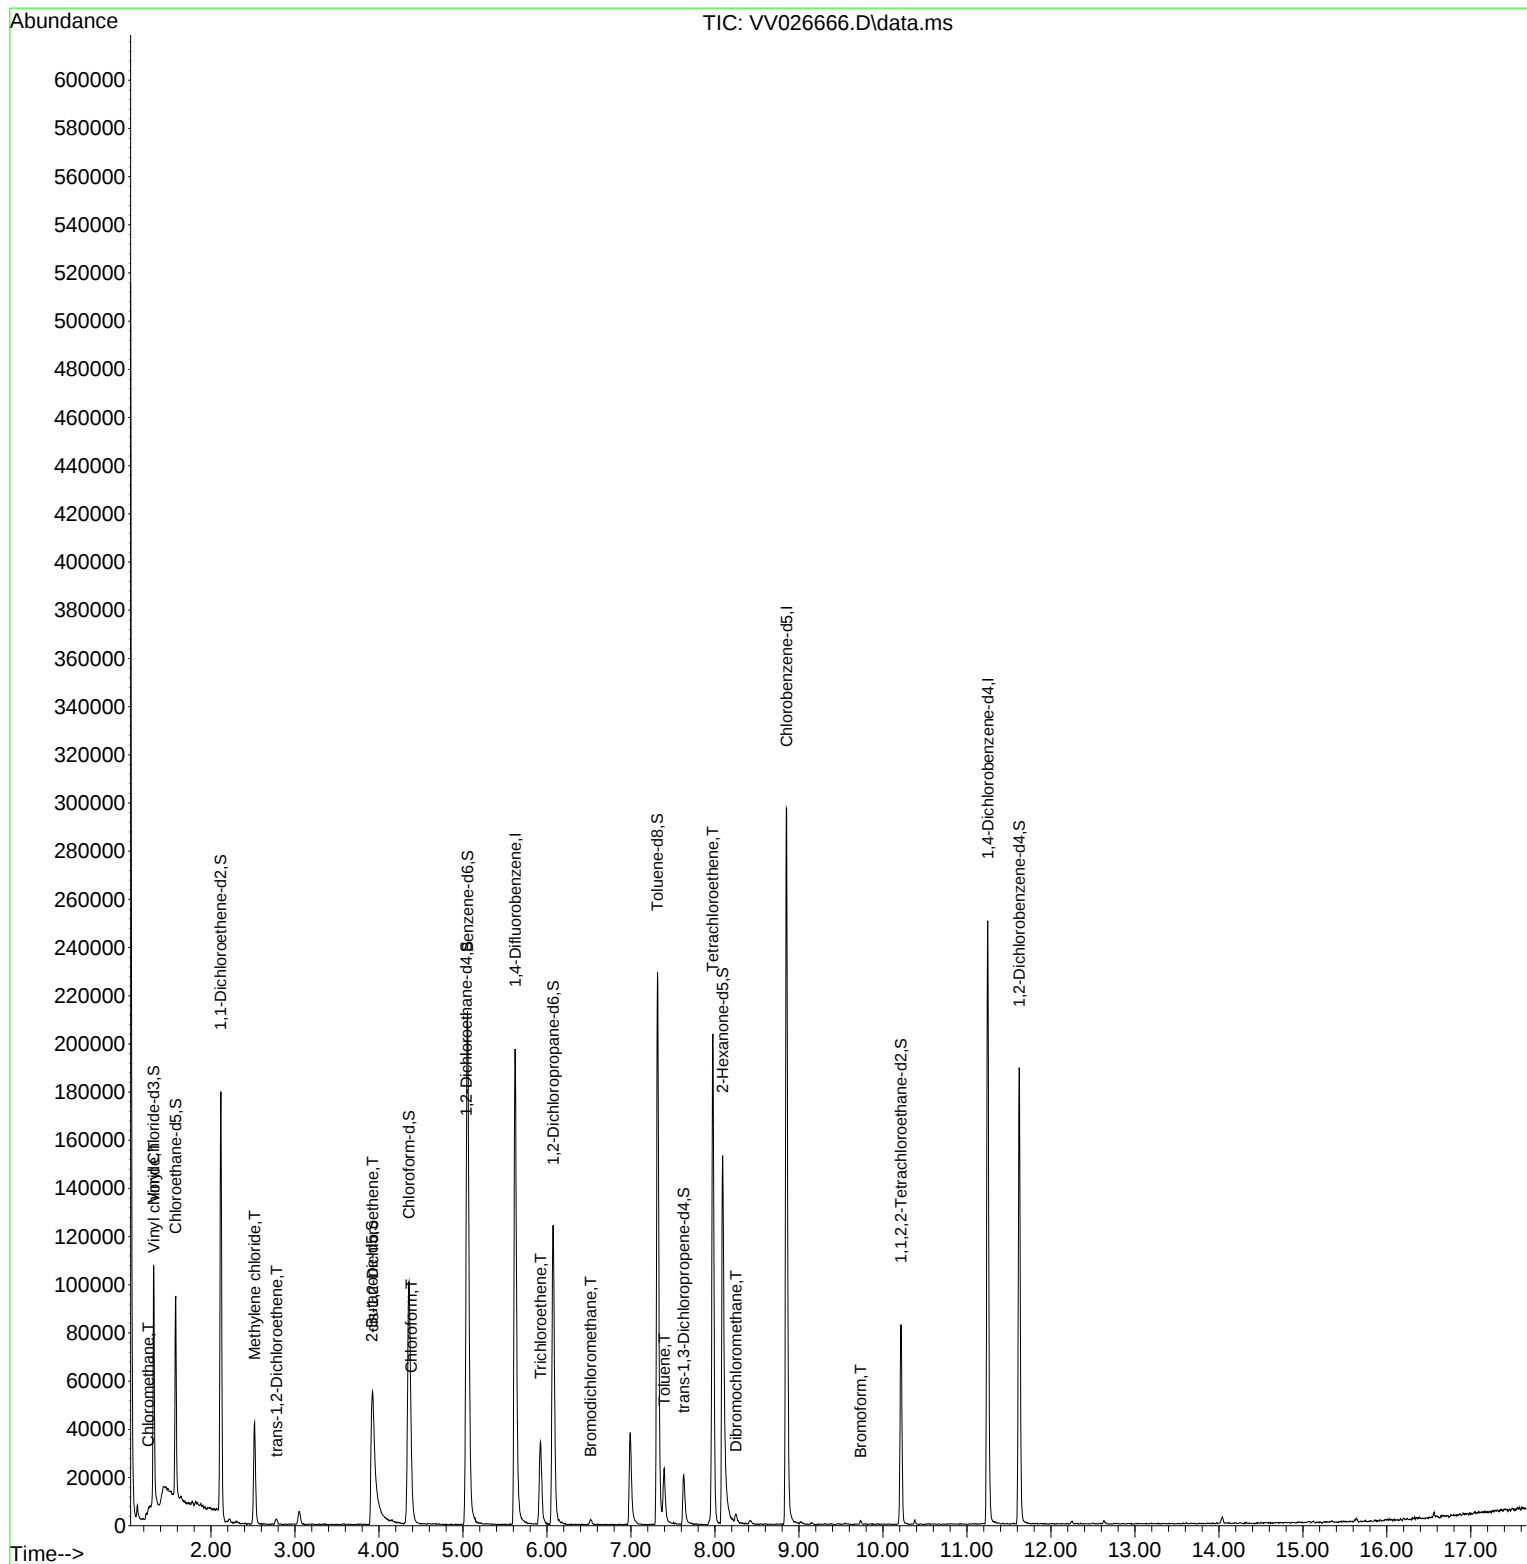


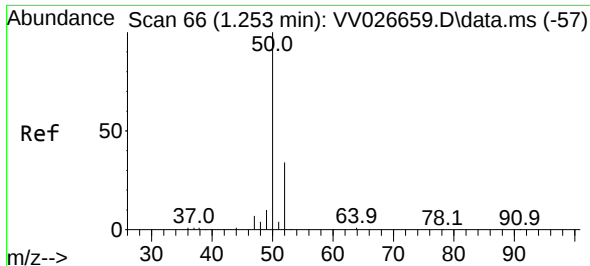

#3
Chloromethane
Concen: 0.102 ug/L
RT: 1.252 min Scan# 60
Delta R.T. -0.000 min
Lab File: VV026666.D
Acq: 06 Jul 2022 15:19




Instrument :
MSVOA_V
ClientSampleId :
C0AN5DL


Tgt Ion: 50 Resp: 1533
Ion Ratio Lower Upper
50 100
52 52.3 23.0 42.6#

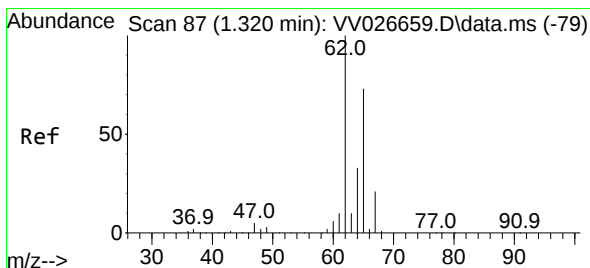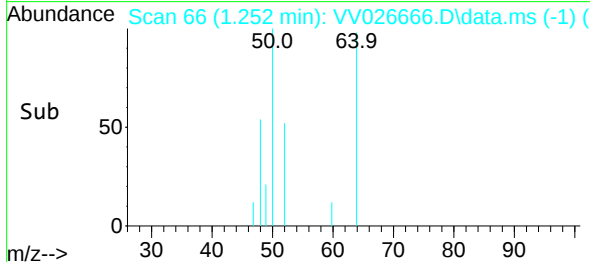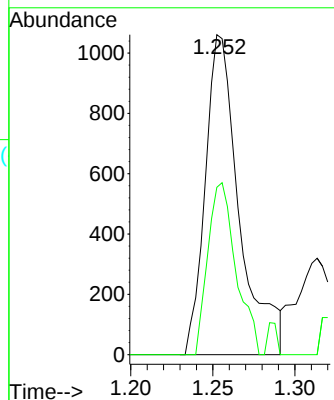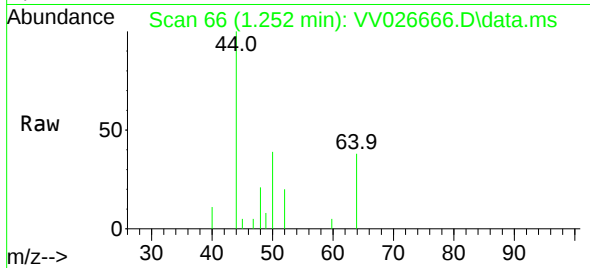

#5
Vinyl chloride
Concen: 0.297 ug/L
RT: 1.323 min Scan# 88
Delta R.T. 0.003 min
Lab File: VV026666.D
Acq: 06 Jul 2022 15:19

Tgt Ion: 62 Resp: 4779
Ion Ratio Lower Upper
62 100
64 125.5 26.2 48.6#


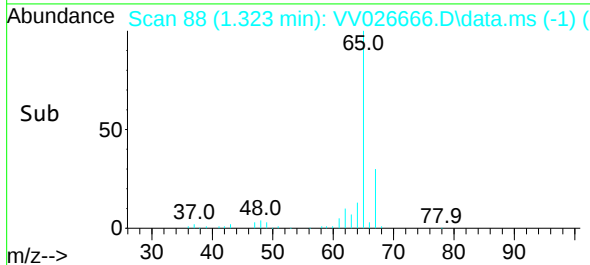
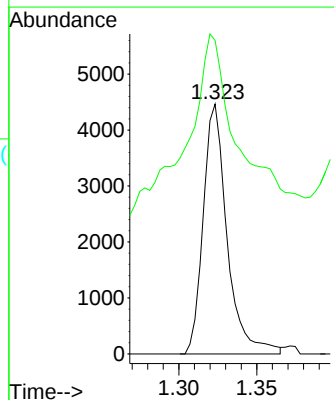
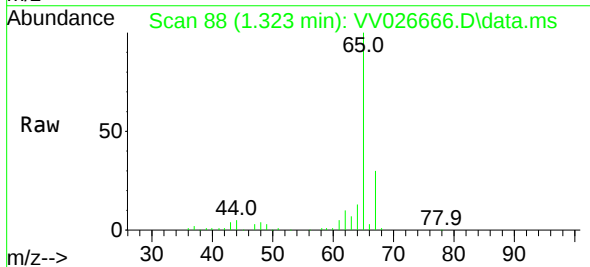


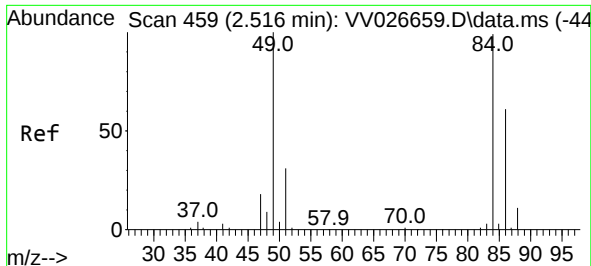

#16
Methylene chloride
Concen: 1.423 ug/L
RT: 2.519 min Scan# 41
Delta R.T. 0.003 min
Lab File: VV026666.D
Acq: 06 Jul 2022 15:19




Instrument :
MSVOA_V
ClientSampleId :
C0AN5DL


Tgt Ion: 84 Resp: 18506
Ion Ratio Lower Upper
84 100
86 65.1 46.0 85.4
49 105.4 77.7 144.3

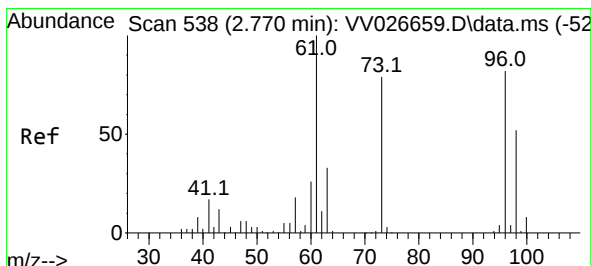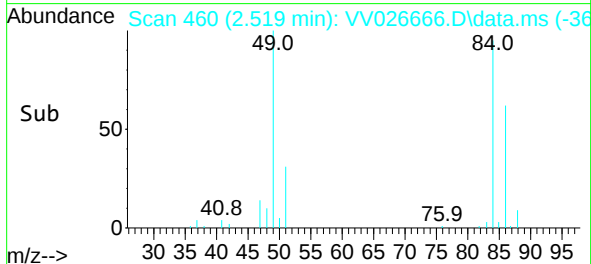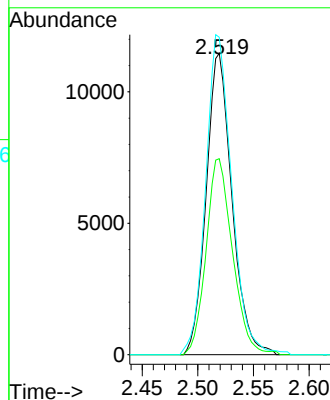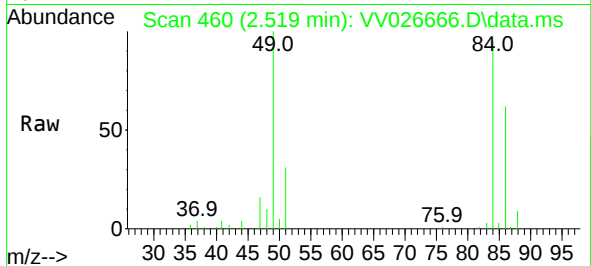

#18
trans-1,2-Dichloroethene
Concen: 0.055 ug/L
RT: 2.783 min Scan# 542
Delta R.T. 0.013 min
Lab File: VV026666.D
Acq: 06 Jul 2022 15:19

Tgt Ion: 96 Resp: 682
Ion Ratio Lower Upper
96 100
61 74.1 90.4 167.8#
98 59.2 45.6 84.8

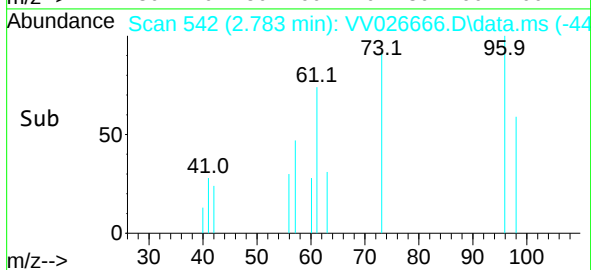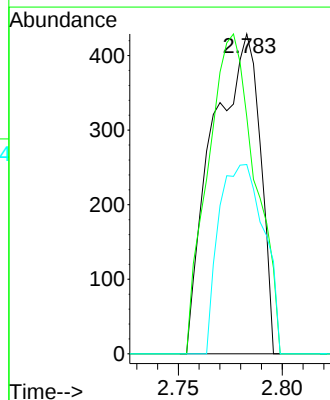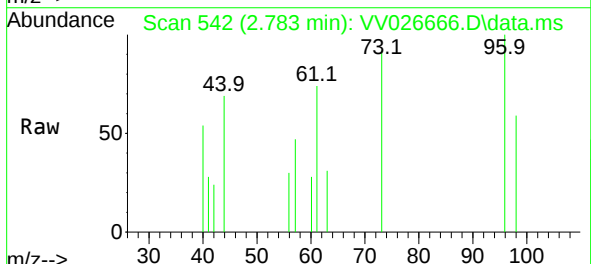

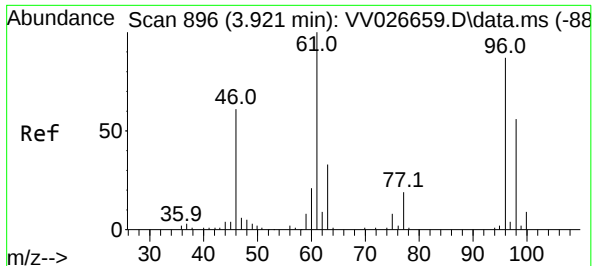

#22

cis-1,2-Dichloroethene

Concen: 1.100 ug/L

RT: 3.928 min Scan# 896

Delta R.T. 0.006 min

Lab File: VV026666.D

Acq: 06 Jul 2022 15:19

Instrument :

MSVOA_V

ClientSampleId :

C0AN5DL





Tgt Ion: 96 Resp: 13645

Ion Ratio Lower Upper

96 100

61 115.2 82.0 152.2

68 0.0 0.0 0.0

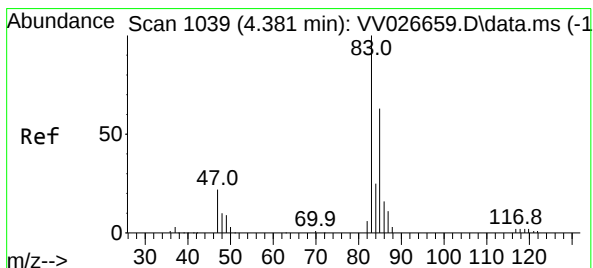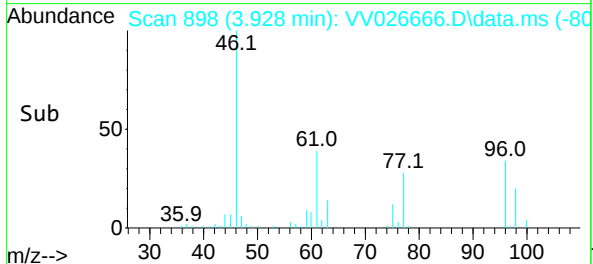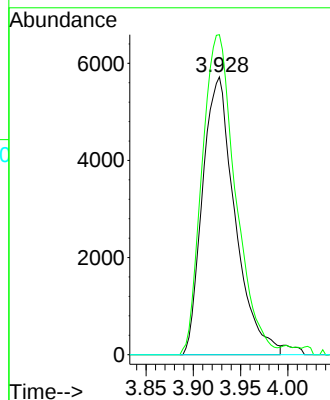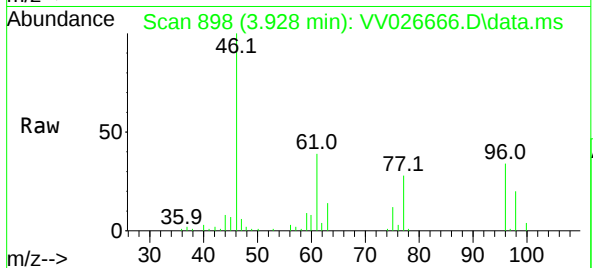

#25

Chloroform

Concen: 0.258 ug/L

RT: 4.384 min Scan# 1040

Delta R.T. 0.003 min

Lab File: VV026666.D




Acq: 06 Jul 2022 15:19


Tgt Ion: 83 Resp: 6191

Ion Ratio Lower Upper

83 100


85 62.6 44.0 81.8

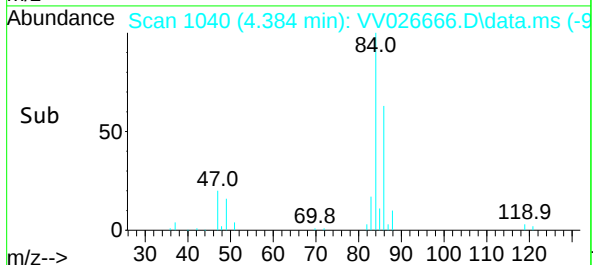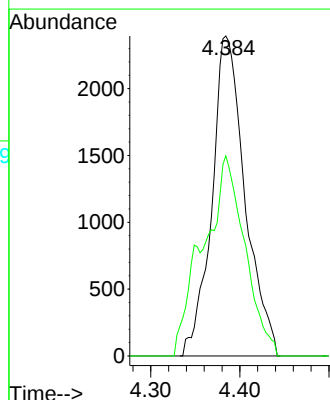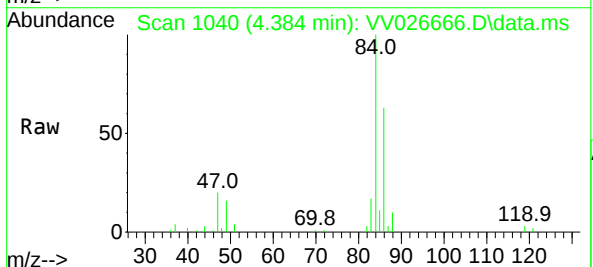



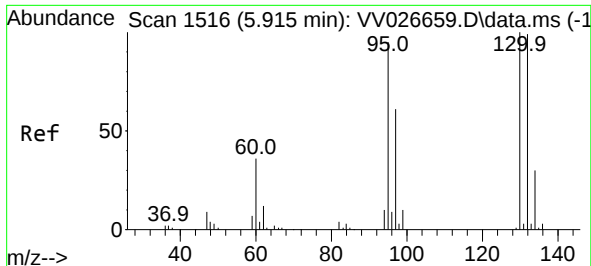


#34
Trichloroethene
Concen: 0.933 ug/L
RT: 5.924 min Scan# 11
Delta R.T. 0.009 min
Lab File: VV026666.D
Acq: 06 Jul 2022 15:19


Instrument :
MSVOA_V
ClientSampleId :
C0AN5DL

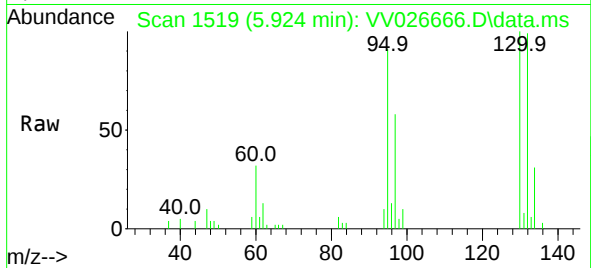



Tgt Ion: 95 Resp: 12740
Ion Ratio Lower Upper
95 100
97 63.6 46.8 87.0
132 108.9 69.9 129.7
130 110.3 72.0 133.8

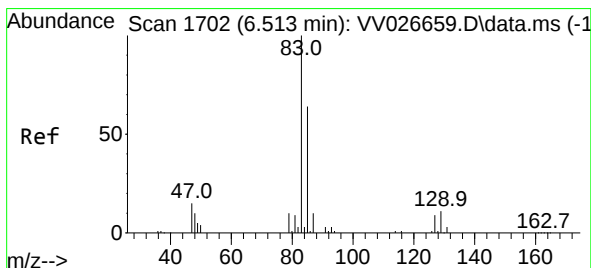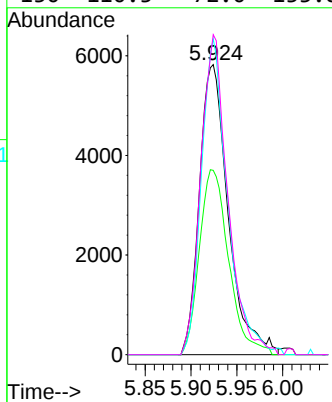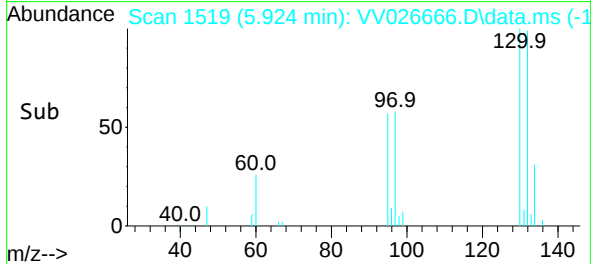


#38
Bromodichloromethane
Concen: 0.121 ug/L
RT: 6.519 min Scan# 1704
Delta R.T. 0.006 min
Lab File: VV026666.D
Acq: 06 Jul 2022 15:19

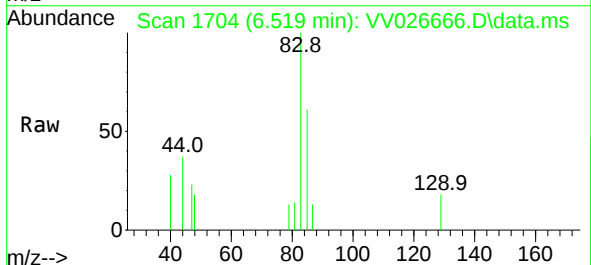

Tgt Ion: 83 Resp: 1794
Ion Ratio Lower Upper
83 100
85 61.2 44.0 81.8
127 0.0 6.6 10.0#



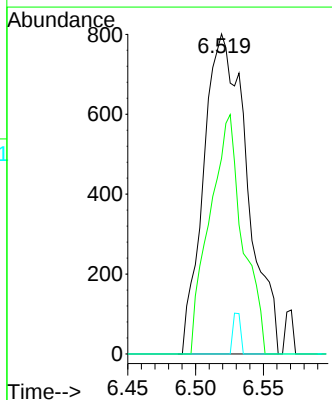
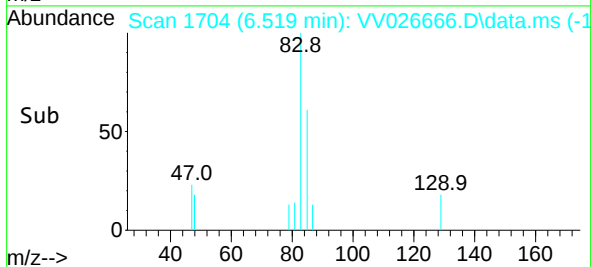


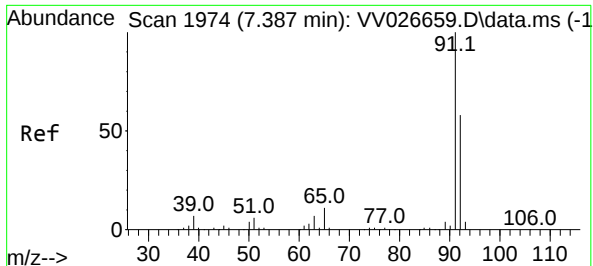

#42
Toluene
Concen: 0.341 ug/L
RT: 7.397 min Scan# 1974
Delta R.T. 0.009 min
Lab File: VV026666.D
Acq: 06 Jul 2022 15:19




Instrument :
MSVOA_V
ClientSampleId :
C0AN5DL


Tgt Ion: 91 Resp: 18267
Ion Ratio Lower Upper
91 100
92 50.5 40.3 74.9

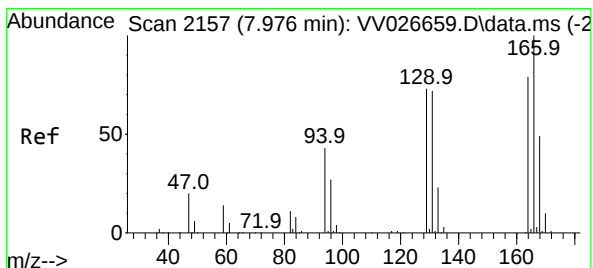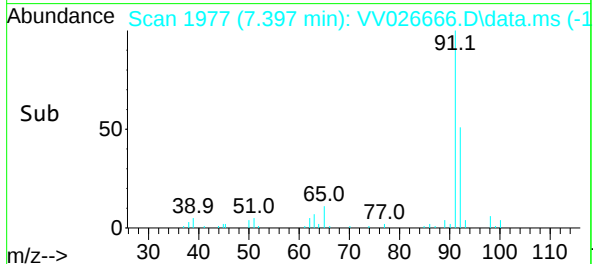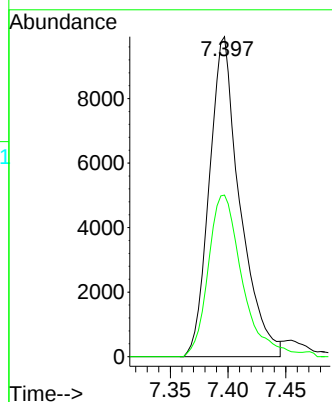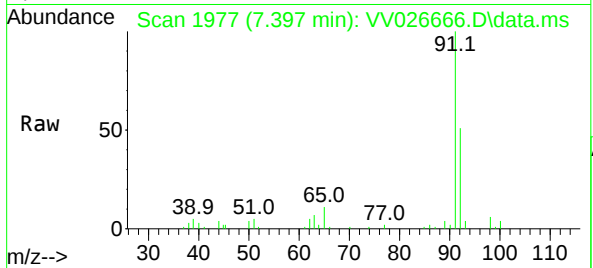

#47
Tetrachloroethene
Concen: 4.529 ug/L
RT: 7.976 min Scan# 2157
Delta R.T. -0.000 min
Lab File: VV026666.D
Acq: 06 Jul 2022 15:19

Tgt Ion: 164 Resp: 49225
Ion Ratio Lower Upper
164 100
129 95.1 66.4 123.2
131 87.2 64.4 119.6
166 126.0 88.1 163.7

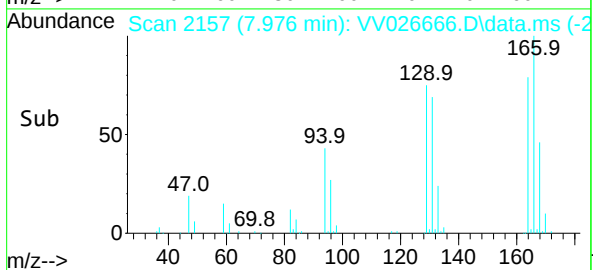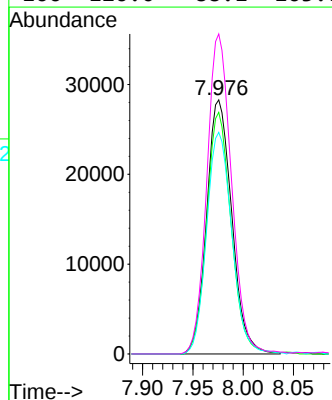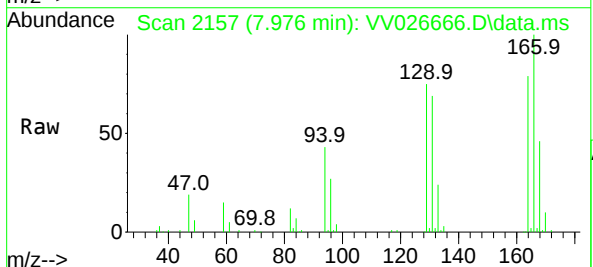

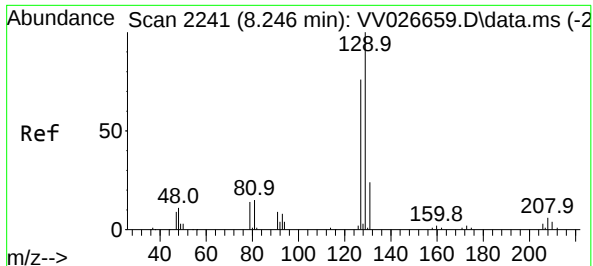

#49

Dibromochloromethane

Concen: 0.274 ug/L

RT: 8.249 min Scan# 21

Delta R.T. 0.003 min

Lab File: VV026666.D

Acq: 06 Jul 2022 15:19

Instrument :

MSVOA_V

ClientSampleId :





C0AN5DL

Tgt Ion:129 Resp: 2193

Ion Ratio Lower Upper

129 100

127 60.4 54.2 100.6

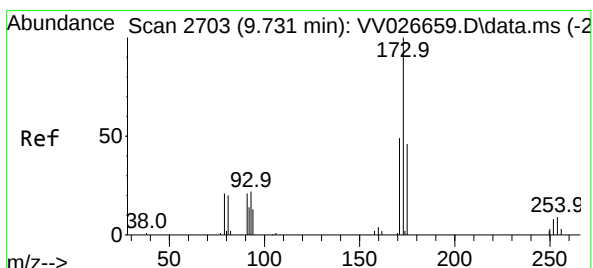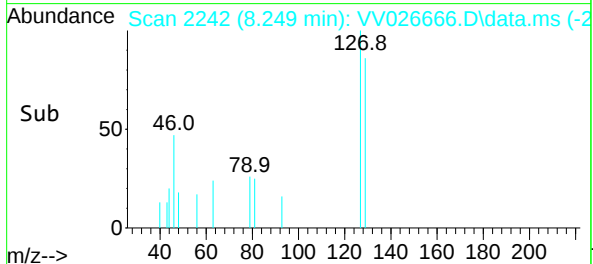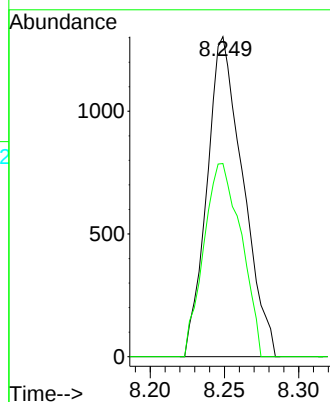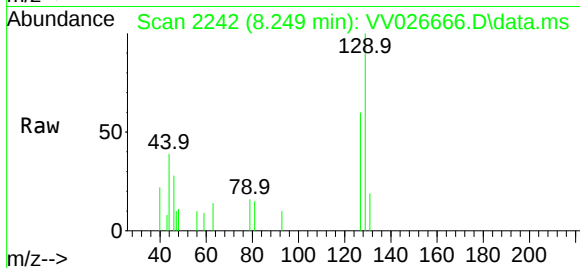

#59

Bromoform

Concen: 0.275 ug/L

RT: 9.734 min Scan# 2704

Delta R.T. 0.003 min

Lab File: VV026666.D

Acq: 06 Jul 2022 15:19

Tgt Ion:173 Resp: 722

Ion Ratio Lower Upper

173 100

175 46.0 37.9 56.9

254 0.0 6.3 9.5#

