

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070622\
 Data File : VV026663.D
 Acq On : 06 Jul 2022 13:18
 Operator : SY/MD
 Sample : N3598-05
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AN3

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV026663.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.320	79	87	107	rBV	97418	114651	20.49%	2.378%
2	1.580	161	168	182	rVB	91557	104347	18.65%	2.165%
3	2.117	326	335	355	rVB	184254	273253	48.83%	5.669%
4	2.304	384	393	406	rVB	8482	13053	2.33%	0.271%
5	2.519	450	460	471	rBV	12095	19901	3.56%	0.413%
6	3.934	885	900	929	rBV3	31935	142610	25.48%	2.959%
7	4.375	1016	1037	1063	rBV3	147897	521679	93.22%	10.823%
8	5.056	1233	1249	1280	rBV2	228996	559641	100.00%	11.610%
9	5.622	1414	1425	1456	rBV	205788	430606	76.94%	8.933%
10	6.075	1551	1566	1594	rBV	128285	268302	47.94%	5.566%
11	6.992	1841	1851	1877	rBV	41009	79295	14.17%	1.645%
12	7.320	1942	1953	1972	rBV	240151	423346	75.65%	8.783%
13	7.397	1972	1977	1997	rVB4	6168	14018	2.50%	0.291%
14	7.628	2039	2049	2064	rBV	23104	41779	7.47%	0.867%
15	7.940	2136	2146	2157	rBV2	8330	14388	2.57%	0.298%
16	8.095	2183	2194	2227	rBV2	159713	335374	59.93%	6.958%
17	8.854	2418	2430	2451	rBV	323789	526465	94.07%	10.922%
18	10.217	2843	2854	2875	rBV	87161	139907	25.00%	2.902%
19	10.381	2894	2905	2916	rBV2	22362	34752	6.21%	0.721%
20	11.249	3164	3175	3196	rBV	275016	429669	76.78%	8.914%
21	11.622	3280	3291	3307	rBV	214120	333274	59.55%	6.914%




Sum of corrected areas: 4820310

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070622\
Data File : VV026663.D
Acq On : 06 Jul 2022 13:18
Operator : SY/MD
Sample : N3598-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COAN3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

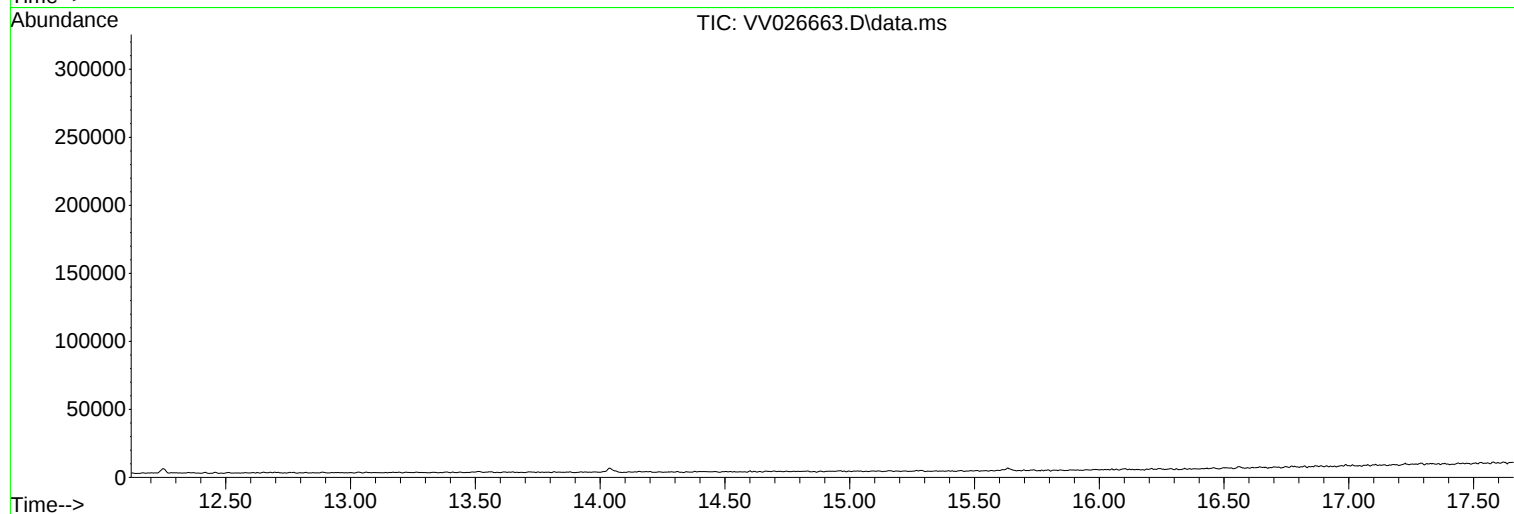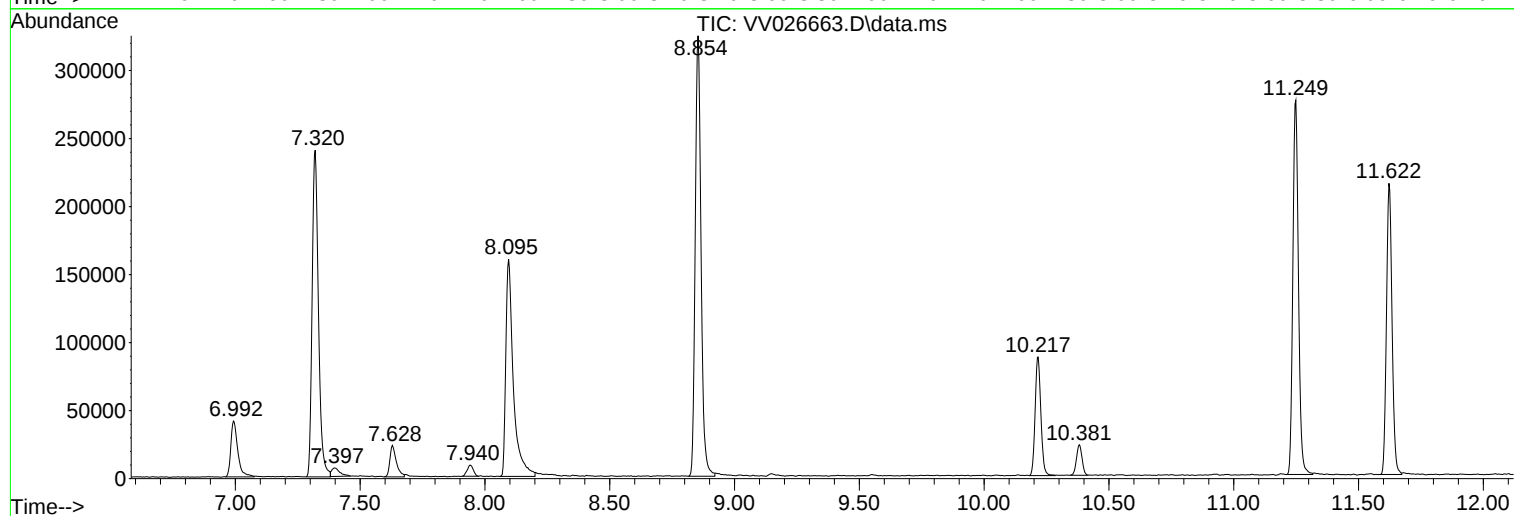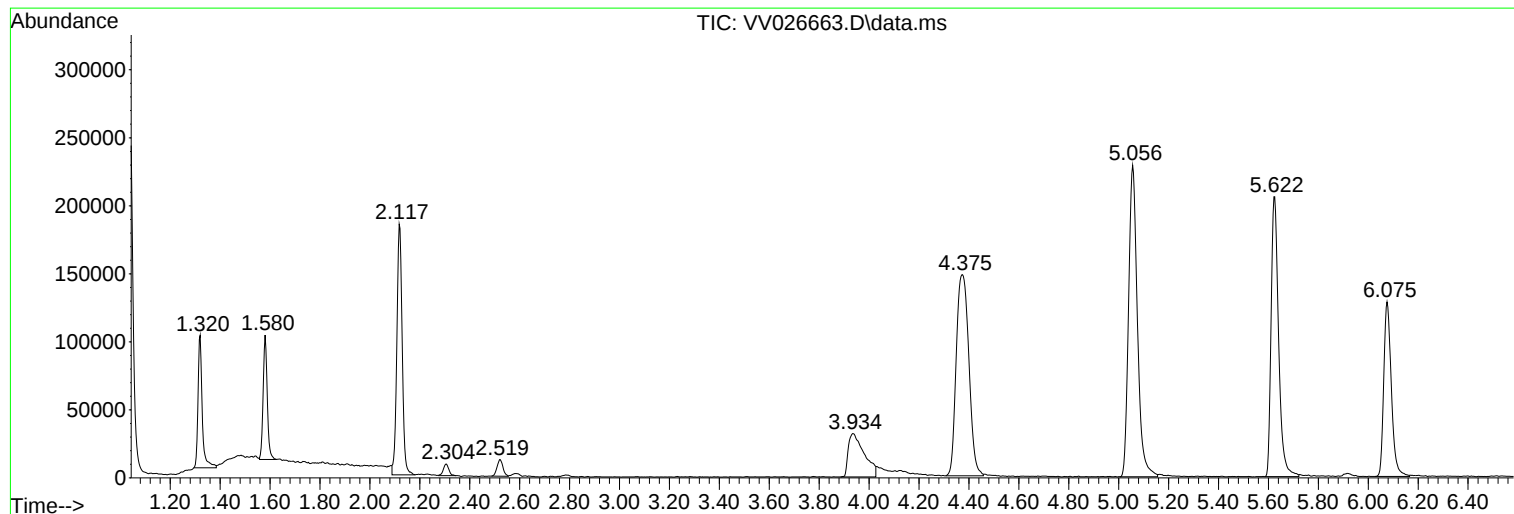

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070622\
Data File : VV026663.D
Acq On : 06 Jul 2022 13:18
Operator : SY/MD
Sample : N3598-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AN3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070622\
Data File : VV026663.D
Acq On : 06 Jul 2022 13:18
Operator : SY/MD
Sample : N3598-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AN3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc