

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070622\
 Data File : VV026664.D
 Acq On : 06 Jul 2022 13:42
 Operator : SY/MD
 Sample : N3598-06
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AN5

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV026664.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.124	19	26	42	rVB2	125720	135369	1.08%	0.570%
2	1.252	60	66	78	rBV	377828	434804	3.46%	1.829%
3	1.320	78	87	106	rVB3	360695	455863	3.63%	1.918%
4	2.117	326	335	351	rVB2	189720	293158	2.33%	1.233%
5	2.776	525	540	562	rBV4	70092	153704	1.22%	0.647%
6	3.921	876	896	932	rBV	816057	2023251	16.11%	8.513%
7	4.365	1018	1034	1063	rVB3	120698	381961	3.04%	1.607%
8	5.056	1233	1249	1283	rBV2	227340	575758	4.59%	2.423%
9	5.622	1412	1425	1449	rBV	230411	469643	3.74%	1.976%
10	5.918	1500	1517	1553	rBV	1186821	2298071	18.30%	9.669%
11	6.075	1554	1566	1590	rVV	128109	267481	2.13%	1.125%
12	7.320	1941	1953	1964	rBV	248047	432038	3.44%	1.818%
13	7.390	1964	1975	2001	rVB	710078	1219637	9.71%	5.132%
14	7.976	2134	2157	2184	rBV	7709984	12555799	100.00%	52.829%
15	8.091	2184	2193	2230	rVV	197525	404195	3.22%	1.701%
16	8.249	2231	2242	2256	rVB	85732	145832	1.16%	0.614%
17	8.853	2418	2430	2452	rBV	343219	568287	4.53%	2.391%
18	10.217	2843	2854	2868	rBV	85822	135533	1.08%	0.570%
19	11.249	3164	3175	3193	rBV	307073	474047	3.78%	1.995%
20	11.622	3280	3291	3308	rBV	214562	342242	2.73%	1.440%




Sum of corrected areas: 23766673

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070622\
Data File : VV026664.D
Acq On : 06 Jul 2022 13:42
Operator : SY/MD
Sample : N3598-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COAN5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

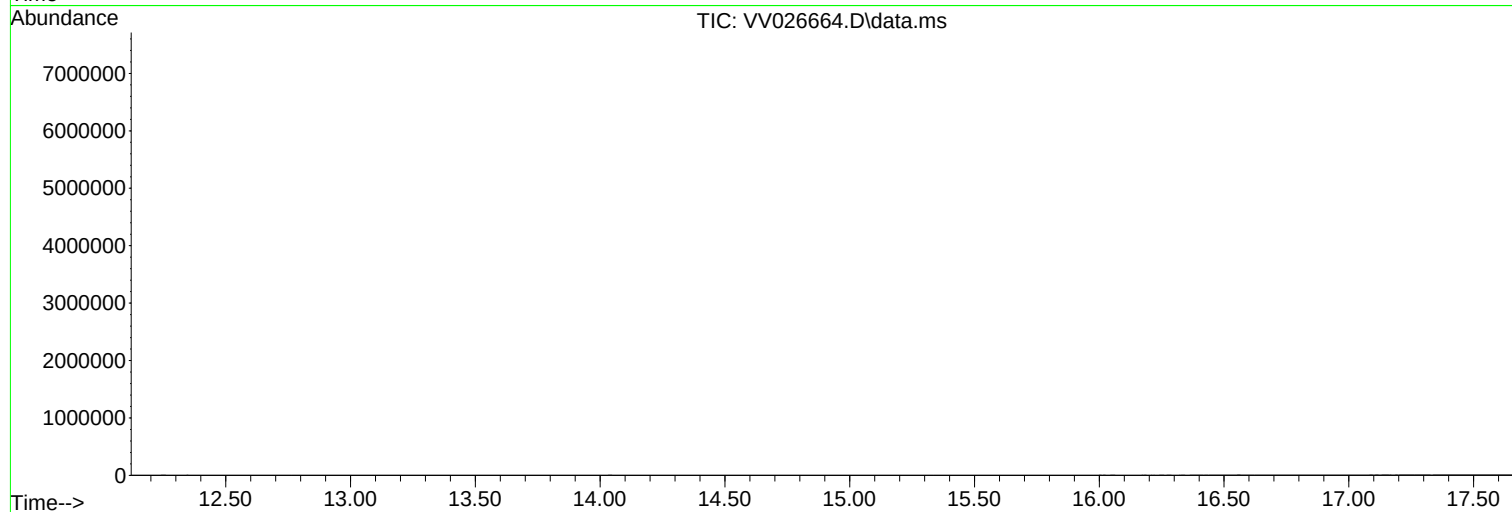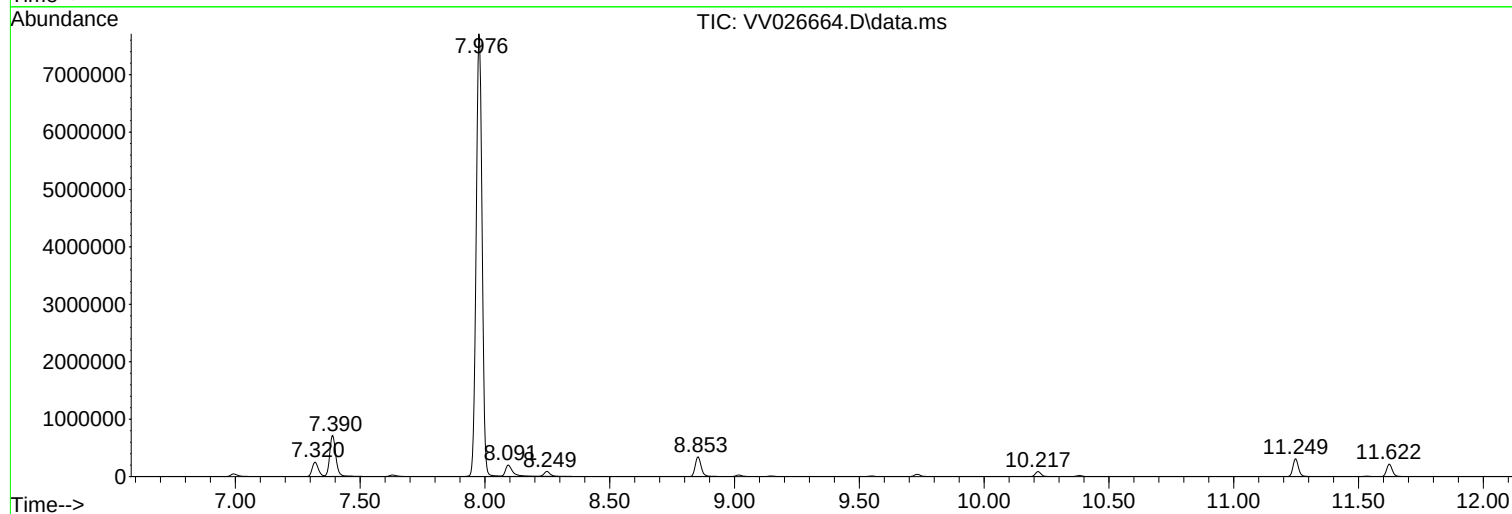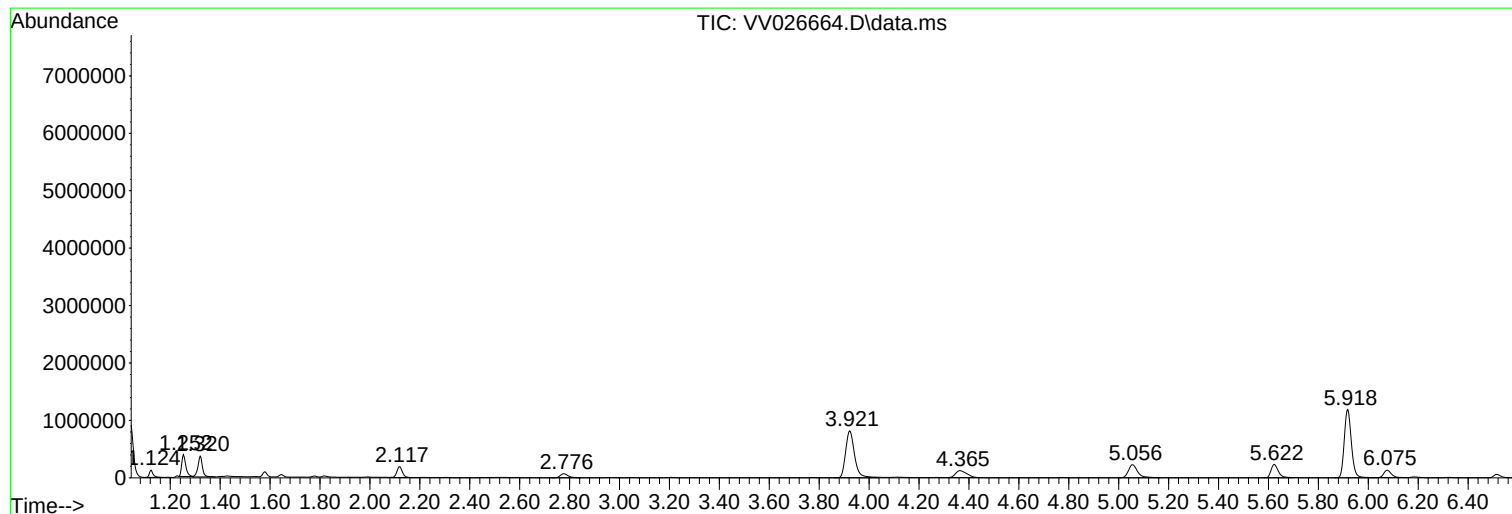

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070622\
Data File : VV026664.D
Acq On : 06 Jul 2022 13:42
Operator : SY/MD
Sample : N3598-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AN5










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Straight-Chai... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.124	1.44 ug/L	135369	1,4-Difluorobenzene	5.622

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Propene	42	C3H6	000115-07-1	90
2			Propene	42	C3H6	000115-07-1	42
3			Cyclopropane	42	C3H6	000075-19-4	9
4			Cyclopropane	42	C3H6	000075-19-4	7
5			Cyclopropene	40	C3H4	002781-85-3	5

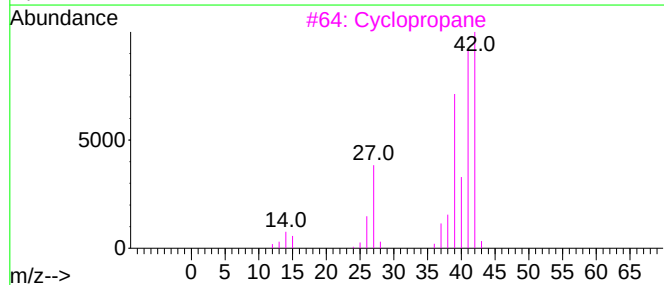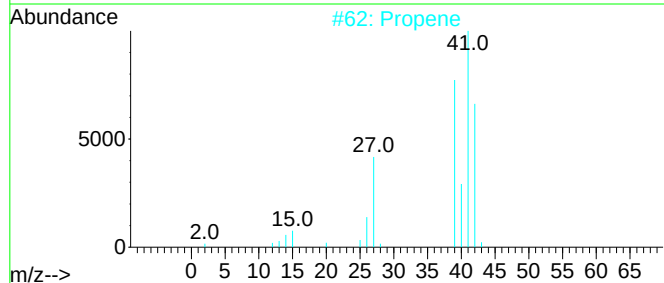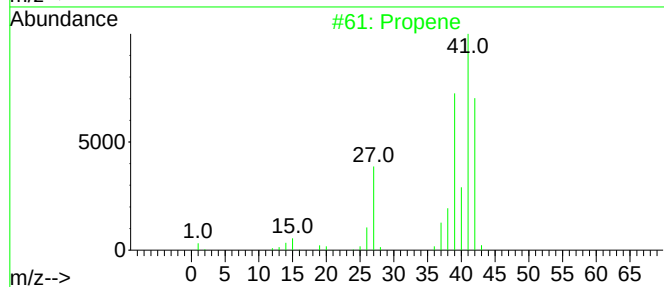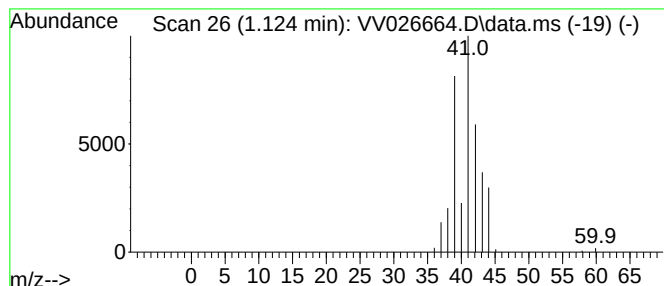

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070622\
Data File : VV026664.D
Acq On : 06 Jul 2022 13:42
Operator : SY/MD
Sample : N3598-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AN5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: S...	1.124	1.4	ug/L	135369	1	5.622	469643	5.0