

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070622\
 Data File : VV026665.D
 Acq On : 06 Jul 2022 14:23
 Operator : SY/MD
 Sample : VIBLK273
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK273

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV026665.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.320	79	87	102	rBV	94887	102170	19.26%	2.407%
2	1.580	161	168	182	rVB	83835	99082	18.68%	2.335%
3	2.117	325	335	352	rVB	177257	259122	48.85%	6.106%
4	2.519	449	460	474	rBV	29558	48793	9.20%	1.150%
5	3.050	613	625	638	rBV3	5054	10302	1.94%	0.243%
6	3.918	884	895	897	rBV	33170	46093	8.69%	1.086%
7	4.358	1013	1032	1057	rBV	100162	255620	48.19%	6.023%
8	5.053	1232	1248	1277	rBV2	216223	530438	100.00%	12.499%
9	5.622	1413	1425	1452	rBV	199191	414631	78.17%	9.770%
10	5.921	1507	1518	1532	rBV10	3375	7536	1.42%	0.178%
11	6.072	1552	1565	1587	rBV	123113	255650	48.20%	6.024%
12	6.989	1840	1850	1871	rBV	38394	75485	14.23%	1.779%
13	7.317	1937	1952	1975	rBV	227505	404606	76.28%	9.534%
14	7.625	2039	2048	2070	rBV	20934	40658	7.66%	0.958%
15	7.979	2150	2158	2169	rVB3	9384	16126	3.04%	0.380%
16	8.091	2181	2193	2229	rBV2	157837	329499	62.12%	7.764%
17	8.850	2417	2429	2450	rBV	304256	500775	94.41%	11.800%
18	10.214	2841	2853	2873	rVB2	84209	132205	24.92%	3.115%
19	11.246	3164	3174	3195	rBV	262077	406522	76.64%	9.579%
20	11.622	3280	3291	3318	rBV	193803	308681	58.19%	7.273%




Sum of corrected areas: 4243994

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070622\
Data File : VV026665.D
Acq On : 06 Jul 2022 14:23
Operator : SY/MD
Sample : VIBLK273
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK273

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

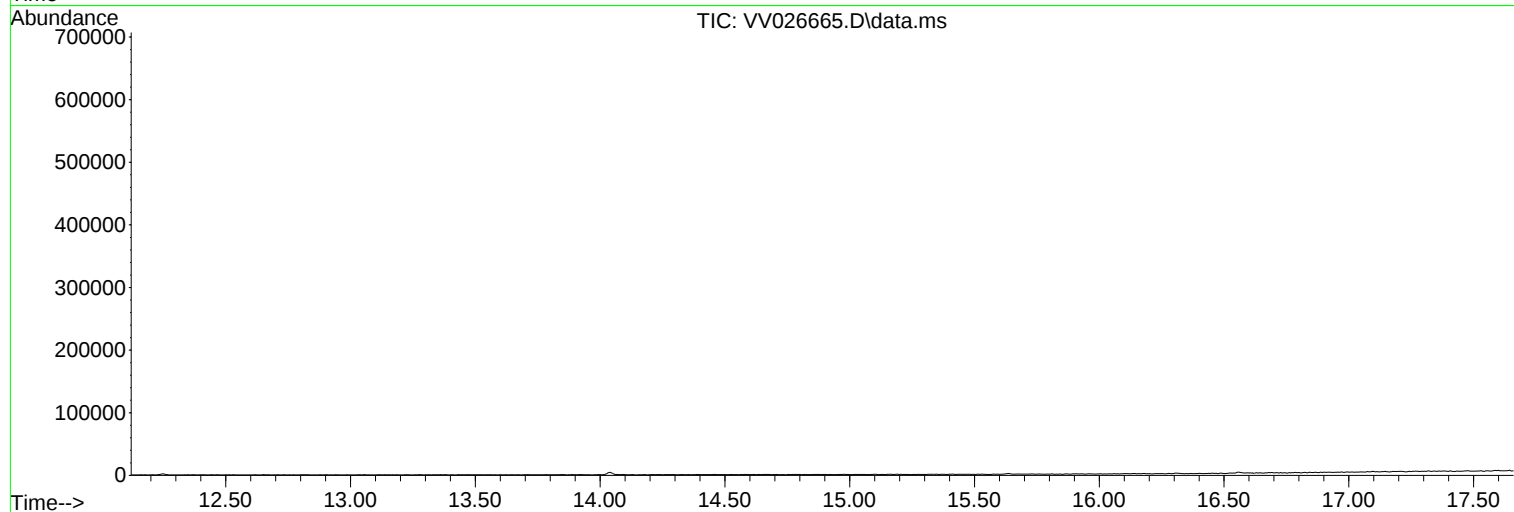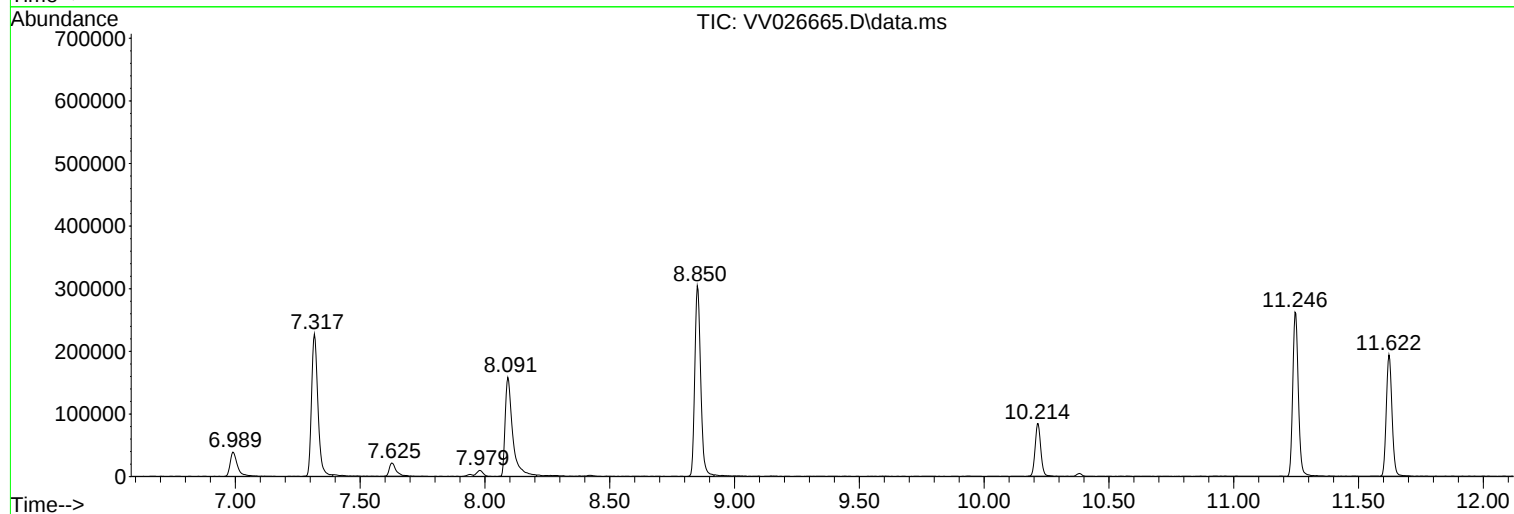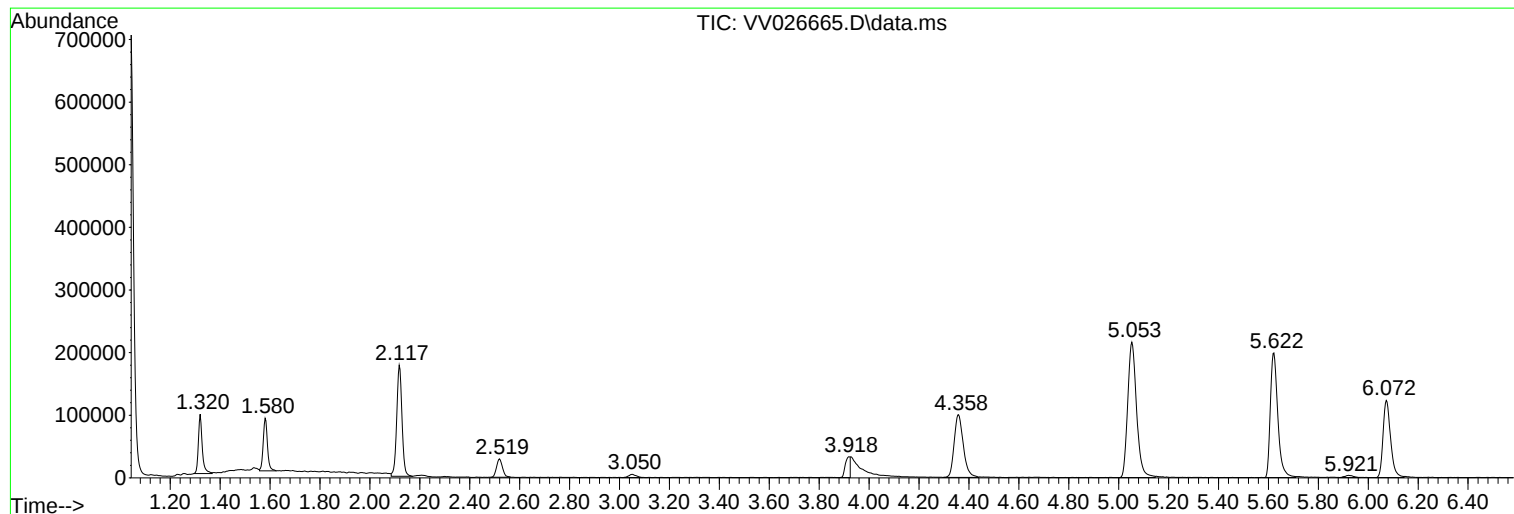

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070622\
Data File : VV026665.D
Acq On : 06 Jul 2022 14:23
Operator : SY/MD
Sample : VIBLK273
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK273

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070622\
Data File : VV026665.D
Acq On : 06 Jul 2022 14:23
Operator : SY/MD
Sample : VIBLK273
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK273

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc