


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070622\
 Data File : VV026658.D
 Acq On : 06 Jul 2022 08:49
 Operator : SY/MD
 Sample : BFB339
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB339

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Fri Jul 08 23:50:05 2022

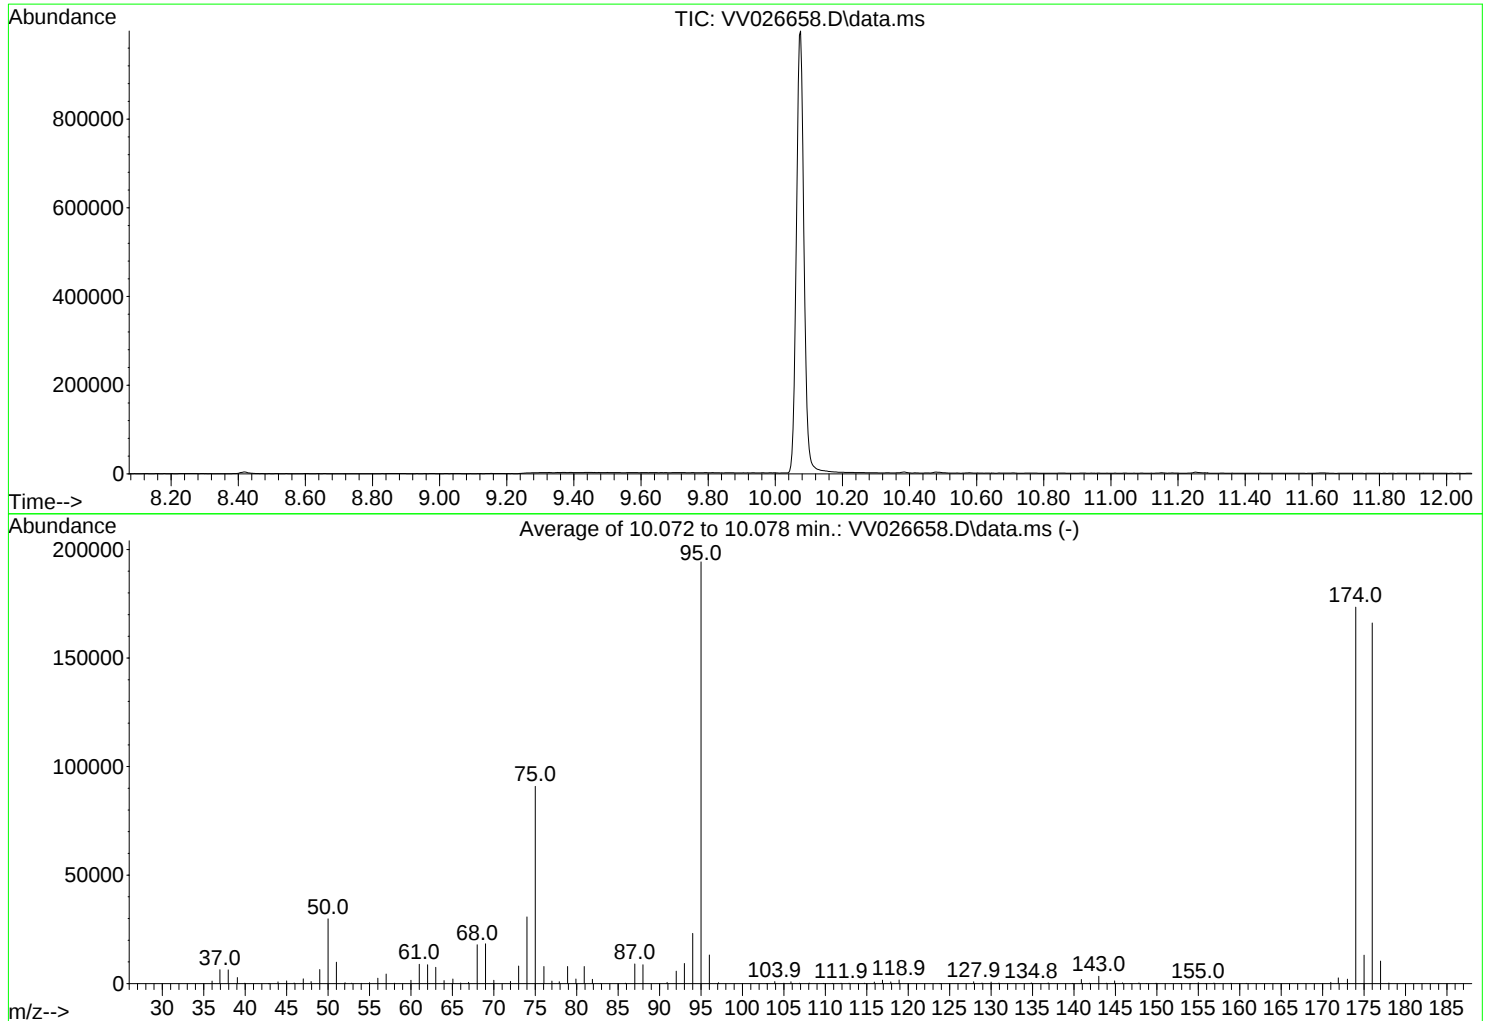

AutoFind: Scans 2809, 2810, 2811; Background Corrected with Scan 2796

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.4	29848	PASS
75	95	30	80	46.8	90923	PASS
95	95	100	100	100.0	194325	PASS
96	95	5	9	6.8	13177	PASS
173	174	0.00	2	1.2	2101	PASS
174	95	50	120	89.3	173461	PASS
175	174	5	9	7.6	13121	PASS
176	174	95	105	95.8	166187	PASS
177	176	5	10	6.3	10387	PASS

m/z	Abundance
36.00	1149.0
36.90	122.0
37.90	458.0
39.90	198.0
43.90	296.0

Instrument :
MSVOA_V
ClientSampleId :
BFB339

m/z	Abundance
36.00	2362.0
37.00	6937.0
38.00	7406.0
39.10	2804.0
40.00	484.0
44.00	1159.0
45.00	1353.0
45.90	300.0
47.00	2397.0
48.00	976.0
49.00	6757.0
50.00	31200.0
51.00	10533.0
52.00	498.0
52.90	206.0
54.00	193.0
55.00	478.0
56.00	2633.0
57.00	4480.0
58.00	241.0
60.00	1675.0
61.00	9391.0
62.00	9215.0
63.00	7981.0
64.00	1501.0
65.00	2246.0
66.00	342.0
67.00	580.0
68.00	18792.0
69.00	19040.0
70.00	1588.0
72.00	1104.0
73.00	8516.0
74.00	31656.0
75.00	95160.0
76.00	8482.0
77.00	1161.0
77.90	931.0
78.90	8261.0
79.90	2203.0
80.90	8329.0
81.90	2014.0
82.90	185.0
85.90	258.0
87.00	9202.0
88.00	9034.0
90.90	657.0
92.00	5819.0
93.00	9456.0
94.00	24072.0
95.00	199488.0
96.00	13647.0
97.10	469.0
103.90	961.0
105.00	230.0
105.90	898.0
106.90	231.0
108.00	288.0
109.80	145.0
110.90	175.0
111.90	239.0
112.90	200.0
114.80	229.0
115.90	645.0
116.90	1630.0
117.90	818.0
118.90	1687.0
123.80	110.0
127.90	946.0
128.90	278.0
130.00	760.0
130.90	279.0
135.00	349.0
136.90	339.0
139.90	179.0
140.90	1989.0
141.90	228.0
143.00	3507.0
143.90	291.0
144.90	1379.0
145.80	334.0
146.80	123.0
147.80	418.0
148.70	110.0
149.90	206.0
152.90	142.0
154.00	103.0
154.90	470.0
155.90	105.0
156.90	339.0
159.00	225.0
160.80	211.0

Instrument :
MSVOA_V
ClientSampleId :
BFB339

171.00	730.0
171.90	2595.0
173.00	2154.0
174.00	173952.0
175.00	13694.0
176.00	167552.0
177.00	10649.0
178.00	319.0

Instrument :
MSVOA_V
ClientSampleId :
BFB339

m/z	Abundance
36.00	2444.0
37.00	6713.0
38.00	7022.0
39.00	2899.0
40.00	424.0
42.80	107.0
44.00	1166.0
45.00	1330.0
45.90	301.0
47.00	2319.0
48.00	984.0
49.00	6733.0
50.00	30928.0
51.00	10232.0
52.10	479.0
52.80	203.0
54.00	178.0
55.00	506.0
56.00	2592.0
57.00	4592.0
58.00	244.0
60.00	1620.0
61.00	9300.0
62.00	8927.0
63.00	7768.0
64.00	1434.0
65.00	2241.0
66.00	329.0
66.90	582.0
68.00	18552.0
69.00	18984.0
70.00	1632.0
72.00	1076.0
73.00	8489.0
74.00	31904.0
75.00	94136.0
76.10	8117.0
77.00	1226.0
77.90	936.0
78.90	8078.0
79.90	2188.0
80.90	8104.0
81.90	2048.0
82.90	179.0
85.90	231.0
87.00	9407.0
88.00	9018.0
90.90	601.0
92.00	5998.0
93.00	9661.0
94.00	24040.0
95.00	201344.0
96.00	13740.0
97.10	439.0
103.90	952.0
105.00	228.0
105.80	956.0
106.90	252.0
108.10	289.0
109.80	143.0
110.90	174.0
111.90	262.0
112.80	223.0
114.70	260.0
115.90	737.0
116.90	1694.0
117.90	796.0
118.90	1760.0
127.90	902.0
128.90	280.0
130.00	769.0
130.90	289.0
134.80	387.0
136.90	337.0
139.80	174.0
140.90	2016.0
141.90	249.0
143.00	3537.0
143.90	272.0
144.90	1254.0
145.90	341.0
146.80	122.0
147.80	386.0
148.80	105.0
149.90	219.0
152.80	164.0
155.00	491.0
156.90	326.0
158.90	225.0
160.80	185.0
171.00	593.0
171.90	2752.0

Instrument :
MSVOA_V
ClientSampleId :
BFB339

173.00	2134.0
174.00	179968.0
175.00	13677.0
176.00	171968.0
177.00	10785.0
178.00	302.0

Instrument :
MSVOA_V
ClientSampleId :
BFB339

m/z	Abundance
36.00	2307.0
37.00	5990.0
38.00	6001.0
39.00	2813.0
40.00	330.0
44.00	1072.0
45.00	1176.0
45.90	276.0
47.00	1886.0
47.90	846.0
49.00	5991.0
50.00	27416.0
51.00	8958.0
52.10	414.0
52.80	219.0
54.10	152.0
55.00	476.0
56.00	2269.0
57.00	4307.0
58.00	260.0
60.00	1474.0
61.00	8069.0
62.00	7884.0
63.00	6853.0
64.00	1200.0
65.10	1990.0
66.00	289.0
66.90	525.0
68.00	16472.0
69.00	17112.0
70.00	1466.0
72.00	951.0
73.00	7445.0
74.00	28600.0
75.00	83472.0
76.10	7025.0
77.00	1186.0
77.90	791.0
78.90	7377.0
79.90	1959.0
80.90	7333.0
81.90	1899.0
82.90	176.0
85.90	227.0
87.00	8606.0
88.00	7957.0
90.90	581.0
92.00	5540.0
93.00	8791.0
94.00	21336.0
95.00	182144.0
96.00	12145.0
97.10	339.0
102.90	114.0
103.90	875.0
105.00	208.0
105.90	868.0
106.90	209.0
108.10	247.0
109.80	117.0
110.80	154.0
111.90	246.0
112.80	228.0
114.70	264.0
115.90	769.0
116.90	1510.0
117.90	754.0
118.90	1566.0
127.90	776.0
128.90	320.0
130.00	677.0
131.00	292.0
134.80	412.0
136.90	334.0
139.80	118.0
140.90	1854.0
141.90	254.0
143.00	3170.0
144.00	206.0
144.90	1080.0
145.90	354.0
146.80	101.0
147.90	349.0
149.90	233.0
152.80	204.0
155.10	451.0
156.90	307.0
158.90	216.0
160.80	168.0
171.10	415.0
171.90	2733.0
173.00	2014.0

Instrument :
MSVOA_V
ClientSampleId :
BFB339

174.00	166464.0
175.00	11992.0
176.00	159040.0
177.00	9728.0
178.00	252.0

Instrument :
MSVOA_V
ClientSampleId :
BFB339