




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070623\
 Data File : VV031645.D
 Acq On : 06 Jul 2023 11:07
 Operator : SY/MD
 Sample : 03504-01ME
 Misc : 3.83g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A46R7ME

Manual IntegrationsAPPROVED

Quant Time: Jul 07 02:35:52 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Jul 07 02:34:55 2023
 Response via : Initial Calibration

Reviewed By :John Carlone 07/07/2023
 Supervised By :Mahesh Dadoda 07/07/2023

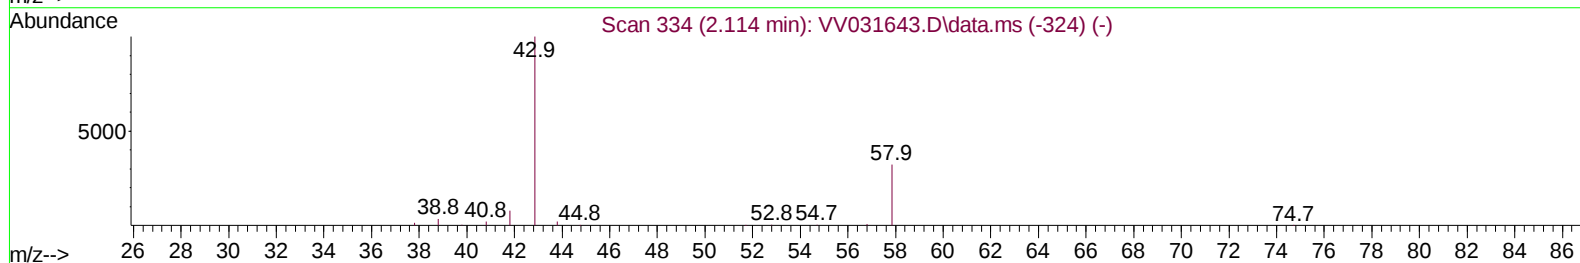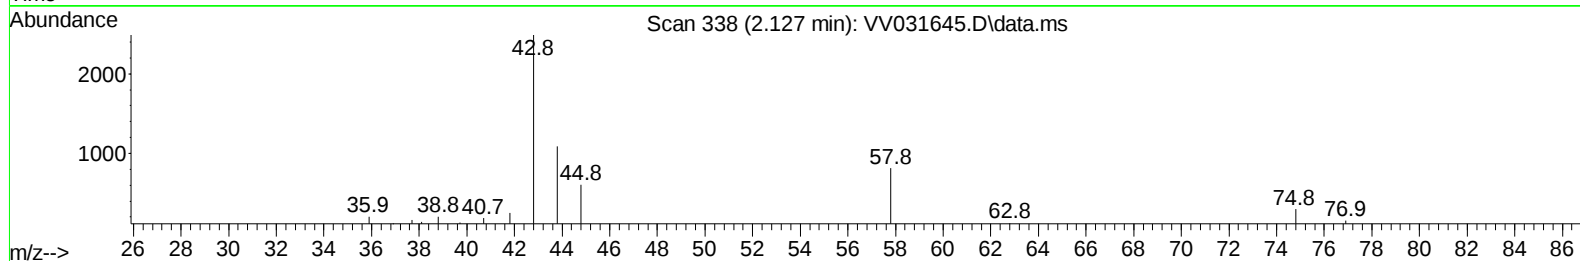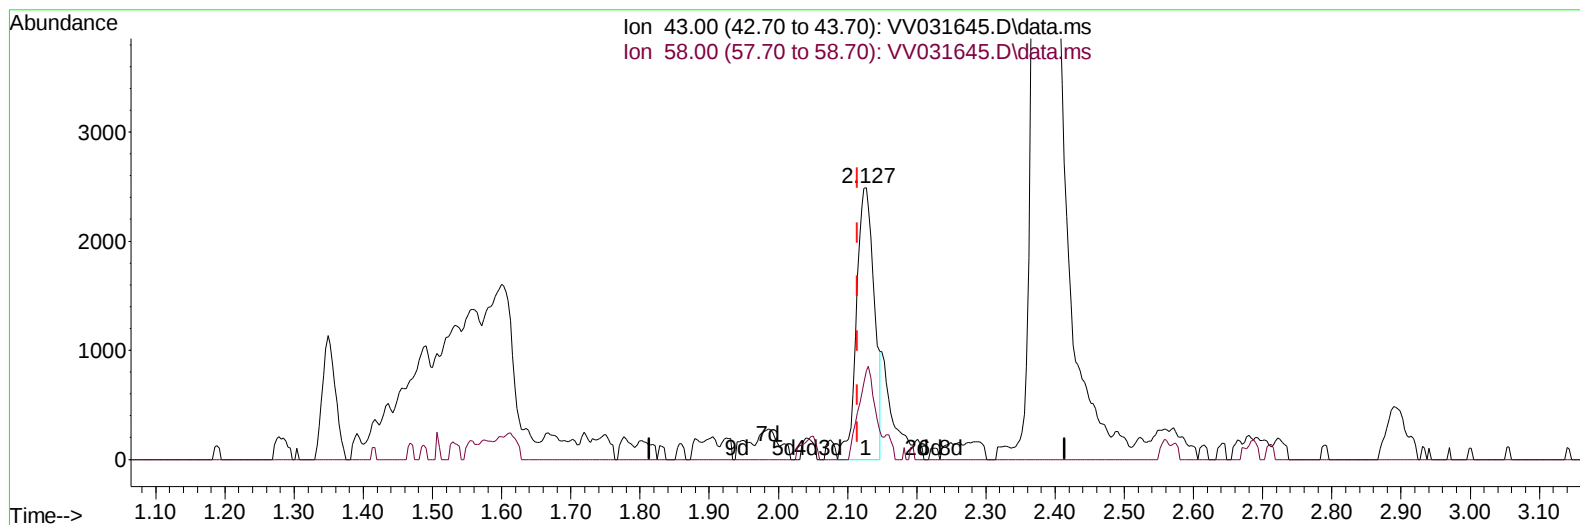

TIC: VV031645.D\data.ms

(13) Acetone (T)

2.127min (+ 0.013) 3.91 ug/L

response 4475

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	34.30	32.16
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070623\
 Data File : VV031645.D
 Acq On : 06 Jul 2023 11:07
 Operator : SY/MD
 Sample : 03504-01ME
 Misc : 3.83g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A46R7ME

Manual IntegrationsAPPROVED

Quant Time: Jul 07 02:35:52 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Jul 07 02:34:55 2023
 Response via : Initial Calibration

Reviewed By :John Carlone 07/07/2023
 Supervised By :Mahesh Dadoda 07/07/2023

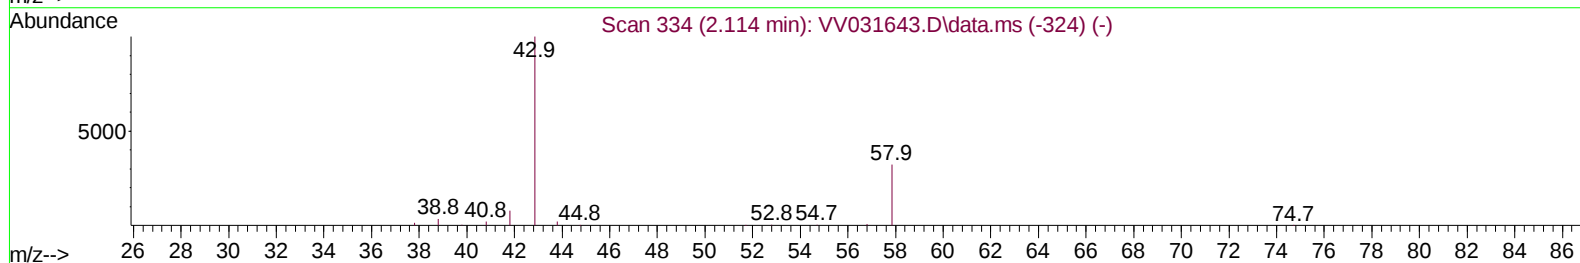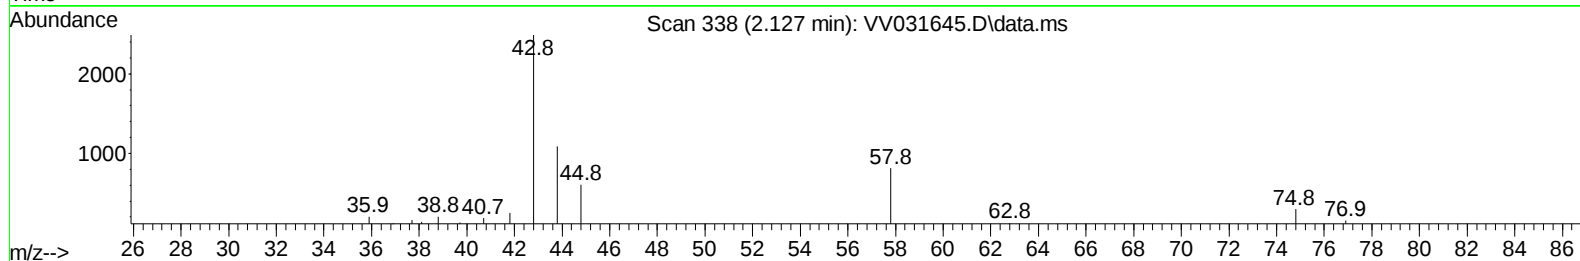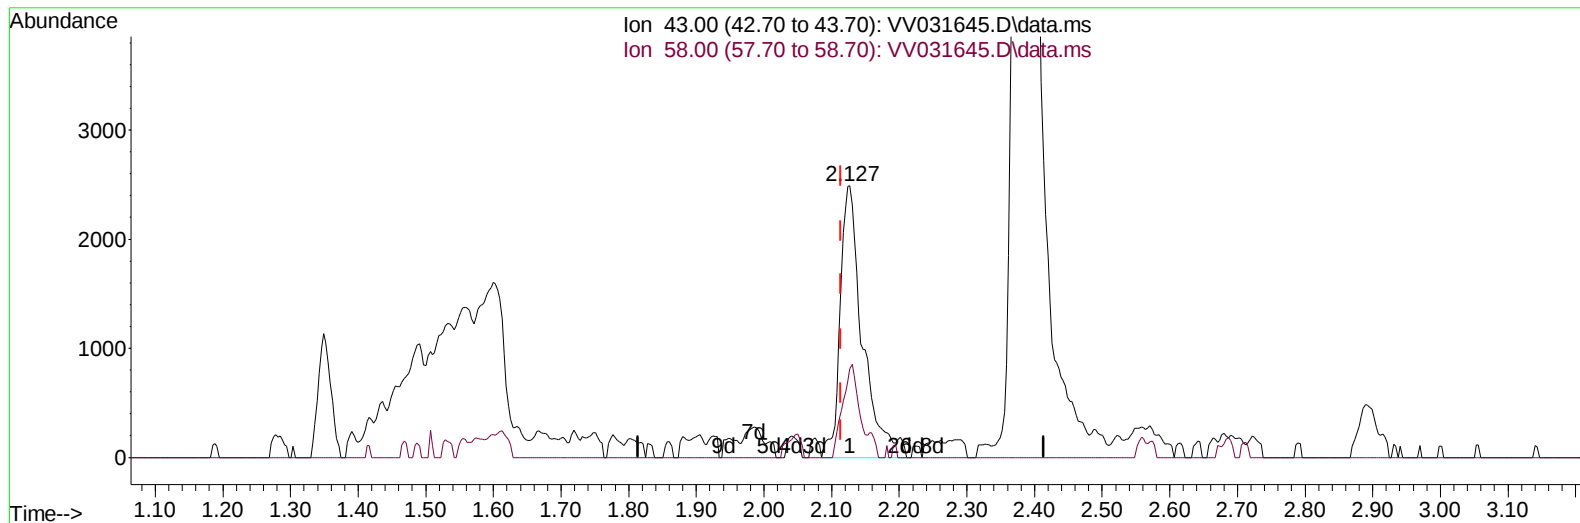

TIC: VV031645.D\data.ms

(13) Acetone (T)

2.127min (+ 0.013) 4.99 ug/L m

response 5715

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	34.30	25.18
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070623\
 Data File : VV031645.D
 Acq On : 06 Jul 2023 11:07
 Operator : SY/MD
 Sample : 03504-01ME
 Misc : 3.83g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A46R7ME

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 07/07/2023
 Supervised By :Mahesh Dadoda 07/07/2023

Quant Time: Jul 07 02:35:52 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Jul 07 02:34:55 2023
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	5.539	114		215341	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.792	117		214610	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.194	152		120506	50.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.278	65		45605	31.821	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135		Recovery	=	63.640%	
7) Chloroethane-d5	1.510	69		22901	18.314	ug/L	-0.02
Spiked Amount 50.000	Range 70	- 130		Recovery	=	36.620%#	
11) 1,1-Dichloroethene-d2	2.043	65		21702	29.382	ug/L	-0.02
Spiked Amount 50.000	Range 60	- 125		Recovery	=	58.760%#	
21) 2-Butanone-d5	3.802	46		97772	84.252	ug/L	0.00
Spiked Amount 100.000	Range 40	- 130		Recovery	=	84.250%	
24) Chloroform-d	4.252	84		120951	33.698	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125		Recovery	=	67.400%#	
26) 1,2-Dichloroethane-d4	4.947	65		81625	36.348	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125		Recovery	=	72.700%	
32) Benzene-d6	4.960	84		187341	31.013	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125		Recovery	=	62.020%#	
36) 1,2-Dichloropropane-d6	5.992	67		72393	33.812	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120		Recovery	=	67.620%#	
41) Toluene-d8	7.249	98		148853	26.852	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120		Recovery	=	53.700%#	
43) trans-1,3-Dichloroprop...	7.561	79		34223	32.789	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125		Recovery	=	65.580%	
47) 2-Hexanone-d5	8.046	63		67041	79.305	ug/L	0.02
Spiked Amount 100.000	Range 45	- 130		Recovery	=	79.310%	
56) 1,1,2,2-Tetrachloroeth...	10.162	84		121150	37.488	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120		Recovery	=	74.980%	
66) 1,2-Dichlorobenzene-d4	11.570	152		82870	36.077	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120		Recovery	=	72.160%#	
Target Compounds							
13) Acetone	2.127	43		5715m	4.991	ug/L	
15) Methyl Acetate	2.381	43		31351	16.261	ug/L	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070623\
Data File : VV031645.D
Acq On : 06 Jul 2023 11:07
Operator : SY/MD
Sample : 03504-01ME
Misc : 3.83g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A46R7ME

Manual IntegrationsAPPROVED

Quant Time: Jul 07 02:35:52 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Jul 07 02:34:55 2023
Response via : Initial Calibration

Reviewed By :John Carlone 07/07/2023
Supervised By :Mahesh Dadoda 07/07/2023

