

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070623\
 Data File : VV031644.D
 Acq On : 06 Jul 2023 10:13
 Operator : SY/MD
 Sample : VV0706MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK365

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

Signal : TIC: VV031644.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	69	74	90	rVB	78336	84176	12.09%	1.404%
2	1.532	147	153	167	rVB	76323	92280	13.25%	1.539%
3	2.060	308	317	332	rBV	148569	212536	30.52%	3.545%
4	2.449	429	438	448	rVB2	5139	8522	1.22%	0.142%
5	2.516	456	459	462	rBV	407	290	0.04%	0.005%
6	2.619	488	491	496	rVB2	377	246	0.04%	0.004%
7	2.761	531	535	536	rBV	303	191	0.03%	0.003%
8	2.799	544	547	550	rBV	203	181	0.03%	0.003%
9	2.915	581	583	584	rBV	286	125	0.02%	0.002%
10	3.217	673	677	679	rBV2	456	318	0.05%	0.005%
11	3.246	683	686	689	rBB2	200	101	0.01%	0.002%
12	3.269	689	693	695	rBV	367	335	0.05%	0.006%
13	3.314	703	707	710	rBV2	207	210	0.03%	0.004%
14	3.343	710	716	718	rBV2	394	392	0.06%	0.007%
15	3.426	740	742	746	rVB2	127	38	0.01%	0.001%
16	3.558	782	783	784	rBV2	112	32	0.00%	0.001%
17	3.568	784	786	787	rVV2	153	49	0.01%	0.001%
18	3.609	795	799	802	rBV2	238	248	0.04%	0.004%
19	3.651	810	812	814	rVB	300	144	0.02%	0.002%
20	3.664	814	816	817	rBV	228	112	0.02%	0.002%
21	3.687	821	823	826	rVV2	229	140	0.02%	0.002%
22	3.712	829	831	834	rVB	288	149	0.02%	0.002%
23	3.793	844	856	894	rBV2	71628	207141	29.75%	3.455%
24	4.252	983	999	1024	rBV2	124574	319545	45.89%	5.330%
25	4.558	1091	1094	1097	rVB2	511	282	0.04%	0.005%
26	4.584	1097	1102	1105	rBV3	554	411	0.06%	0.007%
27	4.761	1155	1157	1160	rBV	232	135	0.02%	0.002%
28	4.847	1182	1184	1188	rVB2	375	153	0.02%	0.003%
29	4.892	1196	1198	1201	rBV	241	83	0.01%	0.001%
30	4.960	1202	1219	1249	rBV2	260813	694476	99.73%	11.585%
31	5.346	1337	1339	1340	rBV2	256	105	0.02%	0.002%
32	5.368	1345	1346	1350	rVV2	322	202	0.03%	0.003%
33	5.400	1354	1356	1358	rBV	216	74	0.01%	0.001%
34	5.449	1369	1371	1373	rBV	195	130	0.02%	0.002%
35	5.539	1386	1399	1425	rBV	236097	492938	70.79%	8.223%
36	5.783	1472	1475	1477	rBV3	369	219	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070623\
 Data File : VV031644.D
 Acq On : 06 Jul 2023 10:13
 Operator : SY/MD
 Sample : VV0706MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK365

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

37	5.831	1480	1490	1504	rVV3	6423	13284	1.91%	0.222%
38	5.992	1527	1540	1561	rBV	168487	349160	50.14%	5.824%
39	6.391	1661	1664	1665	rBV	312	134	0.02%	0.002%
40	6.436	1676	1678	1680	rBV2	346	160	0.02%	0.003%
41	6.474	1687	1690	1694	rBV2	318	326	0.05%	0.005%
42	6.526	1704	1706	1709	rVB2	298	137	0.02%	0.002%
43	6.564	1714	1718	1723	rBV4	526	741	0.11%	0.012%
44	6.632	1737	1739	1742	rBV	339	188	0.03%	0.003%
45	6.648	1742	1744	1746	rVV2	200	94	0.01%	0.002%
46	6.719	1764	1766	1768	rBV	227	138	0.02%	0.002%
47	6.731	1768	1770	1774	rVB	411	244	0.04%	0.004%
48	6.815	1794	1796	1799	rBV2	274	178	0.03%	0.003%
49	6.841	1801	1804	1807	rBV2	632	526	0.08%	0.009%
50	6.918	1816	1828	1852	rBV	79675	154304	22.16%	2.574%
51	7.149	1897	1900	1903	rBV2	396	238	0.03%	0.004%
52	7.249	1918	1931	1953	rBV	248523	450269	64.66%	7.511%
53	7.558	2016	2027	2046	rBV2	61049	111898	16.07%	1.867%
54	7.731	2079	2081	2084	rBV4	337	239	0.03%	0.004%
55	7.793	2098	2100	2102	rVB	373	132	0.02%	0.002%
56	7.866	2118	2123	2124	rBV2	382	273	0.04%	0.005%
57	7.915	2133	2138	2143	rBV4	864	1060	0.15%	0.018%
58	7.953	2148	2150	2151	rBV4	127	32	0.00%	0.001%
59	8.030	2163	2174	2207	rBV	218808	398566	57.24%	6.649%
60	8.407	2290	2291	2295	rVB	299	93	0.01%	0.002%
61	8.426	2295	2297	2298	rBV	278	135	0.02%	0.002%
62	8.448	2303	2304	2306	rVB	533	148	0.02%	0.002%
63	8.561	2337	2339	2342	rBV2	317	191	0.03%	0.003%
64	8.622	2355	2358	2361	rBV3	263	215	0.03%	0.004%
65	8.670	2371	2373	2375	rBV	544	239	0.03%	0.004%
66	8.702	2380	2383	2385	rBV	270	206	0.03%	0.003%
67	8.731	2391	2392	2395	rVB	293	103	0.01%	0.002%
68	8.789	2399	2410	2441	rBV	369205	616070	88.47%	10.277%
69	9.001	2474	2476	2480	rVB	354	213	0.03%	0.004%
70	9.024	2480	2483	2484	rBV	212	97	0.01%	0.002%
71	9.069	2496	2497	2501	rBV3	393	313	0.04%	0.005%
72	9.182	2530	2532	2537	rBV	361	226	0.03%	0.004%
73	9.214	2540	2542	2546	rVB3	362	140	0.02%	0.002%
74	9.336	2578	2580	2581	rBV3	142	45	0.01%	0.001%
75	9.429	2607	2609	2613	rBV3	318	164	0.02%	0.003%
76	9.500	2623	2631	2634	rBV6	1077	1482	0.21%	0.025%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070623\
 Data File : VV031644.D
 Acq On : 06 Jul 2023 10:13
 Operator : SY/MD
 Sample : VV0706MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK365

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M

Title : VOC Analysis

77	9.834	2733	2735	2737	rVB6	296	104	0.01%	0.002%
78	9.866	2742	2745	2748	rBV3	855	708	0.10%	0.012%
79	9.982	2776	2781	2783	rBV	360	281	0.04%	0.005%
80	10.159	2824	2836	2860	rBV	264952	420186	60.34%	7.009%
81	10.599	2971	2973	2974	rBV	305	126	0.02%	0.002%
82	10.625	2978	2981	2986	rBV3	432	381	0.05%	0.006%
83	11.133	3130	3139	3144	rBV7	2173	3548	0.51%	0.059%
84	11.191	3146	3157	3181	rVV	447170	696355	100.00%	11.616%
85	11.403	3220	3223	3224	rBV2	469	279	0.04%	0.005%
86	11.506	3253	3255	3257	rBV2	358	160	0.02%	0.003%
87	11.567	3263	3274	3295	rBV	382113	612953	88.02%	10.225%
88	12.593	3587	3593	3602	rVB8	2701	3902	0.56%	0.065%
89	13.207	3778	3784	3795	rVB6	4439	6969	1.00%	0.116%
90	13.448	3851	3859	3875	rVB2	13764	20770	2.98%	0.346%
91	13.689	3927	3934	3942	rVB4	6375	8889	1.28%	0.148%




Sum of corrected areas: 5994721

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070623\
Data File : VV031644.D
Acq On : 06 Jul 2023 10:13
Operator : SY/MD
Sample : VV0706MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK365

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

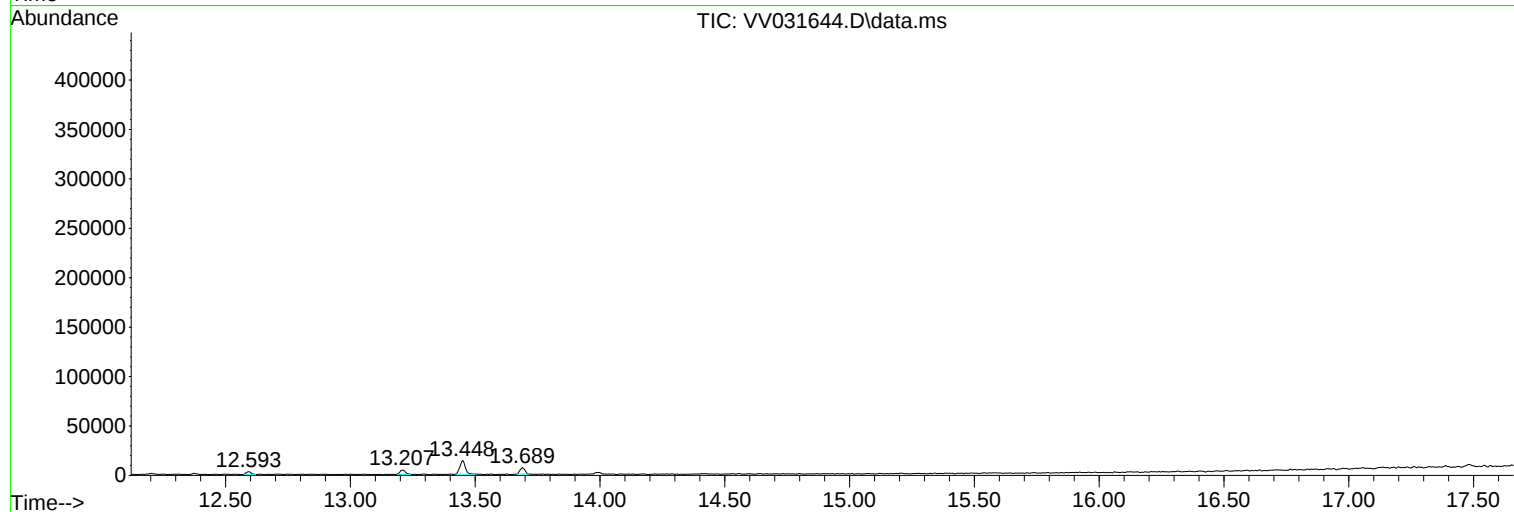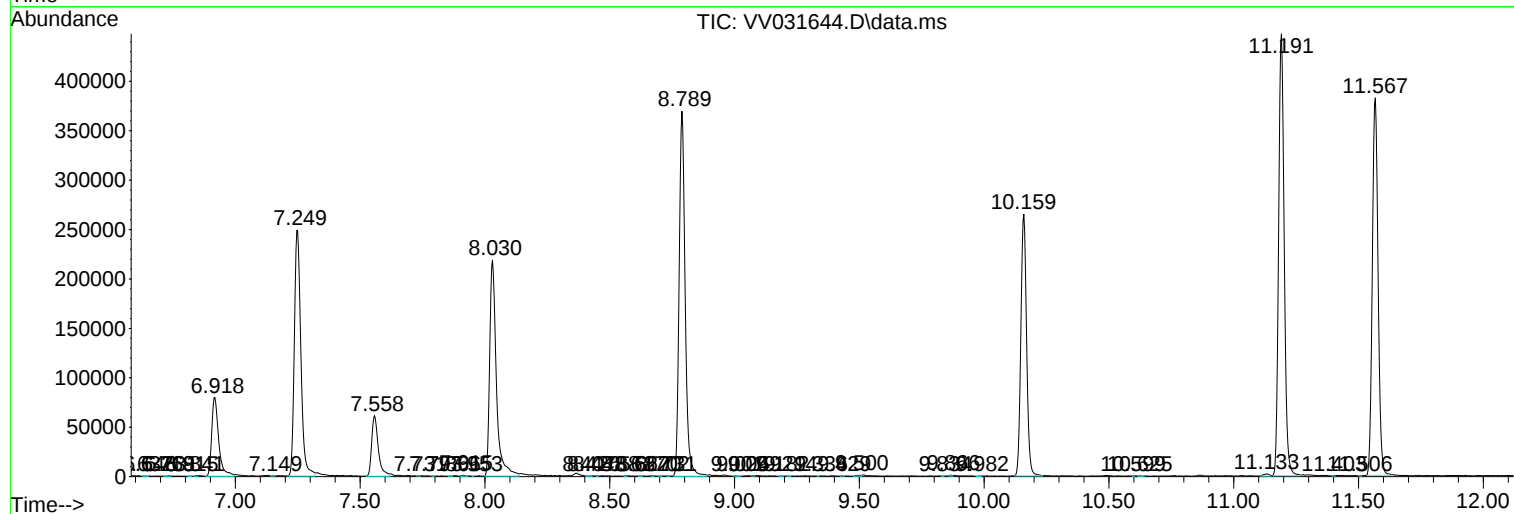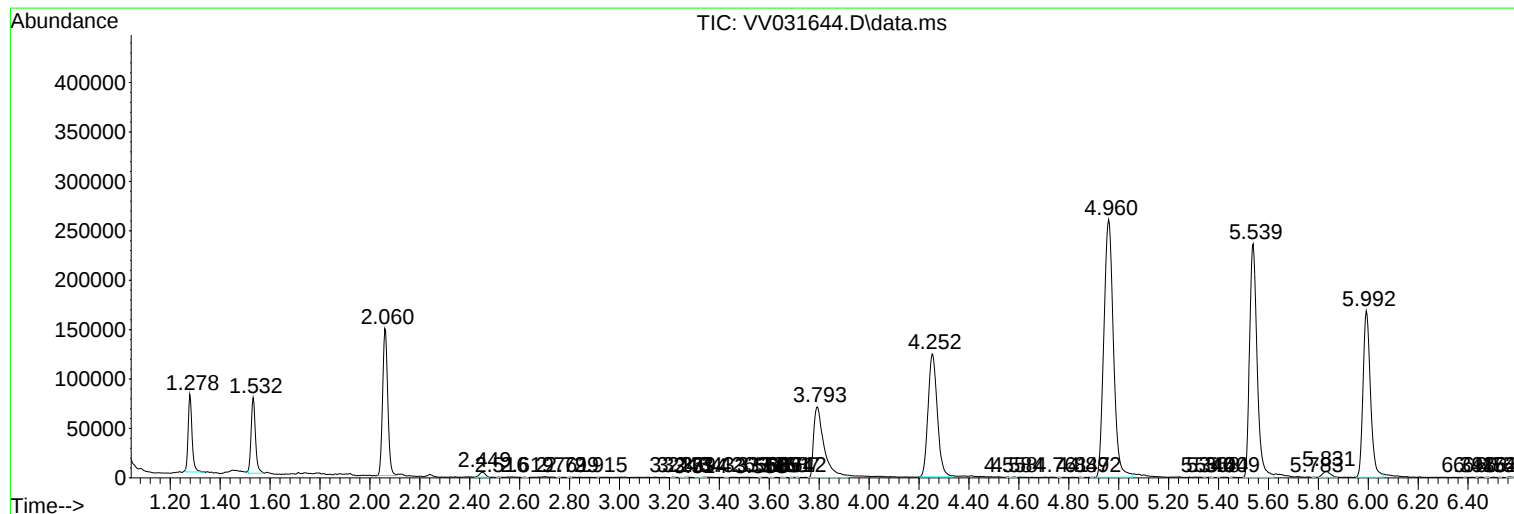

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070623\
Data File : VV031644.D
Acq On : 06 Jul 2023 10:13
Operator : SY/MD
Sample : VV0706MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK365

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070623\
Data File : VV031644.D
Acq On : 06 Jul 2023 10:13
Operator : SY/MD
Sample : VV0706MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK365

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc