

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070623\
 Data File : VV031645.D
 Acq On : 06 Jul 2023 11:07
 Operator : SY/MD
 Sample : 03504-01ME
 Misc : 3.83g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A46R7ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

Signal : TIC: VV031645.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	91	rVB	53923	77431	10.19%	1.374%
2	2.043	303	312	329	rVB	126406	182590	24.03%	3.240%
3	2.381	408	417	430	rBV	23939	45451	5.98%	0.806%
4	2.786	541	543	546	rBV	295	144	0.02%	0.003%
5	2.799	546	547	548	rVV	329	118	0.02%	0.002%
6	2.825	552	555	562	rVB3	289	234	0.03%	0.004%
7	2.892	570	576	577	rBV3	1124	1194	0.16%	0.021%
8	2.969	599	600	602	rBV2	248	108	0.01%	0.002%
9	3.002	608	610	612	rBV2	332	134	0.02%	0.002%
10	3.069	628	631	633	rBV	246	176	0.02%	0.003%
11	3.108	641	643	647	rVB2	394	232	0.03%	0.004%
12	3.162	656	660	662	rVB3	210	130	0.02%	0.002%
13	3.182	662	666	668	rBV2	355	212	0.03%	0.004%
14	3.256	684	689	691	rBV	365	297	0.04%	0.005%
15	3.272	691	694	695	rBV	327	151	0.02%	0.003%
16	3.288	695	699	702	rVV3	303	215	0.03%	0.004%
17	3.323	707	710	711	rBV	259	123	0.02%	0.002%
18	3.355	716	720	722	rBV	221	184	0.02%	0.003%
19	3.551	778	781	785	rBV	137	99	0.01%	0.002%
20	3.622	802	803	805	rBV	260	114	0.02%	0.002%
21	3.654	809	813	814	rBV	209	167	0.02%	0.003%
22	3.706	826	829	830	rBV2	186	107	0.01%	0.002%
23	3.754	839	844	847	rBV2	329	378	0.05%	0.007%
24	3.802	850	859	890	rBV2	43406	156117	20.55%	2.770%
25	4.191	978	980	982	rBV2	444	211	0.03%	0.004%
26	4.252	983	999	1028	rVV	108887	283873	37.37%	5.036%
27	4.484	1065	1071	1073	rBV3	574	392	0.05%	0.007%
28	4.519	1077	1082	1085	rBV3	488	508	0.07%	0.009%
29	4.584	1098	1102	1105	rBV3	395	344	0.05%	0.006%
30	4.629	1112	1116	1120	rBV4	730	640	0.08%	0.011%
31	4.719	1141	1144	1147	rBV2	273	204	0.03%	0.004%
32	4.767	1156	1159	1162	rBV2	194	128	0.02%	0.002%
33	4.786	1162	1165	1169	rVV2	197	187	0.02%	0.003%
34	4.805	1169	1171	1174	rVB	310	127	0.02%	0.002%
35	4.822	1174	1176	1177	rBV	228	104	0.01%	0.002%
36	4.957	1202	1218	1246	rBV3	238227	617736	81.31%	10.960%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070623\
 Data File : VV031645.D
 Acq On : 06 Jul 2023 11:07
 Operator : SY/MD
 Sample : 03504-01ME
 Misc : 3.83g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A46R7ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

37	5.175	1283	1286	1289	rVB2	565	319	0.04%	0.006%
38	5.201	1289	1294	1295	rBV	499	315	0.04%	0.006%
39	5.358	1338	1343	1347	rBV	319	348	0.05%	0.006%
40	5.426	1361	1364	1366	rBV2	238	151	0.02%	0.003%
41	5.539	1384	1399	1426	rBV	261076	553310	72.83%	9.817%
42	5.834	1480	1491	1506	rVB6	5981	13293	1.75%	0.236%
43	5.934	1517	1522	1525	rBV3	267	254	0.03%	0.005%
44	5.992	1526	1540	1564	rBV	146307	311390	40.99%	5.525%
45	6.153	1584	1590	1593	rVB5	874	739	0.10%	0.013%
46	6.182	1597	1599	1604	rVB2	656	332	0.04%	0.006%
47	6.374	1655	1659	1664	rVB2	345	270	0.04%	0.005%
48	6.413	1668	1671	1673	rBV2	322	234	0.03%	0.004%
49	6.500	1694	1698	1700	rVB	232	102	0.01%	0.002%
50	6.532	1704	1708	1710	rBV2	290	216	0.03%	0.004%
51	6.731	1768	1770	1775	rVB2	372	198	0.03%	0.004%
52	6.792	1786	1789	1790	rBV	245	121	0.02%	0.002%
53	6.857	1806	1809	1817	rBV2	200	246	0.03%	0.004%
54	6.918	1817	1828	1849	rBV2	69997	140011	18.43%	2.484%
55	7.127	1891	1893	1894	rBV2	310	161	0.02%	0.003%
56	7.169	1903	1906	1907	rBV3	315	173	0.02%	0.003%
57	7.191	1910	1913	1916	rBV2	625	601	0.08%	0.011%
58	7.249	1921	1931	1950	rVV	219471	387621	51.02%	6.877%
59	7.503	2008	2010	2016	rVB2	388	332	0.04%	0.006%
60	7.561	2016	2028	2056	rBV2	51710	105775	13.92%	1.877%
61	7.870	2120	2124	2125	rBV	437	271	0.04%	0.005%
62	7.947	2145	2148	2151	rBV	348	186	0.02%	0.003%
63	8.046	2167	2179	2201	rBV2	144267	350905	46.19%	6.226%
64	8.596	2348	2350	2354	rBV2	186	97	0.01%	0.002%
65	8.709	2383	2385	2387	rBV	193	98	0.01%	0.002%
66	8.792	2398	2411	2438	rBV	401643	689408	90.75%	12.232%
67	8.998	2472	2475	2478	rBV3	468	276	0.04%	0.005%
68	9.037	2484	2487	2488	rBV2	401	257	0.03%	0.005%
69	9.079	2498	2500	2501	rBV2	323	127	0.02%	0.002%
70	9.095	2501	2505	2509	rVV4	719	640	0.08%	0.011%
71	9.178	2528	2531	2535	rVB	288	231	0.03%	0.004%
72	9.291	2562	2566	2570	rBV	553	458	0.06%	0.008%
73	9.316	2570	2574	2577	rVV	330	240	0.03%	0.004%
74	9.442	2611	2613	2614	rBV	266	106	0.01%	0.002%
75	9.484	2625	2626	2629	rBV2	347	195	0.03%	0.003%
76	9.519	2635	2637	2640	rVB2	566	256	0.03%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070623\
 Data File : VV031645.D
 Acq On : 06 Jul 2023 11:07
 Operator : SY/MD
 Sample : 03504-01ME
 Misc : 3.83g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A46R7ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

77	9.554	2646	2648	2650	rBV2	192	113	0.01%	0.002%
78	9.571	2650	2653	2655	rVV	253	140	0.02%	0.002%
79	9.596	2659	2661	2663	rBV2	292	146	0.02%	0.003%
80	9.718	2695	2699	2703	rBV3	470	571	0.08%	0.010%
81	9.808	2725	2727	2731	rVB2	353	155	0.02%	0.003%
82	9.850	2735	2740	2743	rVB3	725	688	0.09%	0.012%
83	9.905	2755	2757	2764	rVB2	403	287	0.04%	0.005%
84	10.162	2824	2837	2859	rBV	245091	402098	52.93%	7.134%
85	10.329	2883	2889	2895	rBV3	939	1271	0.17%	0.023%
86	10.400	2909	2911	2912	rBV3	219	97	0.01%	0.002%
87	10.439	2919	2923	2924	rBV2	270	219	0.03%	0.004%
88	10.490	2936	2939	2943	rVB	586	460	0.06%	0.008%
89	10.606	2973	2975	2977	rVB	275	119	0.02%	0.002%
90	10.664	2989	2993	2994	rBV	186	119	0.02%	0.002%
91	10.866	3052	3056	3059	rBV3	558	502	0.07%	0.009%
92	10.911	3066	3070	3071	rBV2	419	256	0.03%	0.005%
93	10.972	3084	3089	3093	rBV2	420	509	0.07%	0.009%
94	11.194	3146	3158	3178	rBV	481978	759716	100.00%	13.479%
95	11.384	3214	3217	3220	rBV3	401	226	0.03%	0.004%
96	11.570	3258	3275	3293	rBV	344724	536596	70.63%	9.520%
97	11.969	3397	3399	3402	rBV3	435	279	0.04%	0.005%
98	13.120	3755	3757	3760	rBV	463	253	0.03%	0.004%
99	13.779	3959	3962	3964	rBV2	641	413	0.05%	0.007%
100	14.197	4089	4092	4093	rBV	472	267	0.04%	0.005%


Sum of corrected areas: 5636323

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070623\
Data File : VV031645.D
Acq On : 06 Jul 2023 11:07
Operator : SY/MD
Sample : 03504-01ME
Misc : 3.83g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A46R7ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

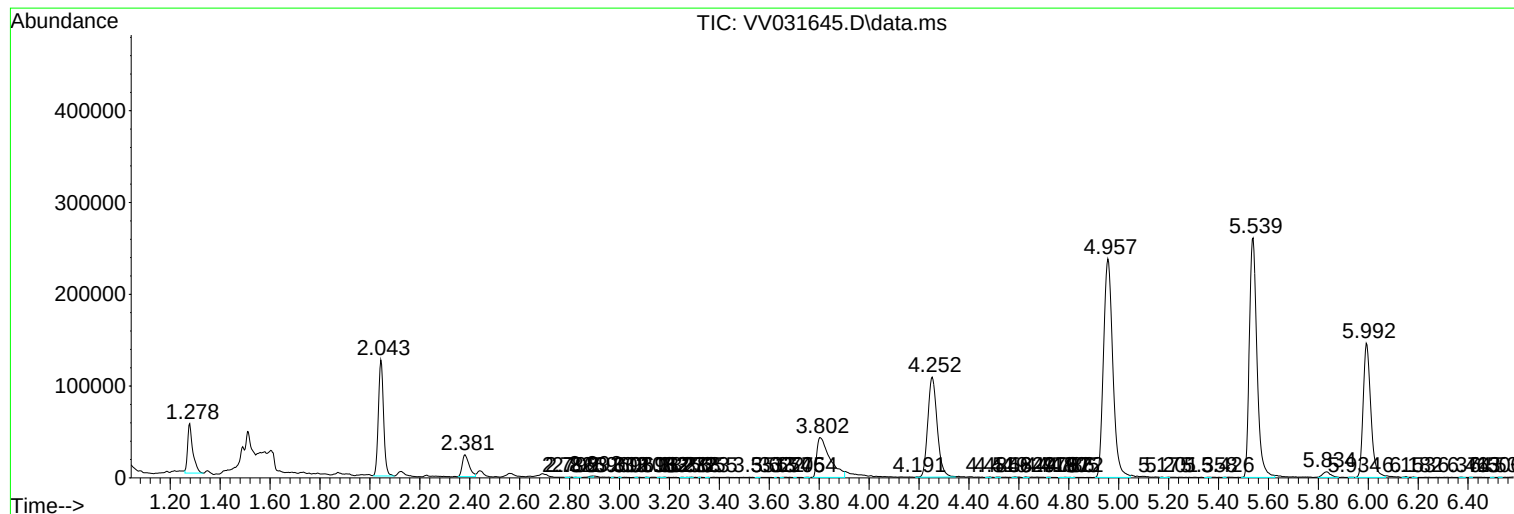

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070623\
Data File : VV031645.D
Acq On : 06 Jul 2023 11:07
Operator : SY/MD
Sample : 03504-01ME
Misc : 3.83g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A46R7ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070623\
Data File : VV031645.D
Acq On : 06 Jul 2023 11:07
Operator : SY/MD
Sample : 03504-01ME
Misc : 3.83g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A46R7ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc