

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070623\
 Data File : VV031646.D
 Acq On : 06 Jul 2023 11:30
 Operator : SY/MD
 Sample : 03504-04ME
 Misc : 4.39g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A46T4ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

Signal : TIC: VV031646.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	90	rVB	51516	72205	10.02%	1.270%
2	2.043	302	312	325	rBV	128966	190089	26.39%	3.345%
3	2.381	409	417	428	rBV	16692	29471	4.09%	0.519%
4	2.558	460	472	482	rBV2	9151	20015	2.78%	0.352%
5	2.706	515	518	523	rVB3	850	747	0.10%	0.013%
6	2.757	532	534	538	rVB3	339	243	0.03%	0.004%
7	2.789	538	544	545	rBV3	352	352	0.05%	0.006%
8	2.818	550	553	555	rBV	368	249	0.03%	0.004%
9	2.863	564	567	571	rBV3	563	462	0.06%	0.008%
10	2.886	571	574	577	rBV3	625	452	0.06%	0.008%
11	2.976	599	602	605	rVB2	240	155	0.02%	0.003%
12	3.092	636	638	641	rVB2	218	125	0.02%	0.002%
13	3.149	652	656	660	rBV	517	423	0.06%	0.007%
14	3.307	702	705	708	rBV2	232	153	0.02%	0.003%
15	3.352	714	719	720	rBV	245	188	0.03%	0.003%
16	3.381	725	728	733	rBV	225	189	0.03%	0.003%
17	3.445	744	748	752	rBV3	395	374	0.05%	0.007%
18	3.532	773	775	779	rVB	261	186	0.03%	0.003%
19	3.558	779	783	784	rBV	251	149	0.02%	0.003%
20	3.609	796	799	800	rBV	334	151	0.02%	0.003%
21	3.706	827	829	836	rVB2	260	132	0.02%	0.002%
22	3.735	836	838	845	rVB3	180	161	0.02%	0.003%
23	3.802	849	859	894	rBV2	49723	172804	23.99%	3.041%
24	4.252	982	999	1024	rBV	109043	287510	39.91%	5.059%
25	4.455	1060	1062	1065	rBV2	370	246	0.03%	0.004%
26	4.571	1096	1098	1101	rVB2	335	180	0.02%	0.003%
27	4.616	1110	1112	1116	rVB2	318	197	0.03%	0.003%
28	4.683	1131	1133	1136	rVB	216	135	0.02%	0.002%
29	4.709	1136	1141	1145	rBV3	423	439	0.06%	0.008%
30	4.841	1180	1182	1188	rVB2	366	238	0.03%	0.004%
31	4.873	1188	1192	1194	rBV	228	191	0.03%	0.003%
32	4.956	1202	1218	1253	rBV3	244122	635077	88.15%	11.174%
33	5.262	1309	1313	1315	rBV	242	156	0.02%	0.003%
34	5.294	1319	1323	1325	rBV2	282	191	0.03%	0.003%
35	5.355	1340	1342	1347	rVB2	267	151	0.02%	0.003%
36	5.538	1385	1399	1429	rBV	247557	527006	73.15%	9.273%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070623\
 Data File : VV031646.D
 Acq On : 06 Jul 2023 11:30
 Operator : SY/MD
 Sample : 03504-04ME
 Misc : 4.39g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A46T4ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

37	5.789	1474	1477	1480	rVB2	546	367	0.05%	0.006%
38	5.834	1480	1491	1504	rVV6	6997	14939	2.07%	0.263%
39	5.992	1527	1540	1568	rBV	149628	321891	44.68%	5.664%
40	6.182	1596	1599	1600	rBV2	318	176	0.02%	0.003%
41	6.320	1639	1642	1644	rBV	183	134	0.02%	0.002%
42	6.333	1644	1646	1649	rVB2	303	128	0.02%	0.002%
43	6.355	1651	1653	1657	rVB	297	119	0.02%	0.002%
44	6.413	1669	1671	1674	rVB2	451	207	0.03%	0.004%
45	6.445	1677	1681	1683	rBV	389	264	0.04%	0.005%
46	6.458	1683	1685	1690	rVV3	271	201	0.03%	0.004%
47	6.519	1701	1704	1708	rBV2	411	212	0.03%	0.004%
48	6.587	1719	1725	1727	rBV2	753	751	0.10%	0.013%
49	6.696	1757	1759	1761	rBV2	360	184	0.03%	0.003%
50	6.744	1772	1774	1780	rVB3	270	193	0.03%	0.003%
51	6.783	1783	1786	1787	rBV2	201	118	0.02%	0.002%
52	6.879	1810	1816	1817	rBV	235	196	0.03%	0.003%
53	6.918	1818	1828	1848	rBV	71048	140977	19.57%	2.481%
54	7.098	1882	1884	1889	rBV2	313	245	0.03%	0.004%
55	7.130	1889	1894	1896	rBV4	449	288	0.04%	0.005%
56	7.185	1906	1911	1919	rBV6	830	887	0.12%	0.016%
57	7.249	1919	1931	1948	rBV	224810	407282	56.53%	7.166%
58	7.561	2018	2028	2047	rBV2	52173	103774	14.40%	1.826%
59	7.725	2074	2079	2082	rBV5	472	425	0.06%	0.007%
60	7.760	2086	2090	2091	rBV2	454	319	0.04%	0.006%
61	7.972	2154	2156	2161	rVB	328	130	0.02%	0.002%
62	8.043	2166	2178	2206	rBV2	165504	383705	53.26%	6.751%
63	8.612	2353	2355	2358	rBV	343	244	0.03%	0.004%
64	8.657	2366	2369	2376	rVB4	766	613	0.09%	0.011%
65	8.747	2394	2397	2398	rBV2	205	129	0.02%	0.002%
66	8.792	2398	2411	2441	rVV	387238	662512	91.96%	11.657%
67	8.995	2471	2474	2478	rBV3	557	447	0.06%	0.008%
68	9.069	2495	2497	2501	rBV	316	266	0.04%	0.005%
69	9.091	2501	2504	2511	rVB4	477	576	0.08%	0.010%
70	9.143	2517	2520	2522	rBV	286	196	0.03%	0.003%
71	9.242	2549	2551	2557	rBV3	275	273	0.04%	0.005%
72	9.275	2559	2561	2566	rVB3	277	170	0.02%	0.003%
73	9.365	2587	2589	2594	rBV2	326	246	0.03%	0.004%
74	9.394	2595	2598	2599	rBV	222	133	0.02%	0.002%
75	9.525	2637	2639	2641	rVB2	326	170	0.02%	0.003%
76	9.628	2668	2671	2672	rBV2	315	200	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070623\
 Data File : VV031646.D
 Acq On : 06 Jul 2023 11:30
 Operator : SY/MD
 Sample : 03504-04ME
 Misc : 4.39g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A46T4ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

77	9.718	2691	2699	2711	rBV5	1442	2881	0.40%	0.051%
78	9.834	2733	2735	2737	rVB	372	139	0.02%	0.002%
79	9.960	2770	2774	2775	rVV	344	194	0.03%	0.003%
80	9.982	2779	2781	2788	rVB2	419	280	0.04%	0.005%
81	10.162	2824	2837	2853	rBV	263695	428009	59.41%	7.531%
82	10.332	2882	2890	2891	rBV2	529	588	0.08%	0.010%
83	10.410	2910	2914	2918	rBV	300	226	0.03%	0.004%
84	10.583	2965	2968	2970	rBV2	330	184	0.03%	0.003%
85	10.599	2970	2973	2976	rVB	465	243	0.03%	0.004%
86	10.853	3050	3052	3054	rBV2	391	200	0.03%	0.004%
87	10.902	3064	3067	3070	rBV	303	212	0.03%	0.004%
88	10.921	3070	3073	3076	rVV3	422	290	0.04%	0.005%
89	10.959	3082	3085	3087	rBV2	363	257	0.04%	0.005%
90	11.004	3096	3099	3101	rBV	343	234	0.03%	0.004%
91	11.046	3106	3112	3114	rBV2	487	456	0.06%	0.008%
92	11.117	3133	3134	3136	rBV	418	149	0.02%	0.003%
93	11.133	3136	3139	3145	rVB2	769	613	0.09%	0.011%
94	11.194	3146	3158	3175	rBV	474376	720422	100.00%	12.676%
95	11.570	3263	3275	3294	rBV	337674	539948	74.95%	9.501%
96	12.490	3559	3561	3565	rBV2	510	398	0.06%	0.007%
97	13.082	3742	3745	3747	rBV	485	305	0.04%	0.005%
98	13.210	3781	3785	3787	rBV3	694	611	0.08%	0.011%
99	13.532	3882	3885	3887	rBV2	425	239	0.03%	0.004%
100	14.220	4095	4099	4103	rBV4	757	727	0.10%	0.013%




Sum of corrected areas: 5683284

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070623\
Data File : VV031646.D
Acq On : 06 Jul 2023 11:30
Operator : SY/MD
Sample : 03504-04ME
Misc : 4.39g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A46T4ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

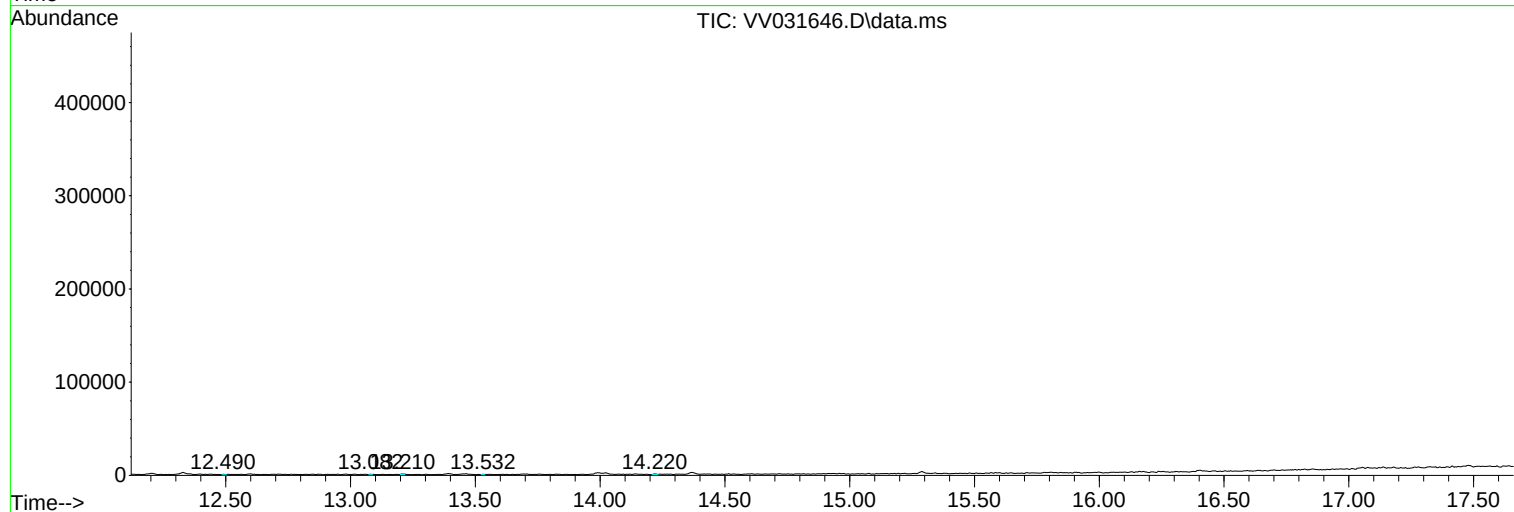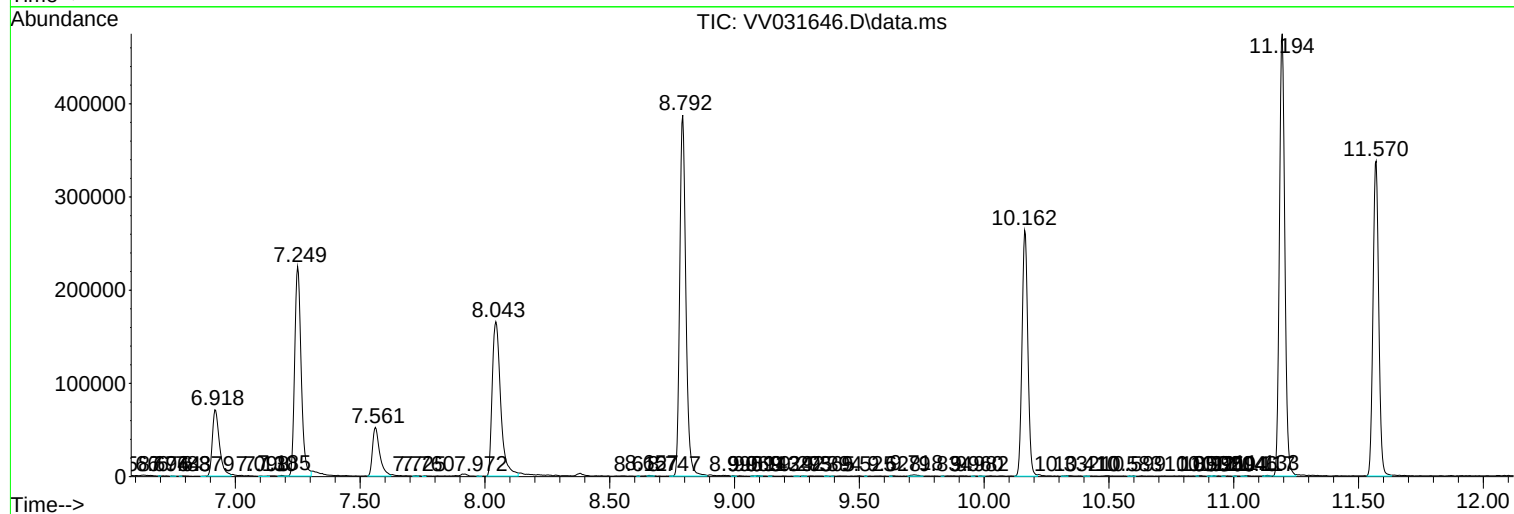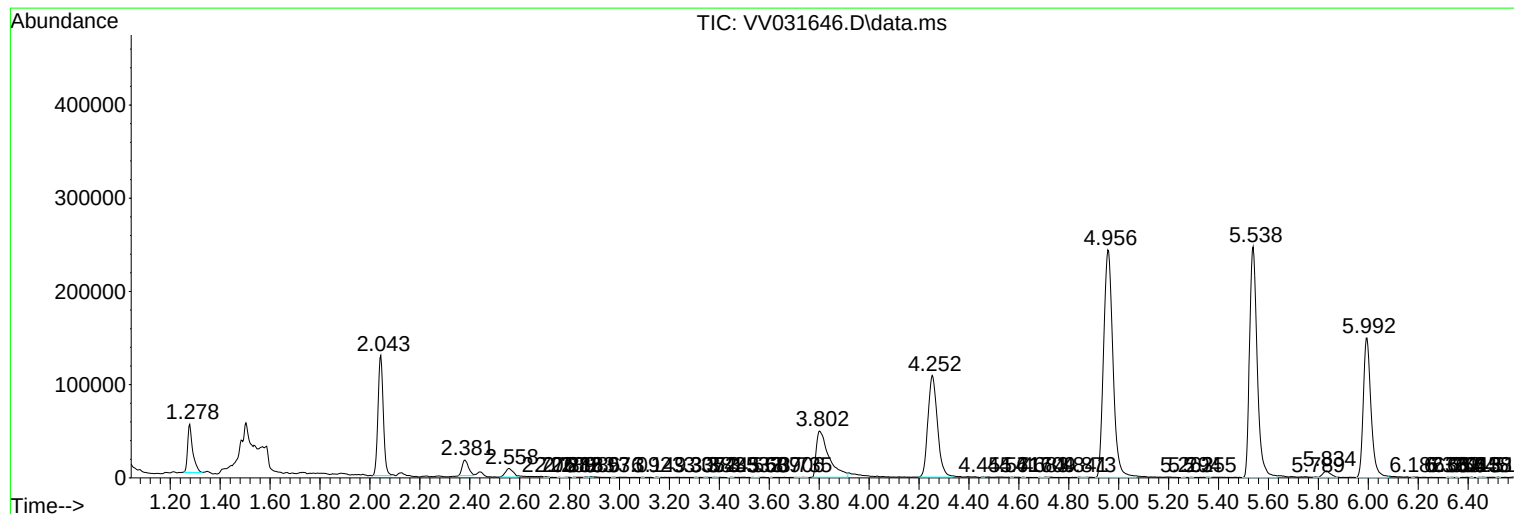

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070623\
Data File : VV031646.D
Acq On : 06 Jul 2023 11:30
Operator : SY/MD
Sample : 03504-04ME
Misc : 4.39g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A46T4ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070623\
Data File : VV031646.D
Acq On : 06 Jul 2023 11:30
Operator : SY/MD
Sample : 03504-04ME
Misc : 4.39g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A46T4ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc