

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070623\
 Data File : VV031648.D
 Acq On : 06 Jul 2023 12:17
 Operator : SY/MD
 Sample : 03444-12ME
 Misc : 4.27g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A46T6ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

Signal : TIC: VV031648.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	91	rVB	45485	67199	9.62%	1.261%
2	2.044	303	312	329	rVB	110079	161018	23.06%	3.021%
3	2.381	407	417	429	rBV	25711	47996	6.87%	0.901%
4	2.558	462	472	489	rBV2	9724	21492	3.08%	0.403%
5	2.818	551	553	555	rBV	229	115	0.02%	0.002%
6	2.835	556	558	560	rVB	300	81	0.01%	0.002%
7	2.883	564	573	576	rBV5	1385	1724	0.25%	0.032%
8	2.970	597	600	601	rBV2	343	189	0.03%	0.004%
9	2.992	605	607	610	rBV	158	109	0.02%	0.002%
10	3.005	610	611	616	rVB2	331	146	0.02%	0.003%
11	3.031	616	619	620	rBV	331	160	0.02%	0.003%
12	3.040	620	622	626	rVB2	312	181	0.03%	0.003%
13	3.143	652	654	656	rVB	210	87	0.01%	0.002%
14	3.159	656	659	662	rBV3	203	162	0.02%	0.003%
15	3.175	662	664	667	rBV2	289	218	0.03%	0.004%
16	3.236	680	683	684	rBV	209	86	0.01%	0.002%
17	3.246	684	686	691	rVB	407	244	0.03%	0.005%
18	3.278	691	696	699	rBV3	390	475	0.07%	0.009%
19	3.320	708	709	712	rBV2	185	119	0.02%	0.002%
20	3.391	728	731	735	rBV	111	74	0.01%	0.001%
21	3.436	742	745	748	rBV2	209	128	0.02%	0.002%
22	3.484	758	760	766	rVB2	412	310	0.04%	0.006%
23	3.513	766	769	774	rBV	367	288	0.04%	0.005%
24	3.613	796	800	802	rVB	255	160	0.02%	0.003%
25	3.626	802	804	805	rBV2	109	57	0.01%	0.001%
26	3.728	834	836	839	rBV	160	89	0.01%	0.002%
27	3.757	842	845	847	rBV3	280	170	0.02%	0.003%
28	3.802	849	859	887	rBV2	47992	157753	22.59%	2.960%
29	4.253	985	999	1027	rVB2	101799	263059	37.67%	4.936%
30	4.397	1041	1044	1047	rBV3	420	359	0.05%	0.007%
31	4.481	1067	1070	1071	rBV2	210	145	0.02%	0.003%
32	4.529	1083	1085	1087	rVB	353	141	0.02%	0.003%
33	4.564	1093	1096	1099	rBV	385	307	0.04%	0.006%
34	4.642	1117	1120	1121	rBV	427	204	0.03%	0.004%
35	4.671	1126	1129	1131	rBV	258	135	0.02%	0.003%
36	4.748	1150	1153	1157	rVB2	282	212	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070623\
 Data File : VV031648.D
 Acq On : 06 Jul 2023 12:17
 Operator : SY/MD
 Sample : 03444-12ME
 Misc : 4.27g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A46T6ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

37	4.770	1157	1160	1163	rBV2	105	95	0.01%	0.002%
38	4.822	1172	1176	1178	rBV3	282	223	0.03%	0.004%
39	4.873	1189	1192	1194	rVB2	244	113	0.02%	0.002%
40	4.889	1194	1197	1202	rBV2	243	210	0.03%	0.004%
41	4.957	1202	1218	1250	rBV2	222838	581008	83.20%	10.901%
42	5.124	1268	1270	1271	rBV	333	163	0.02%	0.003%
43	5.166	1281	1283	1285	rBV2	254	98	0.01%	0.002%
44	5.359	1341	1343	1345	rBV	190	105	0.02%	0.002%
45	5.397	1352	1355	1357	rBV2	247	117	0.02%	0.002%
46	5.410	1357	1359	1361	rBV	196	123	0.02%	0.002%
47	5.433	1365	1366	1371	rVB	248	138	0.02%	0.003%
48	5.455	1371	1373	1378	rBV	294	154	0.02%	0.003%
49	5.481	1378	1381	1384	rBV2	265	191	0.03%	0.004%
50	5.539	1387	1399	1426	rBV	238004	503742	72.13%	9.451%
51	5.831	1481	1490	1503	rBV4	6393	12447	1.78%	0.234%
52	5.995	1527	1541	1566	rBV	140967	302664	43.34%	5.679%
53	6.227	1612	1613	1615	rBV	403	178	0.03%	0.003%
54	6.317	1637	1641	1645	rBV2	296	204	0.03%	0.004%
55	6.336	1645	1647	1650	rBV	135	82	0.01%	0.002%
56	6.558	1713	1716	1717	rBV	176	93	0.01%	0.002%
57	6.568	1717	1719	1720	rVV	236	84	0.01%	0.002%
58	6.625	1734	1737	1738	rBV2	435	247	0.04%	0.005%
59	6.725	1765	1768	1770	rBV2	162	122	0.02%	0.002%
60	6.783	1783	1786	1787	rBV2	211	104	0.01%	0.002%
61	6.844	1802	1805	1810	rVB	368	295	0.04%	0.006%
62	6.870	1810	1813	1814	rBV	175	100	0.01%	0.002%
63	6.879	1814	1816	1817	rBV	238	81	0.01%	0.002%
64	6.921	1817	1829	1854	rBV	65251	131520	18.83%	2.468%
65	7.111	1885	1888	1895	rBV2	296	311	0.04%	0.006%
66	7.169	1903	1906	1907	rBV2	618	288	0.04%	0.005%
67	7.249	1921	1931	1949	rBV	200701	350843	50.24%	6.583%
68	7.506	2009	2011	2012	rBV	385	122	0.02%	0.002%
69	7.561	2019	2028	2054	rBV2	48170	96028	13.75%	1.802%
70	7.706	2070	2073	2074	rBV	312	137	0.02%	0.003%
71	7.744	2083	2085	2087	rBV2	315	135	0.02%	0.003%
72	7.989	2158	2161	2163	rBV2	202	120	0.02%	0.002%
73	8.043	2166	2178	2207	rBV	159239	369546	52.92%	6.934%
74	8.346	2269	2272	2275	rVB2	454	264	0.04%	0.005%
75	8.448	2303	2304	2305	rBV2	160	49	0.01%	0.001%
76	8.603	2349	2352	2355	rBV	330	272	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070623\
 Data File : VV031648.D
 Acq On : 06 Jul 2023 12:17
 Operator : SY/MD
 Sample : 03444-12ME
 Misc : 4.27g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A46T6ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

77	8.632	2358	2361	2362	rBV2	199	111	0.02%	0.002%
78	8.693	2378	2380	2381	rVB2	250	54	0.01%	0.001%
79	8.793	2398	2411	2430	rBV	378732	644990	92.36%	12.102%
80	9.024	2480	2483	2484	rBV2	393	193	0.03%	0.004%
81	9.137	2516	2518	2519	rBV2	167	55	0.01%	0.001%
82	9.188	2531	2534	2537	rBV2	329	210	0.03%	0.004%
83	9.362	2585	2588	2589	rBV	326	158	0.02%	0.003%
84	9.487	2624	2627	2630	rBV2	506	279	0.04%	0.005%
85	9.510	2632	2634	2636	rBV	309	176	0.03%	0.003%
86	9.725	2692	2701	2707	rBV4	808	1488	0.21%	0.028%
87	10.005	2786	2788	2793	rVB	411	163	0.02%	0.003%
88	10.085	2808	2813	2815	rBV2	242	195	0.03%	0.004%
89	10.120	2822	2824	2825	rBV	334	149	0.02%	0.003%
90	10.162	2825	2837	2859	rVV	245617	398479	57.06%	7.476%
91	10.272	2869	2871	2874	rBV2	324	209	0.03%	0.004%
92	10.329	2887	2889	2891	rBV	343	161	0.02%	0.003%
93	10.362	2896	2899	2903	rBV	511	274	0.04%	0.005%
94	10.899	3063	3066	3069	rVB2	309	140	0.02%	0.003%
95	11.037	3107	3109	3112	rVB	432	180	0.03%	0.003%
96	11.063	3112	3117	3119	rBV	361	295	0.04%	0.006%
97	11.194	3147	3158	3177	rBV	452949	698363	100.00%	13.103%
98	11.567	3262	3274	3296	rBV	315199	501501	71.81%	9.409%
99	13.210	3780	3785	3791	rBV4	1362	1391	0.20%	0.026%
100	14.371	4140	4146	4154	rBV4	1656	2411	0.35%	0.045%




Sum of corrected areas: 5329833

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070623\
Data File : VV031648.D
Acq On : 06 Jul 2023 12:17
Operator : SY/MD
Sample : 03444-12ME
Misc : 4.27g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A46T6ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

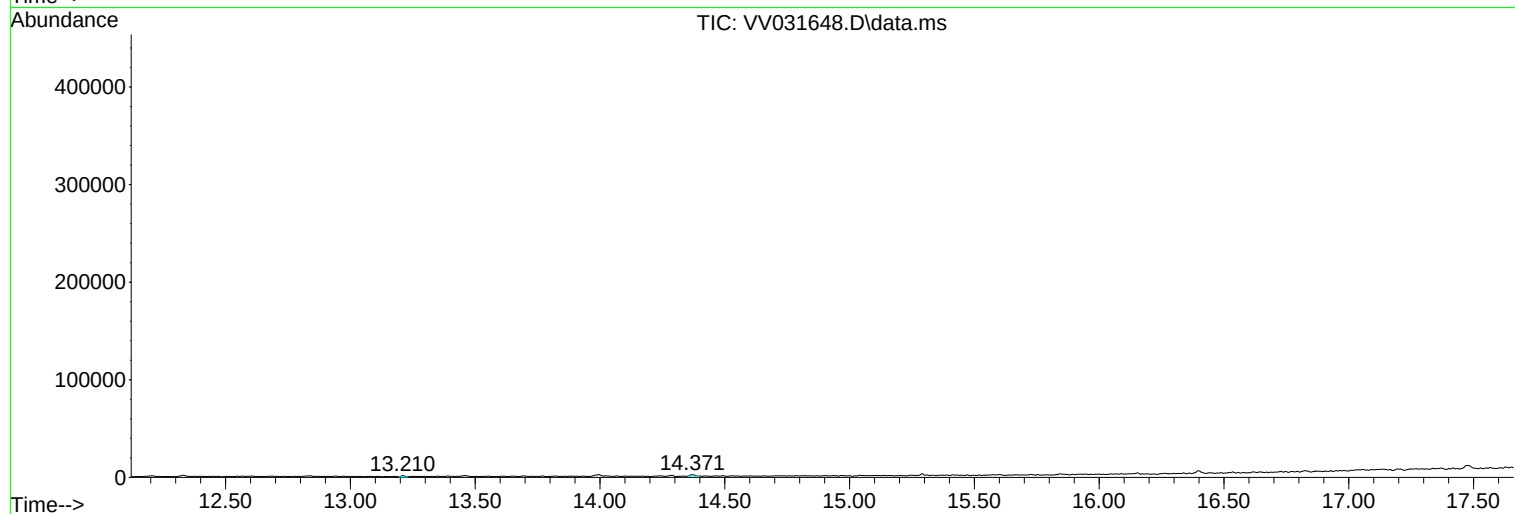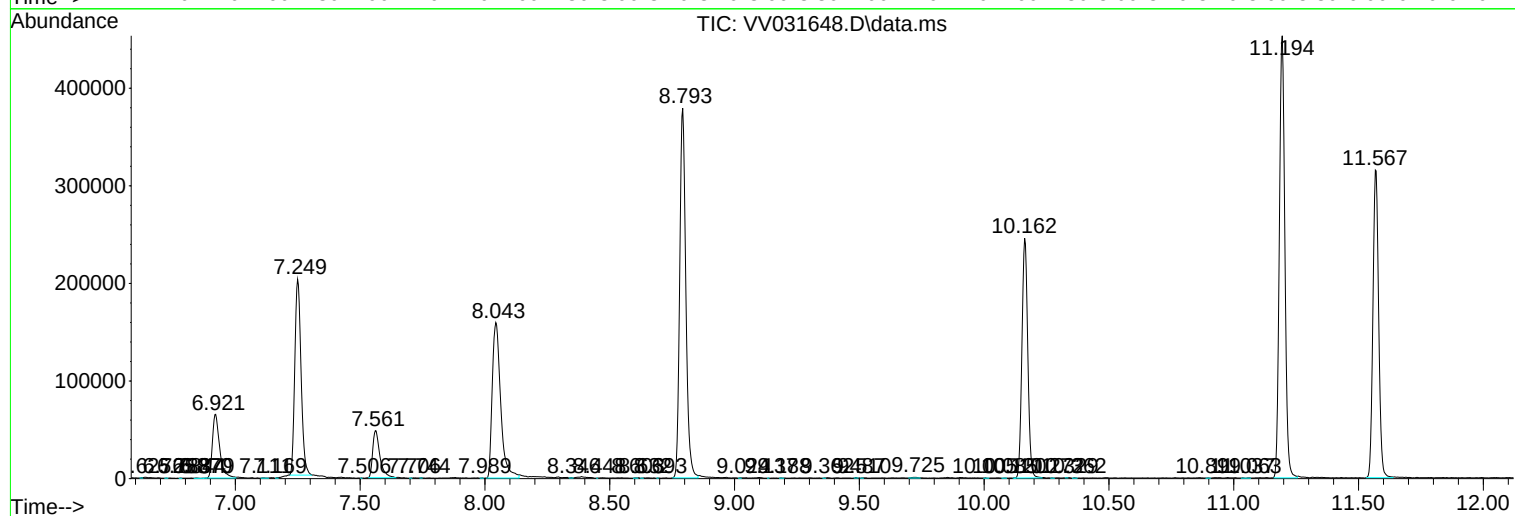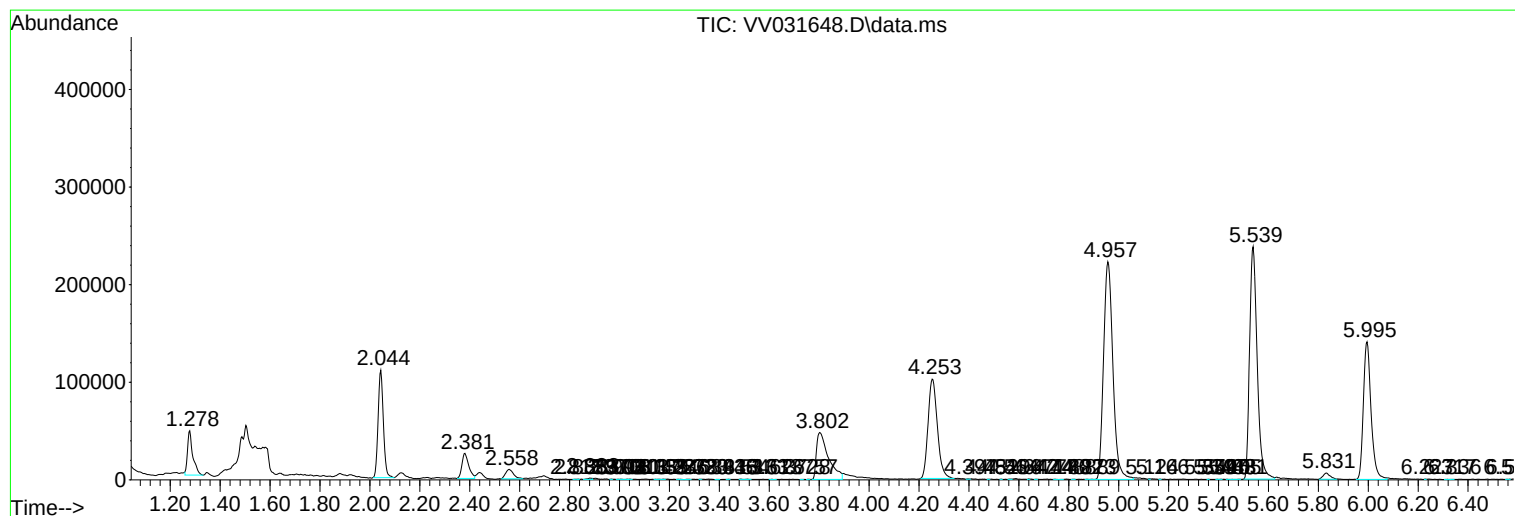

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070623\
Data File : VV031648.D
Acq On : 06 Jul 2023 12:17
Operator : SY/MD
Sample : 03444-12ME
Misc : 4.27g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A46T6ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070623\
Data File : VV031648.D
Acq On : 06 Jul 2023 12:17
Operator : SY/MD
Sample : 03444-12ME
Misc : 4.27g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A46T6ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc