

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070623\
 Data File : VV031649.D
 Acq On : 06 Jul 2023 12:40
 Operator : SY/MD
 Sample : 03501-08ME
 Misc : 5.77g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A46X3ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

Signal : TIC: VV031649.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	92	rVB	47736	68324	9.19%	1.227%
2	2.044	302	312	328	rBV	114015	167744	22.56%	3.012%
3	2.381	408	417	429	rBV2	17604	33108	4.45%	0.594%
4	2.558	458	472	486	rBV2	12692	31368	4.22%	0.563%
5	2.777	536	540	542	rBV3	429	350	0.05%	0.006%
6	2.873	568	570	571	rBV	505	235	0.03%	0.004%
7	2.950	590	594	601	rBV	291	277	0.04%	0.005%
8	2.979	601	603	606	rBV2	234	159	0.02%	0.003%
9	3.111	641	644	650	rVB2	204	182	0.02%	0.003%
10	3.175	662	664	665	rBV2	183	81	0.01%	0.001%
11	3.208	672	674	677	rVB	259	107	0.01%	0.002%
12	3.230	677	681	684	rBV3	293	262	0.04%	0.005%
13	3.262	690	691	692	rBV3	106	30	0.00%	0.001%
14	3.310	704	706	708	rBV	81	43	0.01%	0.001%
15	3.327	708	711	714	rVB	227	131	0.02%	0.002%
16	3.359	718	721	726	rVB2	281	198	0.03%	0.004%
17	3.442	744	747	749	rBV2	240	170	0.02%	0.003%
18	3.497	760	764	768	rBV	408	339	0.05%	0.006%
19	3.532	773	775	781	rBV2	169	106	0.01%	0.002%
20	3.561	781	784	786	rBV2	228	163	0.02%	0.003%
21	3.645	808	810	812	rVB	223	92	0.01%	0.002%
22	3.677	817	820	823	rVB	268	177	0.02%	0.003%
23	3.722	831	834	835	rBV	167	97	0.01%	0.002%
24	3.741	837	840	843	rVV2	322	248	0.03%	0.004%
25	3.806	849	860	889	rBV	51453	172853	23.25%	3.103%
26	4.253	982	999	1029	rBV	105687	277384	37.30%	4.980%
27	4.597	1099	1106	1108	rBV2	309	258	0.03%	0.005%
28	4.626	1108	1115	1118	rVV2	220	280	0.04%	0.005%
29	4.690	1131	1135	1140	rBV	561	434	0.06%	0.008%
30	4.725	1143	1146	1148	rBV	299	138	0.02%	0.002%
31	4.738	1148	1150	1151	rVV2	120	32	0.00%	0.001%
32	4.796	1166	1168	1170	rVB	153	39	0.01%	0.001%
33	4.818	1173	1175	1176	rBV	143	62	0.01%	0.001%
34	4.828	1176	1178	1181	rBV2	210	122	0.02%	0.002%
35	4.863	1187	1189	1193	rVB	215	87	0.01%	0.002%
36	4.957	1202	1218	1248	rBV2	233200	603438	81.15%	10.834%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070623\
 Data File : VV031649.D
 Acq On : 06 Jul 2023 12:40
 Operator : SY/MD
 Sample : 03501-08ME
 Misc : 5.77g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A46X3ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

37	5.298	1321	1324	1327	rBV2	219	130	0.02%	0.002%
38	5.326	1329	1333	1334	rBV	192	124	0.02%	0.002%
39	5.349	1338	1340	1341	rBV	279	109	0.01%	0.002%
40	5.378	1346	1349	1351	rVV	189	99	0.01%	0.002%
41	5.391	1351	1353	1355	rVB	176	93	0.01%	0.002%
42	5.404	1355	1357	1359	rBV	140	70	0.01%	0.001%
43	5.420	1359	1362	1365	rVB2	275	167	0.02%	0.003%
44	5.539	1386	1399	1428	rBV	227528	486673	65.45%	8.738%
45	5.831	1481	1490	1503	rBV7	6582	13559	1.82%	0.243%
46	5.995	1527	1541	1564	rBV	143494	306918	41.28%	5.510%
47	6.179	1596	1598	1600	rVB	468	176	0.02%	0.003%
48	6.211	1606	1608	1609	rBV	241	98	0.01%	0.002%
49	6.297	1633	1635	1636	rVB	118	45	0.01%	0.001%
50	6.336	1644	1647	1648	rBV2	152	89	0.01%	0.002%
51	6.378	1658	1660	1663	rBV	221	128	0.02%	0.002%
52	6.420	1671	1673	1676	rBV	143	99	0.01%	0.002%
53	6.433	1676	1677	1679	rVV	231	84	0.01%	0.002%
54	6.445	1679	1681	1686	rVV	339	192	0.03%	0.003%
55	6.465	1686	1687	1688	rVV	114	24	0.00%	0.000%
56	6.571	1719	1720	1722	rBV2	376	170	0.02%	0.003%
57	6.777	1782	1784	1788	rBV2	194	105	0.01%	0.002%
58	6.818	1794	1797	1800	rBV	212	122	0.02%	0.002%
59	6.879	1813	1816	1817	rBV	193	117	0.02%	0.002%
60	6.921	1817	1829	1859	rVV2	68072	138601	18.64%	2.488%
61	7.085	1876	1880	1883	rBV2	328	309	0.04%	0.006%
62	7.137	1893	1896	1897	rBV2	418	250	0.03%	0.004%
63	7.188	1905	1912	1916	rBV6	821	1077	0.14%	0.019%
64	7.249	1919	1931	1951	rBV	209572	377266	50.74%	6.773%
65	7.494	2002	2007	2009	rBV4	362	301	0.04%	0.005%
66	7.561	2018	2028	2053	rBV	50883	101503	13.65%	1.822%
67	7.722	2076	2078	2082	rBV2	244	167	0.02%	0.003%
68	7.818	2105	2108	2109	rBV	200	89	0.01%	0.002%
69	7.831	2109	2112	2114	rVV	169	100	0.01%	0.002%
70	7.863	2119	2122	2124	rBV2	443	337	0.05%	0.006%
71	7.992	2158	2162	2166	rBV2	303	226	0.03%	0.004%
72	8.043	2167	2178	2207	rBV	166341	385147	51.80%	6.915%
73	8.432	2297	2299	2306	rVB5	442	280	0.04%	0.005%
74	8.535	2329	2331	2334	rBV3	301	157	0.02%	0.003%
75	8.577	2342	2344	2348	rBV2	466	319	0.04%	0.006%
76	8.629	2356	2360	2364	rBV2	467	318	0.04%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070623\
 Data File : VV031649.D
 Acq On : 06 Jul 2023 12:40
 Operator : SY/MD
 Sample : 03501-08ME
 Misc : 5.77g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A46X3ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

77	8.654	2364	2368	2379	rVB3	777	968	0.13%	0.017%
78	8.696	2379	2381	2384	rVB	256	137	0.02%	0.002%
79	8.722	2386	2389	2390	rBV2	161	103	0.01%	0.002%
80	8.793	2399	2411	2436	rBV	362478	619851	83.36%	11.129%
81	9.098	2502	2506	2508	rBV2	320	301	0.04%	0.005%
82	9.124	2513	2514	2516	rVB2	213	55	0.01%	0.001%
83	9.207	2536	2540	2542	rBV2	252	204	0.03%	0.004%
84	9.249	2551	2553	2555	rBV	161	82	0.01%	0.001%
85	9.313	2571	2573	2574	rBV	220	79	0.01%	0.001%
86	9.339	2579	2581	2583	rBV	265	93	0.01%	0.002%
87	9.500	2627	2631	2634	rBV2	298	207	0.03%	0.004%
88	9.625	2668	2670	2672	rBV	193	107	0.01%	0.002%
89	9.709	2693	2696	2698	rBV2	582	438	0.06%	0.008%
90	9.760	2710	2712	2717	rBV	241	150	0.02%	0.003%
91	9.793	2717	2722	2724	rBV	348	323	0.04%	0.006%
92	10.162	2824	2837	2853	rBV	283356	459848	61.84%	8.256%
93	10.278	2870	2873	2874	rBV	244	144	0.02%	0.003%
94	10.477	2933	2935	2937	rBV2	343	221	0.03%	0.004%
95	10.860	3052	3054	3056	rBV3	474	290	0.04%	0.005%
96	11.133	3135	3139	3140	rBV2	568	468	0.06%	0.008%
97	11.194	3146	3158	3183	rBV	478183	743584	100.00%	13.350%
98	11.571	3263	3275	3296	rBV	358706	566325	76.16%	10.168%
99	12.548	3576	3579	3581	rBV2	414	272	0.04%	0.005%
100	13.628	3912	3915	3918	rBV2	671	554	0.07%	0.010%




Sum of corrected areas: 5569760

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070623\
Data File : VV031649.D
Acq On : 06 Jul 2023 12:40
Operator : SY/MD
Sample : 03501-08ME
Misc : 5.77g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A46X3ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

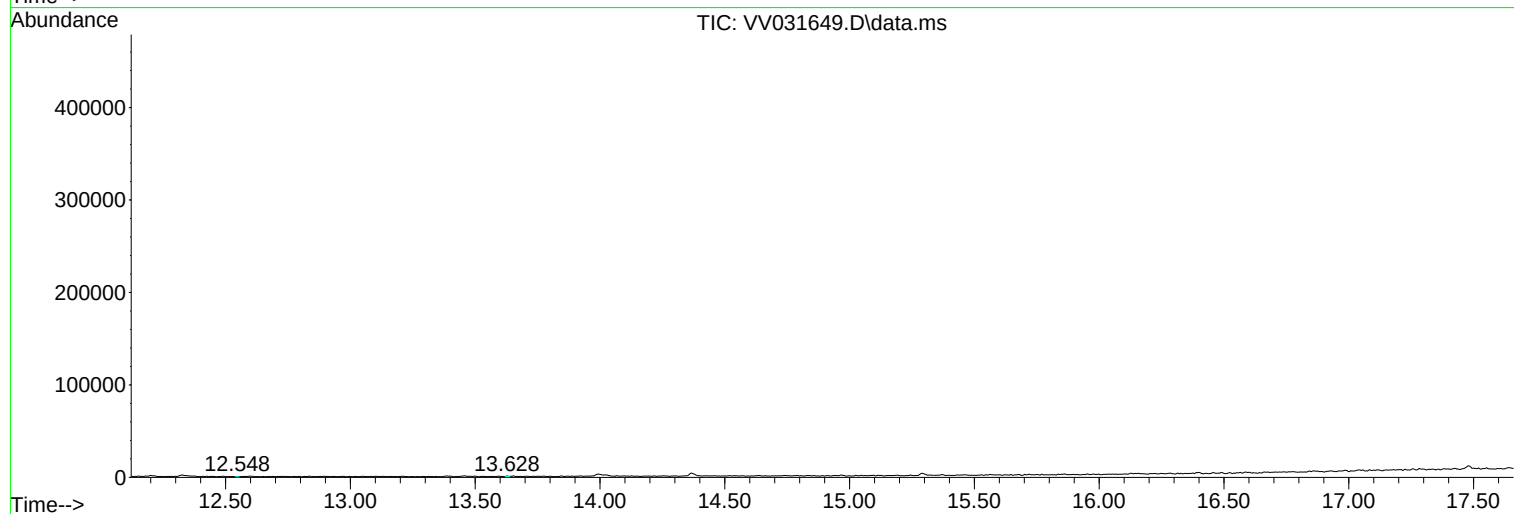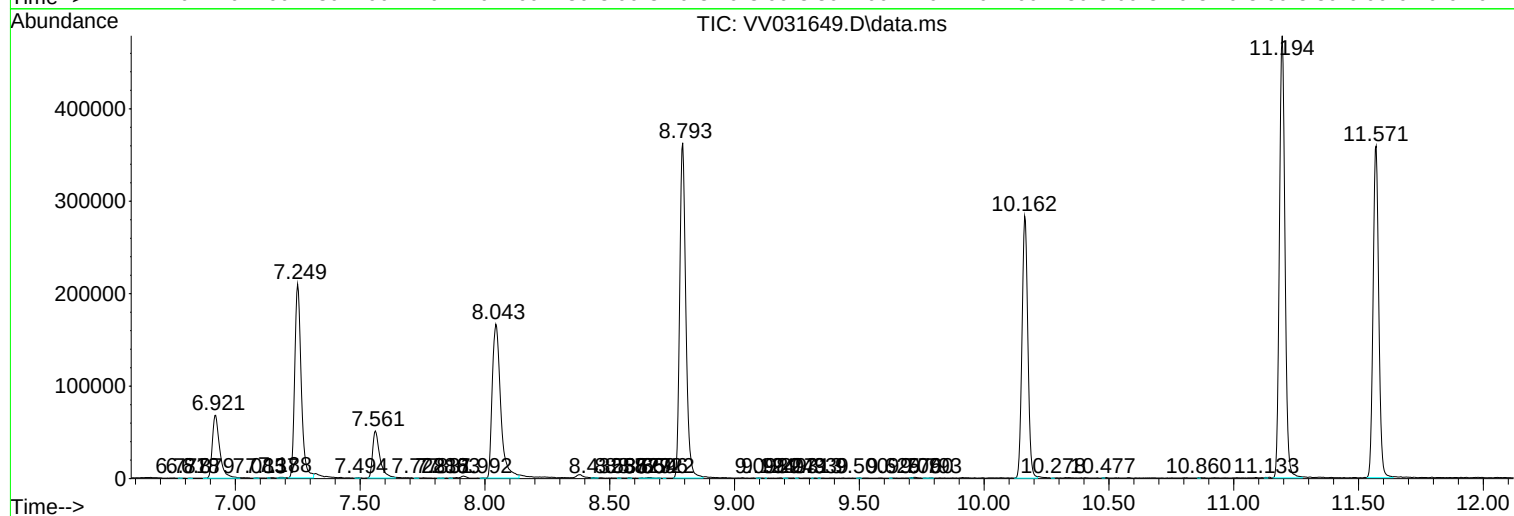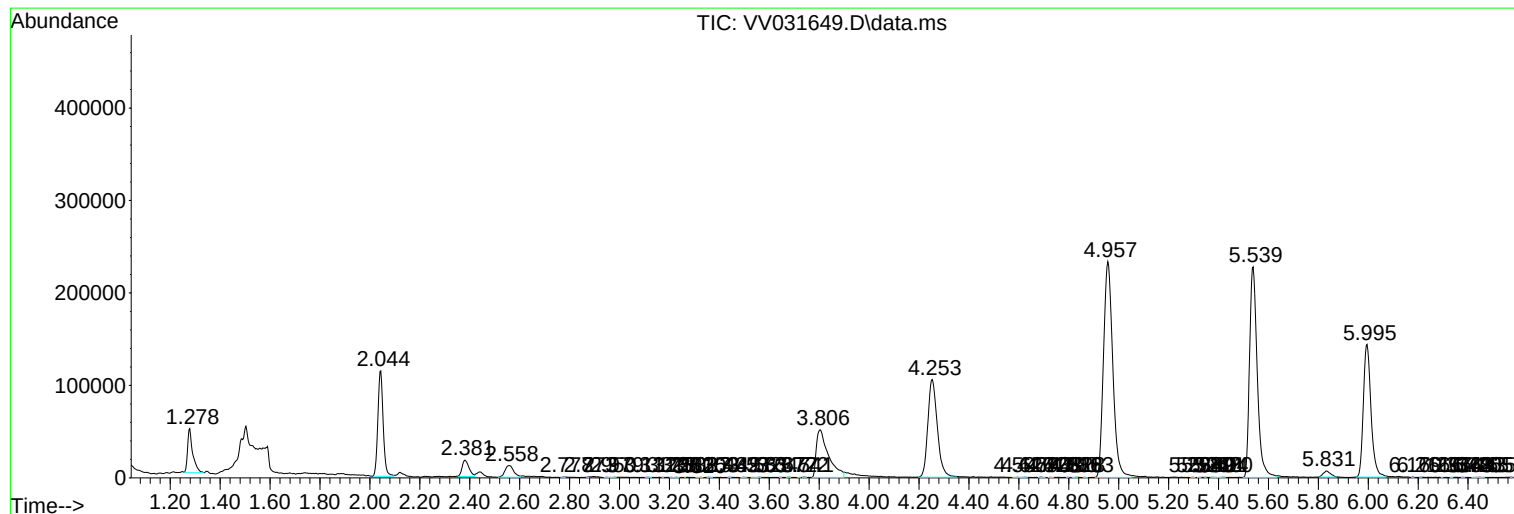

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070623\
Data File : VV031649.D
Acq On : 06 Jul 2023 12:40
Operator : SY/MD
Sample : 03501-08ME
Misc : 5.77g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A46X3ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070623\
Data File : VV031649.D
Acq On : 06 Jul 2023 12:40
Operator : SY/MD
Sample : 03501-08ME
Misc : 5.77g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A46X3ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc