


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070623\
Data File : VV031642.D
Acq On : 06 Jul 2023 08:38
Operator : SY/MD
Sample : BFB394
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB394

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Title : VOC Analysis
Last Update : Fri Jul 07 02:34:55 2023

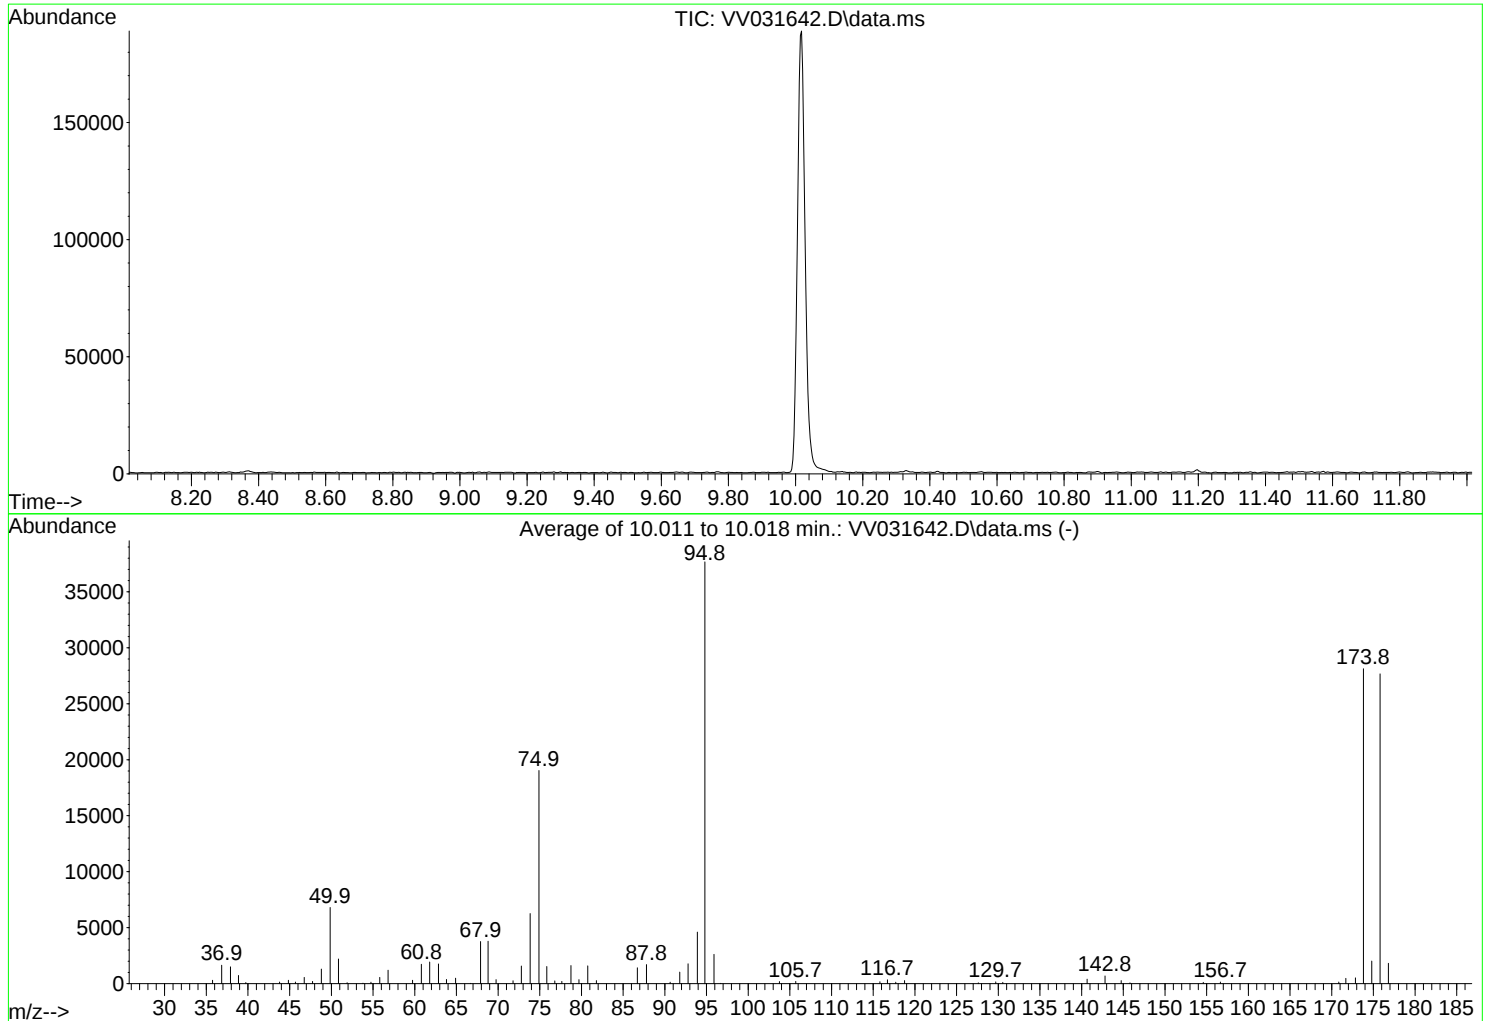

AutoFind: Scans 2790, 2791, 2792; Background Corrected with Scan 2780

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.1	6807	PASS
75	95	30	80	50.5	19040	PASS
95	95	100	100	100.0	37675	PASS
96	95	5	9	6.9	2618	PASS
173	174	0.00	2	1.9	522	PASS
174	95	50	120	74.7	28125	PASS
175	174	5	9	7.2	2014	PASS
176	174	95	105	98.4	27672	PASS
177	176	5	10	6.6	1816	PASS

m/z	Abundance
39.70	153.0
43.80	449.0

Instrument :
MSVOA_V
ClientSampleId :
BFB394

m/z	Abundance
35.70	281.0
36.90	1567.0
37.90	1386.0
38.90	746.0
39.80	229.0
43.80	580.0
44.90	280.0
45.70	179.0
46.70	502.0
47.90	181.0
48.80	1296.0
49.80	6296.0
50.80	2090.0
51.90	122.0
54.80	109.0
55.80	502.0
56.80	1203.0
59.70	301.0
60.80	1608.0
61.80	1823.0
62.90	1604.0
63.80	370.0
64.90	488.0
67.90	3438.0
68.80	3558.0
69.80	281.0
71.80	209.0
72.80	1546.0
73.90	5948.0
74.90	17680.0
75.90	1503.0
76.80	241.0
77.70	161.0
78.80	1505.0
79.70	371.0
80.70	1457.0
81.80	271.0
86.70	1358.0
87.80	1557.0
90.60	128.0
91.80	880.0
92.80	1618.0
93.90	4285.0
94.80	35184.0
95.90	2494.0
96.70	102.0
103.80	185.0
105.70	202.0
115.80	152.0
116.70	325.0
117.60	127.0
118.80	227.0
129.80	127.0
140.70	409.0
142.80	668.0
144.70	232.0
145.80	115.0
154.60	112.0
156.60	140.0
170.80	100.0
171.70	407.0
172.80	440.0
173.80	25288.0
174.80	1869.0
175.80	24632.0
176.80	1850.0

Instrument :
MSVOA_V
ClientSampleId :
BFB394

m/z	Abundance
35.80	287.0
36.90	1664.0
37.90	1568.0
38.90	753.0
39.80	245.0
43.80	607.0
44.90	315.0
45.70	143.0
46.70	560.0
47.70	205.0
48.80	1330.0
49.90	6984.0
50.90	2291.0
51.90	134.0
54.70	121.0
55.80	578.0
56.80	1290.0
59.70	291.0
60.80	1799.0
61.80	1985.0
62.90	1831.0
63.80	389.0
64.90	524.0
67.90	3896.0
68.80	3921.0
69.70	379.0
71.80	269.0
72.80	1604.0
73.80	6435.0
74.90	19688.0
75.90	1570.0
76.80	261.0
77.60	210.0
78.80	1628.0
79.70	389.0
80.80	1679.0
81.80	291.0
86.70	1424.0
87.80	1754.0
90.70	130.0
91.80	1062.0
92.80	1814.0
93.90	4804.0
94.80	39040.0
95.90	2719.0
103.70	184.0
105.70	220.0
115.80	171.0
116.70	357.0
117.70	143.0
118.70	282.0
127.60	118.0
129.70	155.0
130.50	158.0
140.60	385.0
142.80	698.0
144.70	260.0
145.80	103.0
154.60	126.0
156.60	162.0
170.90	145.0
171.70	497.0
172.90	541.0
173.80	28968.0
174.80	2077.0
175.80	28608.0
176.80	1856.0

Instrument :
MSVOA_V
ClientSampleId :
BFB394

m/z	Abundance
35.80	325.0
36.80	1714.0
37.90	1548.0
38.80	692.0
39.80	267.0
43.80	599.0
44.80	319.0
45.80	101.0
46.80	612.0
47.70	229.0
48.80	1272.0
49.90	7140.0
50.90	2231.0
53.80	114.0
54.70	136.0
55.80	604.0
56.80	1118.0
59.80	303.0
60.80	1773.0
61.80	1995.0
62.80	1854.0
63.80	377.0
64.90	461.0
66.70	102.0
67.90	3957.0
68.80	3885.0
69.70	402.0
71.80	300.0
72.80	1549.0
73.80	6418.0
74.90	19752.0
75.80	1499.0
76.80	223.0
77.70	227.0
78.70	1721.0
79.70	334.0
80.80	1637.0
81.80	264.0
86.70	1448.0
87.80	1783.0
90.70	139.0
91.80	1170.0
92.80	1872.0
93.90	4720.0
94.80	38800.0
95.90	2640.0
103.70	173.0
105.70	168.0
115.80	177.0
116.70	364.0
117.80	140.0
118.70	301.0
127.60	112.0
129.60	186.0
130.60	168.0
140.60	391.0
142.80	681.0
144.80	316.0
154.60	117.0
156.70	135.0
170.80	177.0
171.70	531.0
172.90	584.0
173.80	30120.0
174.80	2097.0
175.80	29776.0
176.80	1741.0

Instrument :
MSVOA_V
ClientSampleId :
BFB394