

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV070720\
 Data File : VV017374.D
 Acq On : 07 Jul 2020 13:26
 Operator : SY/MD
 Sample : L3154-13
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H4273

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.1

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR061720WMA.M

Title : TRACE VOA SOM01.0

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.116	3	8	16	rVB3	15900	17038	3.30%	0.299%
2	1.319	59	71	83	rBV2	448823	477485	92.54%	8.390%
3	1.579	145	152	163	rVB	58467	65694	12.73%	1.154%
4	1.650	167	174	179	rBV8	4423	5786	1.12%	0.102%
5	2.126	311	322	334	rBV	122364	179784	34.84%	3.159%
6	2.778	513	525	540	rVB3	51124	91325	17.70%	1.605%
7	3.939	871	886	913	rBV4	141257	403513	78.20%	7.090%
8	4.376	1007	1022	1052	rVB	92273	238964	46.31%	4.199%
9	4.785	1140	1149	1164	rVB	5421	13274	2.57%	0.233%
10	5.074	1220	1239	1265	rBV2	207476	515998	100.00%	9.067%
11	5.257	1285	1296	1313	rVB5	9622	26405	5.12%	0.464%
12	5.643	1401	1416	1443	rBV	197504	419553	81.31%	7.372%
13	5.945	1500	1510	1521	rVB	10126	22899	4.44%	0.402%
14	6.097	1543	1557	1574	rBV2	117489	254411	49.30%	4.470%
15	6.672	1724	1736	1753	rVB9	7805	21177	4.10%	0.372%
16	6.798	1763	1775	1788	rBV8	10102	24665	4.78%	0.433%
17	7.010	1826	1841	1864	rBV2	62567	123110	23.86%	2.163%
18	7.338	1932	1943	1962	rVB	242760	427017	82.76%	7.503%
19	7.466	1975	1983	1989	rBV8	4532	7175	1.39%	0.126%
20	7.643	2030	2038	2045	rBV	35643	56307	10.91%	0.989%
21	7.810	2085	2090	2095	rVB6	5480	6225	1.21%	0.109%
22	7.862	2097	2106	2118	rBV3	16113	28304	5.49%	0.497%
23	8.113	2173	2184	2209	rBV	230484	453806	87.95%	7.974%
24	8.373	2254	2265	2272	rBV3	10456	20497	3.97%	0.360%
25	8.415	2274	2278	2287	rVB8	5003	6345	1.23%	0.111%
26	8.527	2300	2313	2324	rBV8	10460	22325	4.33%	0.392%
27	8.781	2383	2392	2399	rBV10	4040	7230	1.40%	0.127%
28	8.875	2408	2421	2443	rBV	303176	497231	96.36%	8.737%
29	9.129	2489	2500	2504	rBV	9514	15032	2.91%	0.264%
30	9.341	2563	2566	2576	rVB9	4707	5789	1.12%	0.102%
31	9.514	2617	2620	2632	rVB9	8360	10951	2.12%	0.192%
32	10.148	2810	2817	2824	rVB7	5357	8307	1.61%	0.146%
33	10.238	2834	2845	2860	rBV2	85598	145398	28.18%	2.555%
34	11.270	3154	3166	3186	rBV	320869	506976	98.25%	8.909%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV070720\
Data File : VV017374.D
Acq On : 07 Jul 2020 13:26
Operator : SY/MD
Sample : L3154-13
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H4273

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.1 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR061720WMA.M
Title : TRACE VOA SOM01.0

35	11.646	3269	3283	3307	rBV	265630	433359	83.98%	7.615%
36	12.264	3468	3475	3483	rVB6	4014	7217	1.40%	0.127%
37	13.331	3801	3807	3818	rVB6	5835	8039	1.56%	0.141%
38	13.723	3923	3929	3945	rVB6	5529	9078	1.76%	0.160%
39	14.135	4045	4057	4066	rBV6	6967	12400	2.40%	0.218%
40	14.244	4085	4091	4101	rVB9	7583	12764	2.47%	0.224%
41	14.328	4107	4117	4126	rVB9	8528	15930	3.09%	0.280%
42	14.714	4226	4237	4245	rVB9	6791	13633	2.64%	0.240%
43	14.852	4271	4280	4291	rVB9	6236	12653	2.45%	0.222%
44	15.183	4376	4383	4390	rBV9	5787	10074	1.95%	0.177%
45	15.341	4426	4432	4445	rVB9	4750	9074	1.76%	0.159%
46	15.450	4458	4466	4471	rBV9	6827	9137	1.77%	0.161%
47	15.524	4483	4489	4492	rBV7	5309	5912	1.15%	0.104%
48	15.717	4540	4549	4553	rBV9	4198	5644	1.09%	0.099%


Sum of corrected areas: 5690910

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV070720\
Data File : VV017374.D
Acq On : 07 Jul 2020 13:26
Operator : SY/MD
Sample : L3154-13
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H4273

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR061720WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

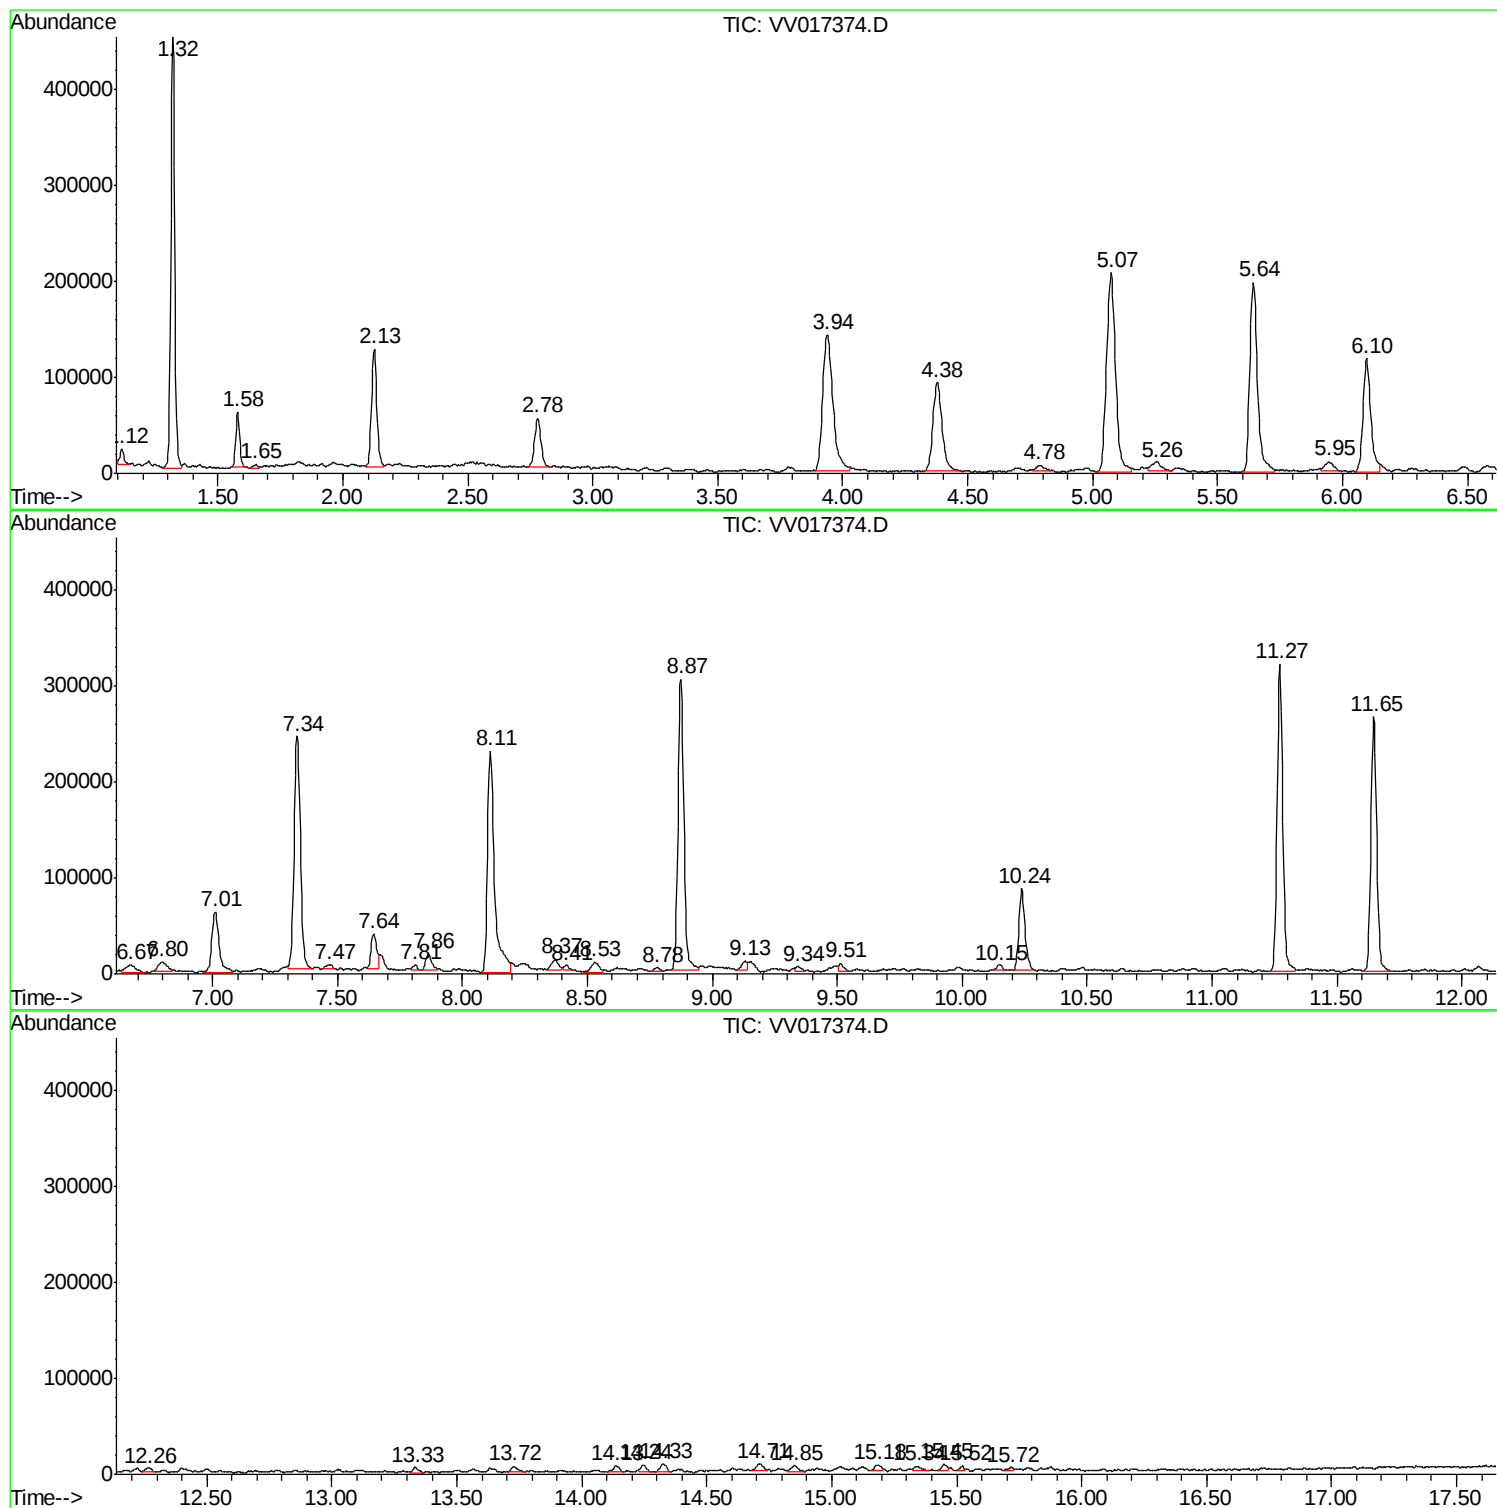

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV070720\
Data File : VV017374.D
Acq On : 07 Jul 2020 13:26
Operator : SY/MD
Sample : L3154-13
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H4273

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR061720WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV070720\
Data File : VV017374.D
Acq On : 07 Jul 2020 13:26
Operator : SY/MD
Sample : L3154-13
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H4273

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR061720WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc