


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV070720\
 Data File : VV017364.D
 Acq On : 07 Jul 2020 08:49
 Operator : SY/MD
 Sample : BFB48
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB48

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR061720WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Wed Jul 08 01:30:57 2020

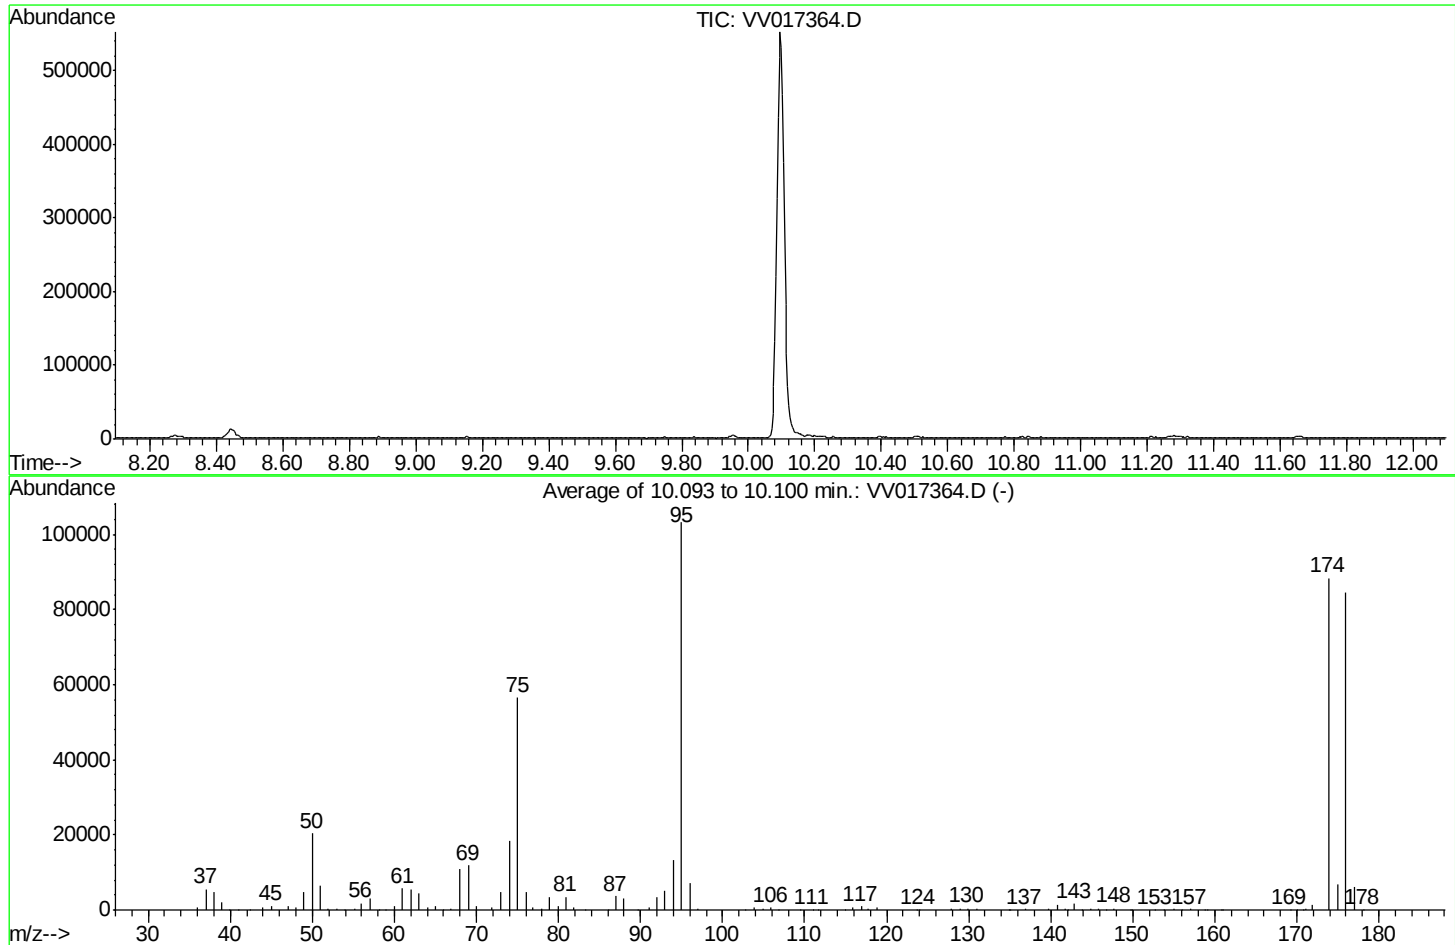

AutoFind: Scans 2800, 2801, 2802; Background Corrected with Scan 2788

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.8	20442	PASS
75	95	30	80	54.7	56440	PASS
95	95	100	100	100.0	103258	PASS
96	95	5	9	6.8	7055	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	85.6	88424	PASS
175	174	5	9	7.6	6737	PASS
176	174	95	101	95.7	84645	PASS
177	176	5	9	7.1	6006	PASS

m/z	Abundance
36.00	962.0
37.00	5540.0
38.00	4891.0
39.00	2256.0
39.90	299.0
42.90	118.0
44.00	1071.0
45.00	1014.0
47.00	965.0
48.00	631.0
49.00	4735.0
50.00	20752.0
51.00	6425.0
51.90	434.0
53.00	246.0
53.90	117.0
54.90	276.0
55.90	1867.0
57.00	3091.0
58.00	187.0
58.80	116.0
60.00	1022.0
61.00	5585.0
62.00	5493.0
63.00	4365.0
64.00	851.0
65.00	1116.0
66.00	154.0
66.90	409.0
68.00	10912.0
69.00	11373.0
70.00	845.0
71.90	764.0
73.00	4838.0
74.00	18104.0
75.00	55632.0
76.00	4531.0
76.90	840.0
77.90	433.0
78.90	3553.0
80.00	917.0
80.90	3399.0
81.90	782.0
83.20	127.0
87.00	3347.0
87.90	3150.0
91.00	729.0
92.00	3057.0
93.00	4832.0
94.00	13093.0
95.00	100880.0
96.00	7089.0
97.00	205.0
102.70	153.0
103.80	594.0
104.90	224.0
105.90	689.0
106.90	194.0
109.50	131.0
110.90	140.0
115.00	173.0
115.90	559.0
116.90	853.0
117.80	469.0
118.90	595.0
123.70	130.0
127.90	424.0
128.90	203.0
129.90	458.0
131.00	198.0
135.10	207.0
136.90	292.0
139.70	233.0
140.90	1082.0
141.70	186.0
142.20	234.0
142.90	1541.0
143.90	147.0
144.90	367.0
145.80	187.0
146.80	162.0
147.70	414.0
155.00	261.0
156.00	124.0
157.00	275.0
159.10	107.0
160.80	150.0
170.10	134.0
171.10	240.0
171.90	1120.0
173.90	83616.0
174.90	6577.0

Instrument :
MSVOA_V
ClientSampleId :
BFB48

175.9080000.0

177.006175.0

Instrument :
MSVOA_V
ClientSampleId :
BFB48

m/z	Abundance
36.00	973.0
37.00	5746.0
38.00	5084.0
39.00	2390.0
40.00	368.0
44.00	1168.0
45.00	1082.0
47.10	1019.0
47.90	656.0
49.00	4977.0
50.00	21272.0
51.00	6771.0
52.00	395.0
52.90	262.0
55.10	307.0
55.90	1824.0
57.00	3265.0
58.10	174.0
58.80	144.0
60.00	1037.0
61.00	6012.0
62.00	5790.0
63.00	4617.0
64.00	852.0
65.00	1049.0
66.00	192.0
66.90	467.0
68.00	11146.0
69.00	12325.0
70.00	900.0
71.90	805.0
73.00	5065.0
74.00	18928.0
75.00	58312.0
76.00	4875.0
76.90	755.0
77.90	434.0
78.90	3563.0
79.90	991.0
80.90	3602.0
81.90	854.0
83.30	108.0
86.20	172.0
87.00	3837.0
87.90	3248.0
89.60	113.0
91.00	813.0
92.00	3360.0
93.00	5223.0
94.00	13684.0
95.00	106816.0
96.00	7325.0
97.00	211.0
102.80	152.0
103.80	628.0
104.90	244.0
105.90	684.0
106.80	174.0
109.50	108.0
111.00	120.0
114.80	168.0
115.90	601.0
116.90	1010.0
117.80	490.0
118.90	586.0
123.90	168.0
127.90	447.0
128.90	222.0
129.80	467.0
130.90	206.0
134.80	238.0
136.80	328.0
139.70	210.0
140.90	1327.0
141.80	223.0
142.00	215.0
142.90	1714.0
143.90	133.0
144.90	375.0
145.80	245.0
146.80	142.0
147.80	398.0
149.70	102.0
152.80	145.0
155.00	280.0
156.00	123.0
157.00	310.0
158.80	129.0
160.70	154.0
170.00	157.0
171.10	305.0
171.90	1222.0

Instrument :
MSVOA_V
ClientSampleId :
BFB48

173.90	91376.0
175.00	6912.0
175.90	87520.0
177.00	6232.0

Instrument :
MSVOA_V
ClientSampleId :
BFB48

m/z	Abundance
36.00	865.0
37.00	5520.0
38.00	4822.0
39.00	2207.0
39.90	411.0
41.00	103.0
42.30	115.0
44.00	1051.0
45.00	1068.0
47.10	972.0
47.90	674.0
49.00	4653.0
50.00	19304.0
51.00	6490.0
52.00	365.0
52.90	296.0
55.10	347.0
55.90	1600.0
57.00	3114.0
58.20	149.0
58.90	136.0
60.00	1050.0
61.00	5634.0
62.00	5463.0
63.00	4326.0
64.00	822.0
65.00	1002.0
66.00	205.0
66.90	445.0
68.00	10710.0
69.00	11865.0
70.00	882.0
71.90	693.0
73.00	4745.0
74.00	18080.0
75.00	55376.0
76.00	4654.0
76.90	629.0
77.90	381.0
78.90	3396.0
79.90	998.0
80.90	3371.0
81.90	847.0
83.40	106.0
86.00	179.0
87.00	3602.0
87.90	3136.0
89.60	140.0
91.00	796.0
92.00	3399.0
93.00	4953.0
94.00	12832.0
95.00	102080.0
96.00	6753.0
97.00	190.0
102.80	162.0
103.80	625.0
104.90	241.0
106.00	536.0
106.80	152.0
111.00	118.0
111.70	101.0
114.70	185.0
115.90	540.0
116.90	1095.0
117.80	492.0
118.90	500.0
123.90	190.0
127.90	506.0
128.90	215.0
129.80	478.0
130.90	215.0
134.90	265.0
136.80	289.0
139.70	137.0
140.90	1487.0
141.80	252.0
142.90	1749.0
143.80	133.0
144.90	331.0
145.80	303.0
147.80	363.0
149.90	135.0
152.70	201.0
153.80	126.0
155.00	281.0
155.90	106.0
157.00	280.0
158.80	145.0
160.70	146.0
161.00	123.0
169.20	116.0

Instrument :
MSVOA_V
ClientSampleId :
BFB48

169.90	129.0
170.70	203.0
171.20	295.0
171.90	1333.0
173.90	90280.0
175.00	6722.0
175.90	86416.0
177.00	5613.0
178.10	107.0

Instrument :
MSVOA_V
ClientSampleId :
BFB48

m/z	Abundance
36.10	197.0
38.80	126.0
40.00	273.0
43.00	124.0
43.90	254.0
53.20	105.0
55.00	180.0
60.10	113.0
72.20	103.0
77.40	185.0
86.10	108.0

Instrument :
MSVOA_V
ClientSampleId :
BFB48