




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070722\
Data File : VV026675.D
Acq On : 07 Jul 2022 13:53
Operator : SY/MD
Sample : N3598-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AN9

Manual IntegrationsAPPROVED

Quant Time: Jul 08 03:00:58 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Jul 08 02:58:15 2022
Response via : Initial Calibration

Reviewed By :John Carlone 07/08/2022
Supervised By :Mahesh Dadoda 07/11/2022

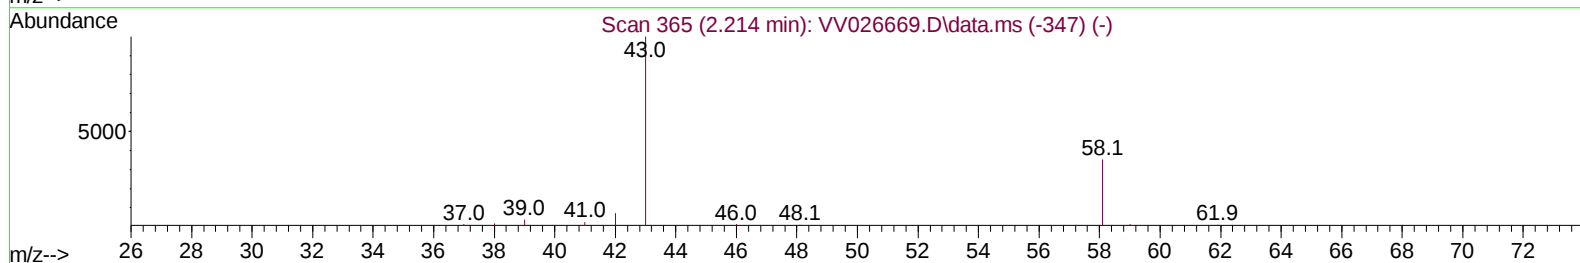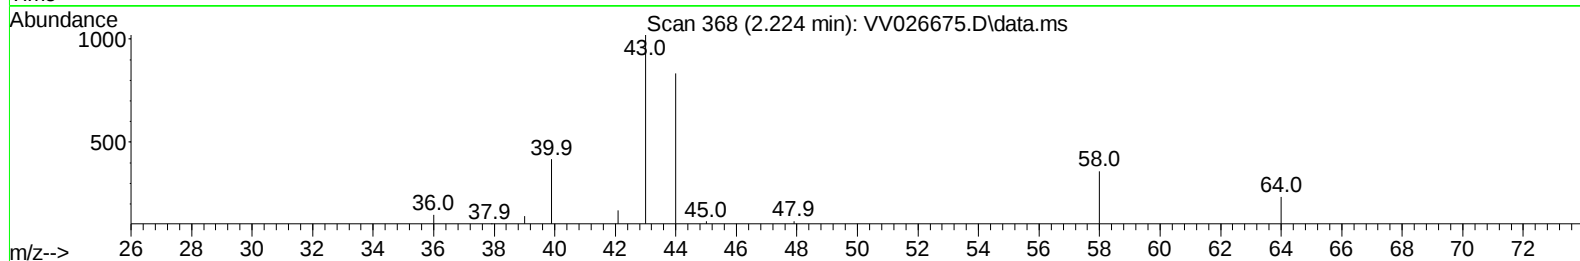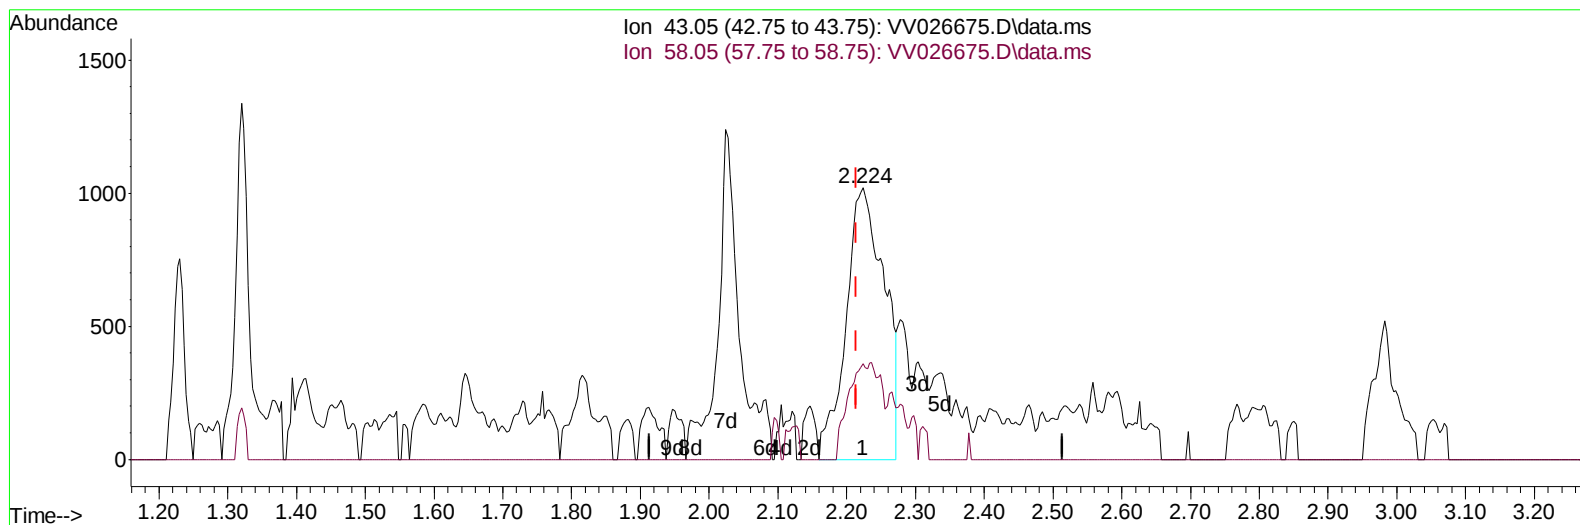

TIC: VV026675.D\data.ms

(13) Acetone (T)

2.224min (+ 0.010) 4.16 ug/L

response 3946

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	37.50	18.09
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070722\
 Data File : VV026675.D
 Acq On : 07 Jul 2022 13:53
 Operator : SY/MD
 Sample : N3598-10
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AN9

Manual IntegrationsAPPROVED

Quant Time: Jul 08 03:00:58 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Jul 08 02:58:15 2022
 Response via : Initial Calibration

Reviewed By :John Carlone 07/08/2022
 Supervised By :Mahesh Dadoda 07/11/2022

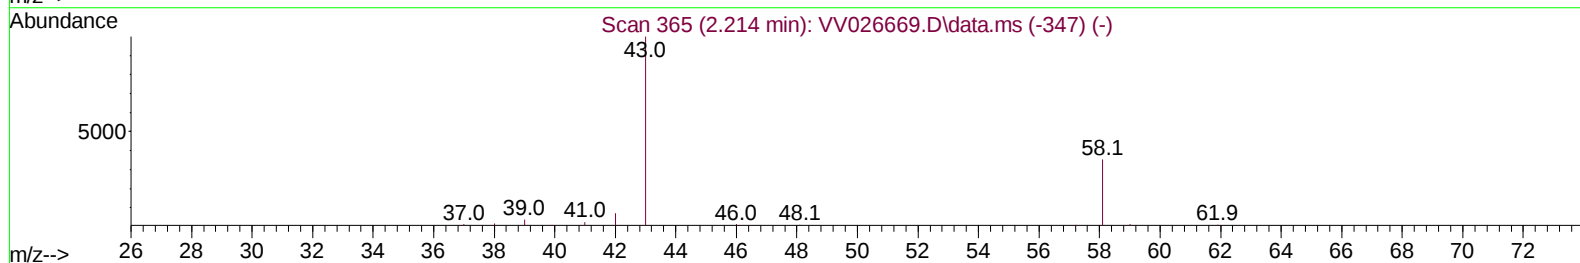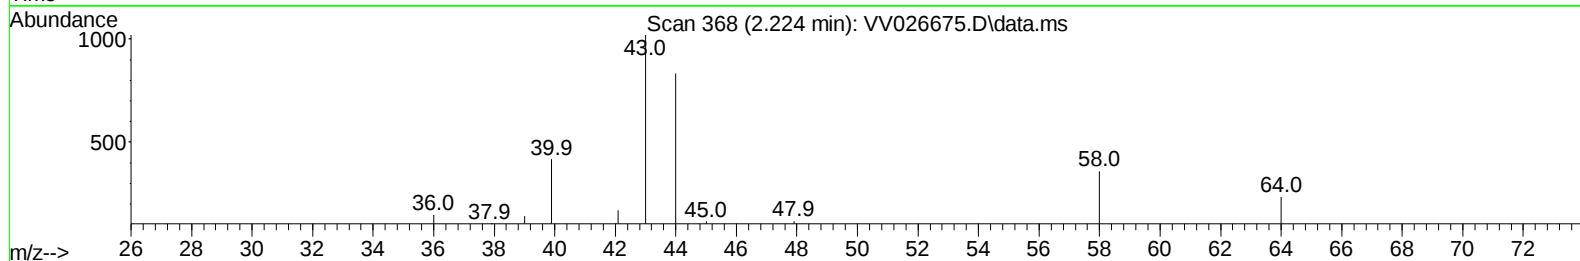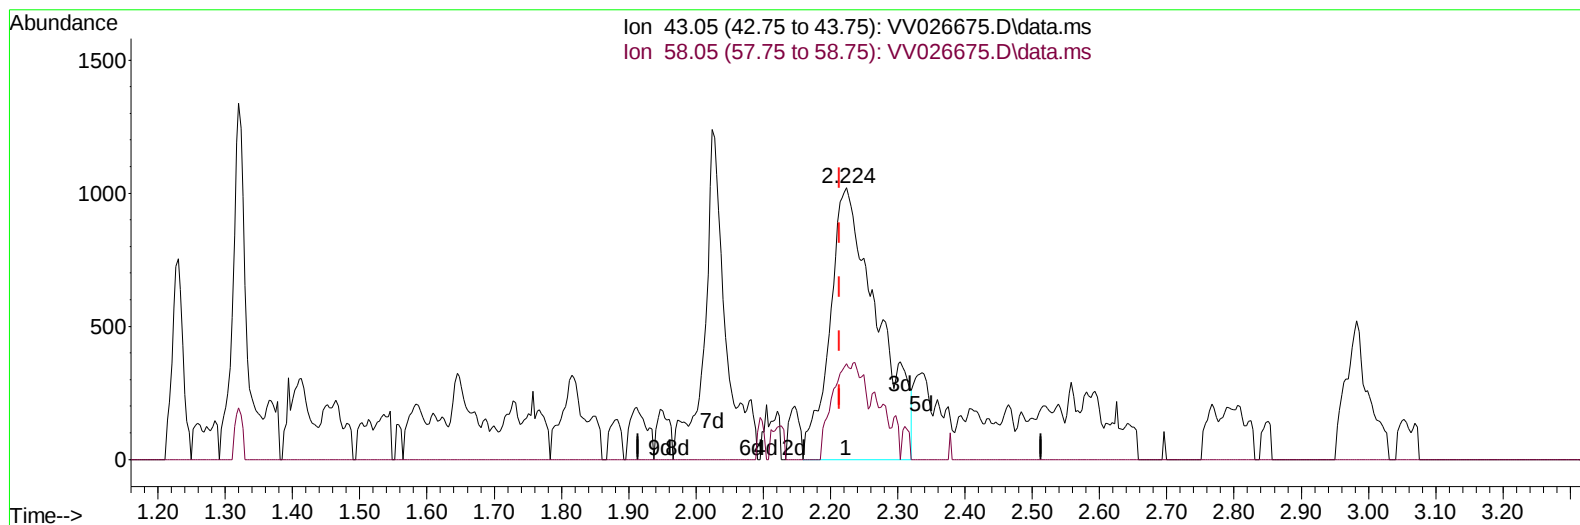

TIC: VV026675.D\data.ms

(13) Acetone (T)

2.224min (+ 0.010) 5.29 ug/L m

response 5019

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	37.50	14.23
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070722\
 Data File : VV026675.D
 Acq On : 07 Jul 2022 13:53
 Operator : SY/MD
 Sample : N3598-10
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COAN9

Manual IntegrationsAPPROVED

Quant Time: Jul 08 03:00:58 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Jul 08 02:58:15 2022
 Response via : Initial Calibration

Reviewed By :John Carlone 07/08/2022
 Supervised By :Mahesh Dadoda 07/11/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.625	114	186937	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	184475	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	75021	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.320	65	56723	3.773	ug/L	0.00
Spiked Amount 5.000	Range 40 - 130		Recovery =	75.400%		
7) Chloroethane-d5	1.581	69	50825	4.208	ug/L	0.00
Spiked Amount 5.000	Range 65 - 130		Recovery =	84.200%		
11) 1,1-Dichloroethene-d2	2.121	63	80187	3.002	ug/L	0.00
Spiked Amount 5.000	Range 60 - 125		Recovery =	60.000%		
20) 2-Butanone-d5	3.934	46	66934	44.782	ug/L	0.01
Spiked Amount 50.000	Range 40 - 130		Recovery =	89.560%		
24) Chloroform-d	4.362	84	109765	4.466	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	89.400%		
26) 1,2-Dichloroethane-d4	5.043	65	42500	4.490	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	89.800%		
32) Benzene-d6	5.060	84	192248	3.628	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	72.600%		
36) 1,2-Dichloropropane-d6	6.076	67	58745	4.032	ug/L	0.00
Spiked Amount 5.000	Range 60 - 140		Recovery =	80.600%		
41) Toluene-d8	7.320	98	151501	3.179	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	63.600%#		
43) trans-1,3-Dichloroprop...	7.632	79	13418	3.563	ug/L	0.00
Spiked Amount 5.000	Range 55 - 130		Recovery =	71.200%		
46) 2-Hexanone-d5	8.092	63	51513	35.908	ug/L	0.00
Spiked Amount 50.000	Range 45 - 130		Recovery =	71.820%		
56) 1,1,2,2-Tetrachloroeth...	10.217	84	39728	4.168	ug/L	0.00
Spiked Amount 5.000	Range 65 - 120		Recovery =	83.400%		
66) 1,2-Dichlorobenzene-d4	11.625	152	51440	4.143	ug/L	0.00
Spiked Amount 5.000	Range 80 - 120		Recovery =	82.800%		
Target Compounds						
					Qvalue	
13) Acetone	2.224	43	5019m	5.293	ug/L	
14) Carbon disulfide	2.304	76	20698	0.621	ug/L	97
16) Methylene chloride	2.523	84	5977	0.446	ug/L	98
25) Chloroform	4.388	83	115263	4.658	ug/L	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070722\
Data File : VV026675.D
Acq On : 07 Jul 2022 13:53
Operator : SY/MD
Sample : N3598-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COAN9

Manual IntegrationsAPPROVED

Quant Time: Jul 08 03:00:58 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Jul 08 02:58:15 2022
Response via : Initial Calibration

Reviewed By :John Carlone 07/08/2022
Supervised By :Mahesh Dadoda 07/11/2022

