

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070722\
 Data File : VV026670.D
 Acq On : 07 Jul 2022 11:06
 Operator : SY/MD
 Sample : VV0707WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK390

Quant Time: Jul 08 02:59:40 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Jul 08 02:58:15 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.625	114	178327	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	174863	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	70292	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.317	65	64140	4.472	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	89.400%
7) Chloroethane-d5	1.581	69	56401	4.895	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	98.000%
11) 1,1-Dichloroethene-d2	2.118	63	89935	3.529	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	70.600%
20) 2-Butanone-d5	3.928	46	71492	50.141	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	100.280%
24) Chloroform-d	4.362	84	113562	4.844	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	96.800%
26) 1,2-Dichloroethane-d4	5.043	65	47011	5.206	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	104.200%
32) Benzene-d6	5.060	84	209688	4.175	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	83.400%
36) 1,2-Dichloropropane-d6	6.076	67	66110	4.786	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	95.800%
41) Toluene-d8	7.320	98	161127	3.567	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	71.400%
43) trans-1,3-Dichloroprop...	7.632	79	14873	4.166	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	83.400%
46) 2-Hexanone-d5	8.092	63	53383	39.257	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	78.520%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	42868	4.744	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	94.800%
66) 1,2-Dichlorobenzene-d4	11.625	152	53498	4.599	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	92.000%
Target Compounds						Qvalue
16) Methylene chloride	2.523	84	11847	0.927	ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070722\
Data File : VV026670.D
Acq On : 07 Jul 2022 11:06
Operator : SY/MD
Sample : VV0707WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK390


Quant Time: Jul 08 02:59:40 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Jul 08 02:58:15 2022
Response via : Initial Calibration

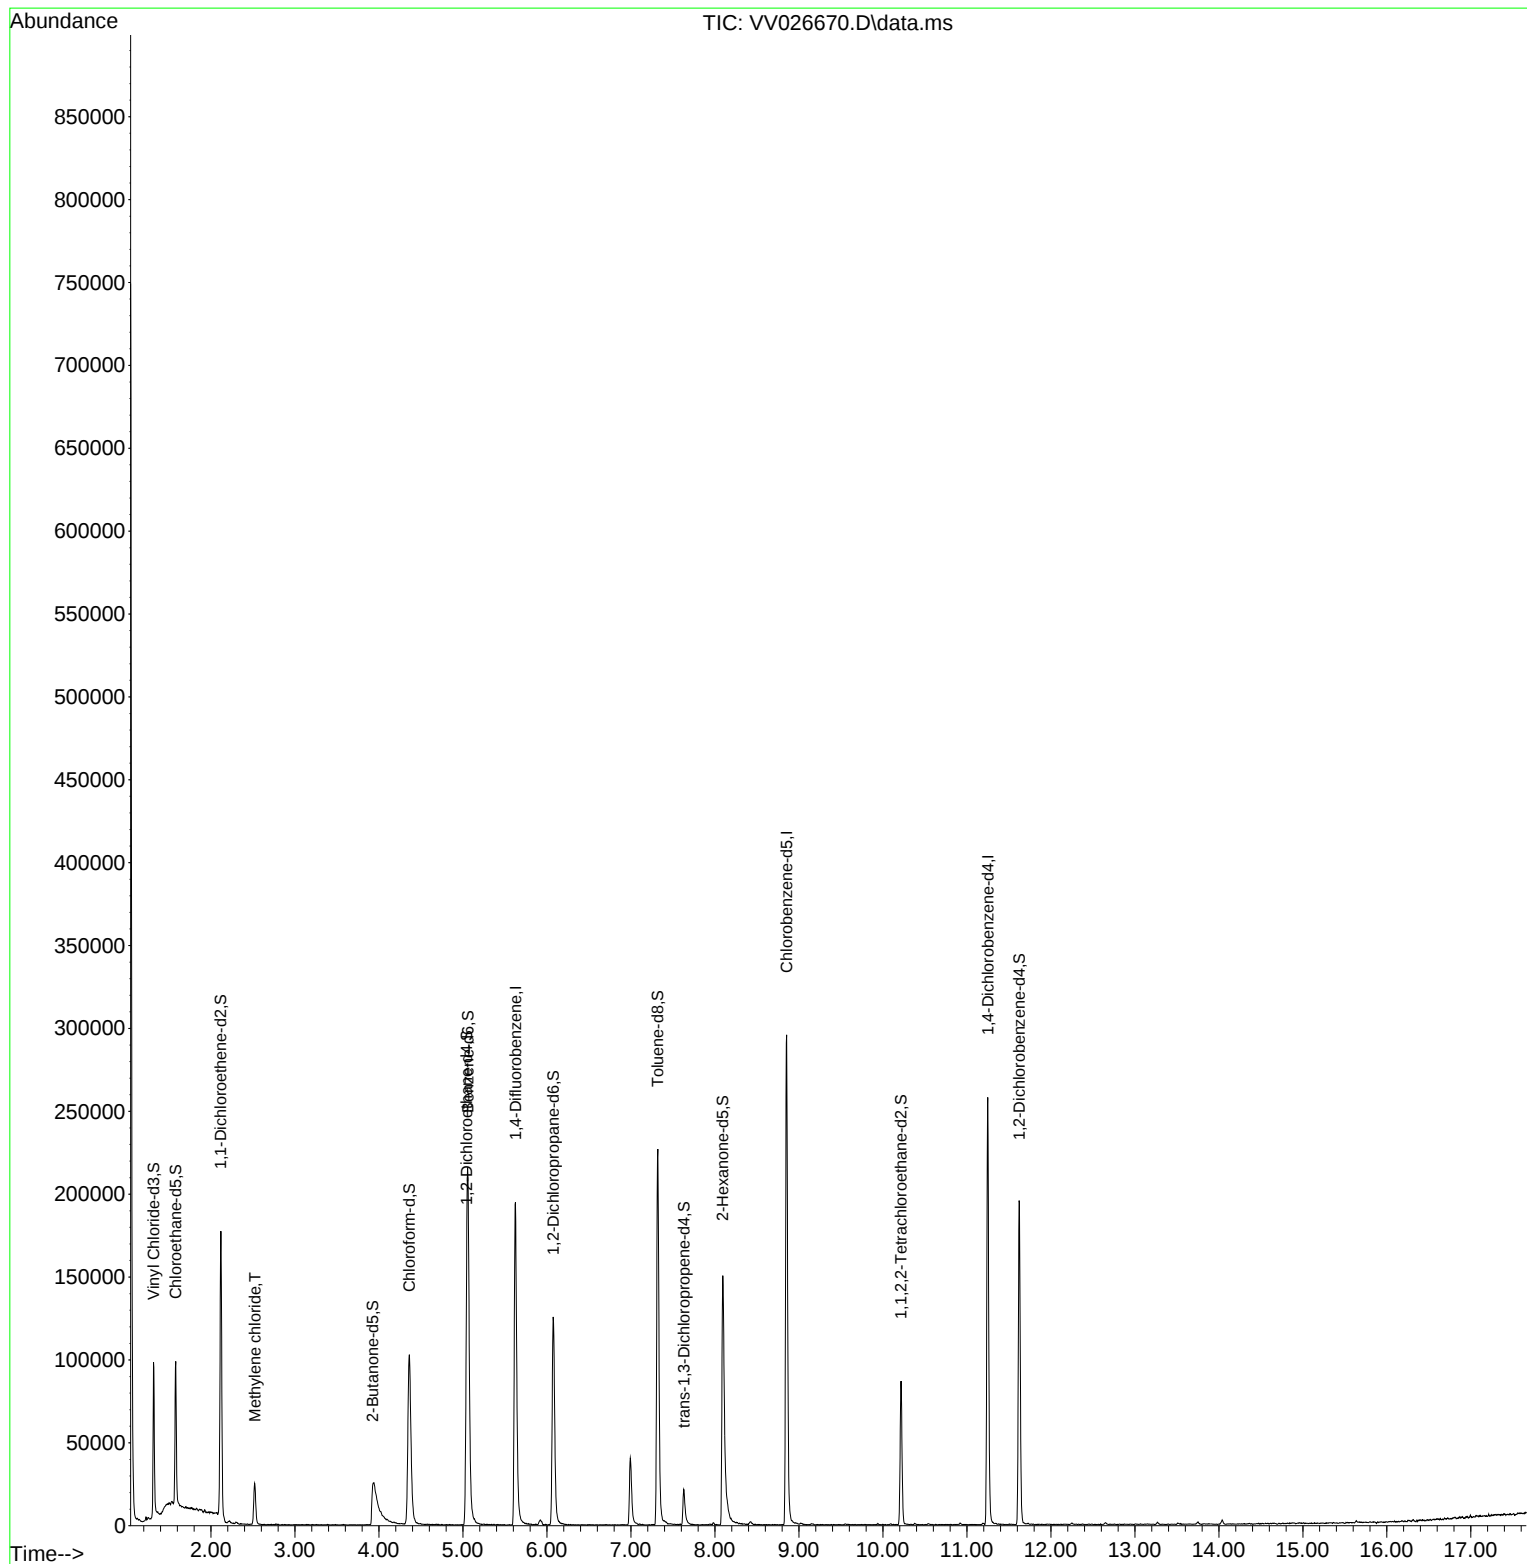

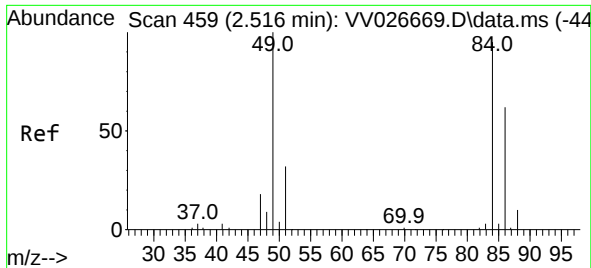

#16
Methylene chloride
Concen: 0.927 ug/L
RT: 2.523 min Scan# 4
Delta R.T. 0.006 min
Lab File: VV026670.D
Acq: 07 Jul 2022 11:06

Instrument :
MSVOA_V
ClientSampleId :
VBLK390

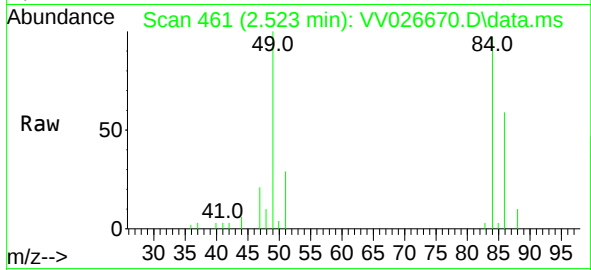

Tgt Ion: 84 Resp: 11847

Ion	Ratio	Lower	Upper
84	100		
86	61.5	46.0	85.4
49	103.6	77.7	144.3

