

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070722\
 Data File : VV026675.D
 Acq On : 07 Jul 2022 13:53
 Operator : SY/MD
 Sample : N3598-10
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AN9

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV026675.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.320	77	87	102	rBV	86728	115467	22.39%	2.522%
2	1.581	162	168	180	rVB	78638	90395	17.53%	1.975%
3	2.121	326	336	352	rVB	157356	234722	45.52%	5.128%
4	2.304	385	393	411	rVB	17696	27504	5.33%	0.601%
5	2.523	450	461	471	rBV	13273	22813	4.42%	0.498%
6	2.587	471	481	494	rVB2	13813	25526	4.95%	0.558%
7	3.934	890	900	937	rBV2	25723	120167	23.31%	2.625%
8	4.378	1017	1038	1068	rBV4	145976	513627	99.62%	11.221%
9	5.056	1225	1249	1275	rBV2	198226	493665	95.74%	10.784%
10	5.625	1414	1426	1452	rBV	202523	416925	80.86%	9.108%
11	5.921	1507	1518	1532	rVB6	3135	6230	1.21%	0.136%
12	6.076	1554	1566	1592	rBV	113760	237385	46.04%	5.186%
13	6.584	1712	1724	1742	rBV6	13034	31251	6.06%	0.683%
14	6.995	1840	1852	1878	rBV	37988	73365	14.23%	1.603%
15	7.143	1885	1898	1916	rBV4	16859	32388	6.28%	0.708%
16	7.320	1942	1953	1972	rBV	215140	379511	73.61%	8.291%
17	7.403	1972	1979	1992	rVB	6014	11348	2.20%	0.248%
18	7.632	2039	2050	2066	rBV2	18544	35648	6.91%	0.779%
19	7.940	2134	2146	2155	rBV2	4615	7698	1.49%	0.168%
20	8.095	2182	2194	2234	rBV2	143640	315116	61.12%	6.884%
21	8.854	2419	2430	2454	rBV	317148	515604	100.00%	11.264%
22	9.137	2509	2518	2534	rVB8	3015	6744	1.31%	0.147%
23	10.217	2843	2854	2874	rBV	78935	125873	24.41%	2.750%
24	10.381	2893	2905	2915	rVB2	9521	15597	3.02%	0.341%
25	11.249	3163	3175	3196	rBV	269567	421495	81.75%	9.208%
26	11.622	3280	3291	3310	rBV	186421	295882	57.39%	6.464%
27	16.561	4821	4827	4834	rBV3	4224	5615	1.09%	0.123%




Sum of corrected areas: 4577561

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070722\
Data File : VV026675.D
Acq On : 07 Jul 2022 13:53
Operator : SY/MD
Sample : N3598-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COAN9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

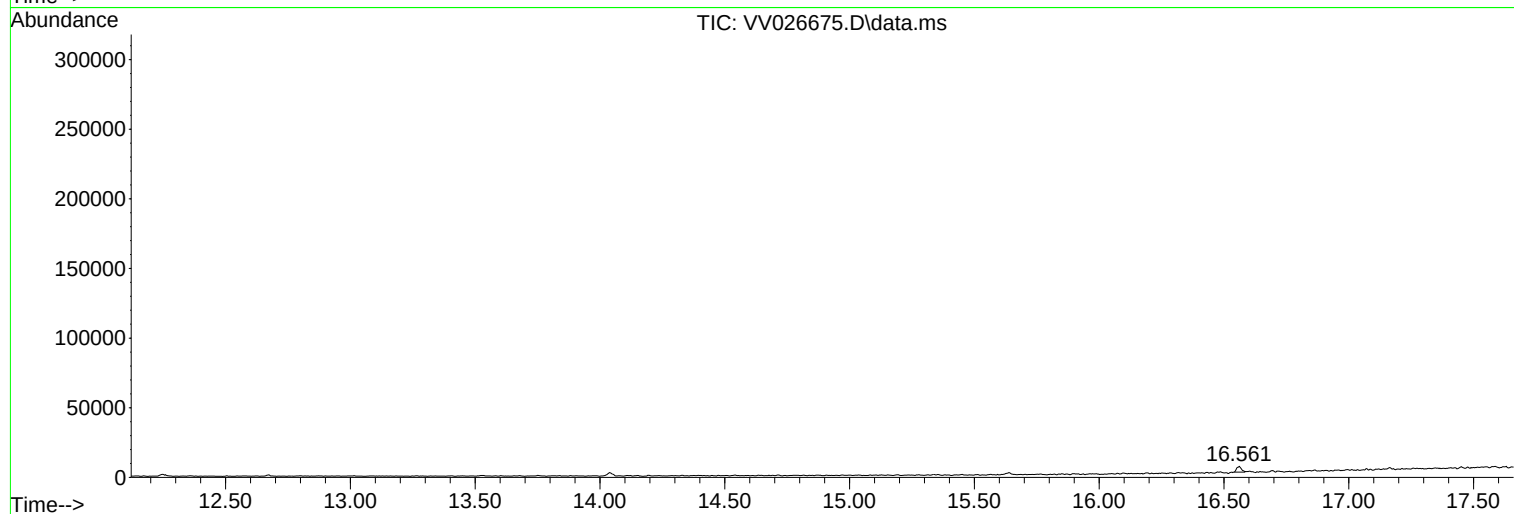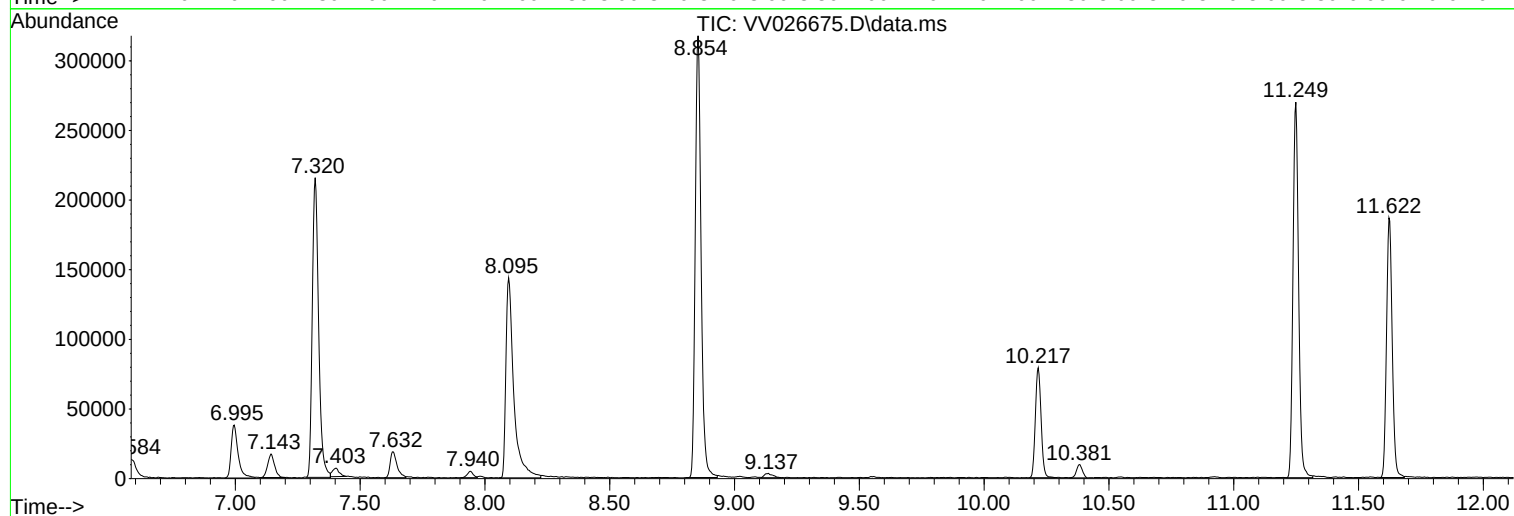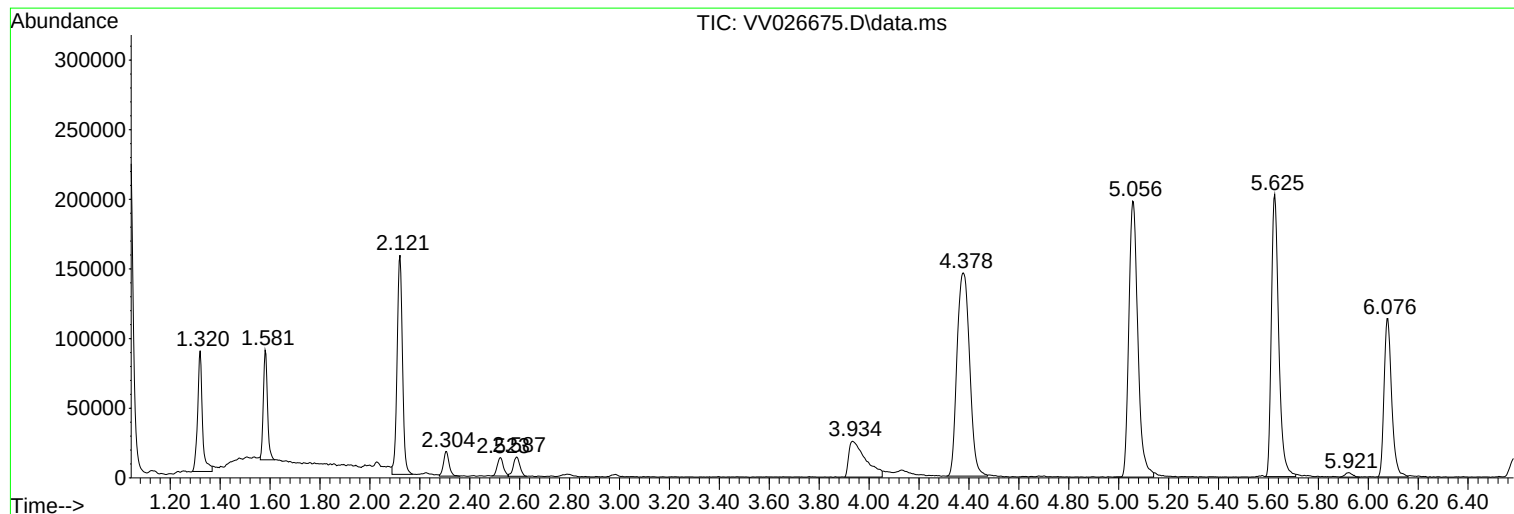

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070722\
Data File : VV026675.D
Acq On : 07 Jul 2022 13:53
Operator : SY/MD
Sample : N3598-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AN9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070722\
Data File : VV026675.D
Acq On : 07 Jul 2022 13:53
Operator : SY/MD
Sample : N3598-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AN9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------