
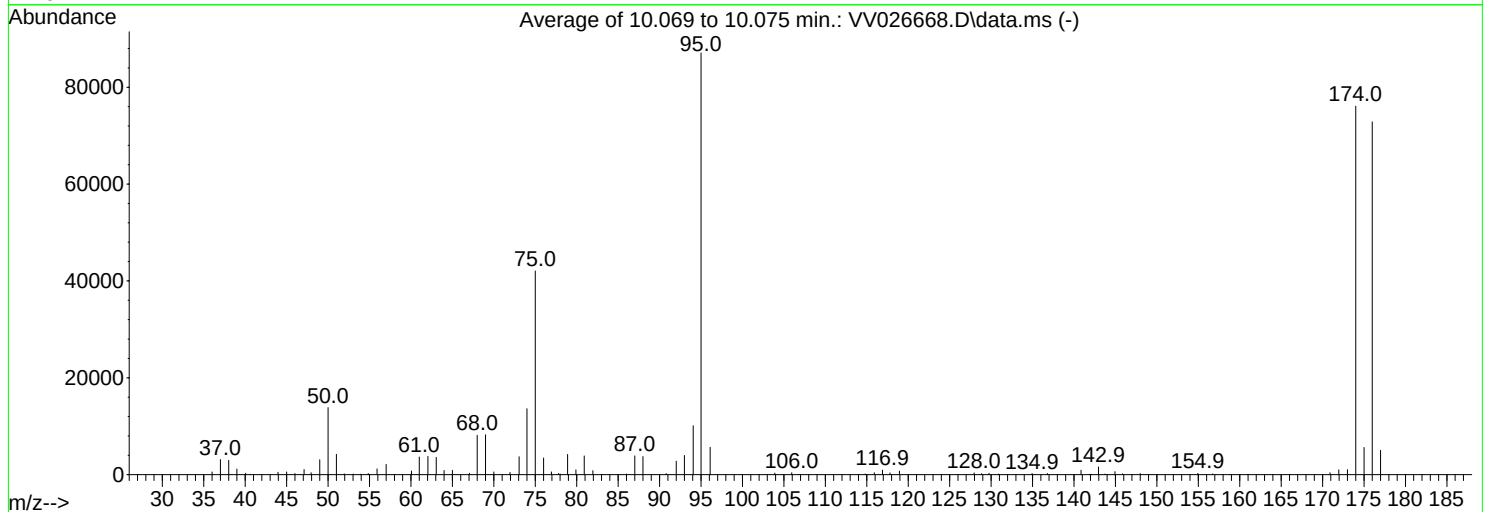


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070722\
Data File : VV026668.D
Acq On : 07 Jul 2022 09:41
Operator : SY/MD
Sample : BFB340
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB340

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Fri Jul 08 23:50:05 2022

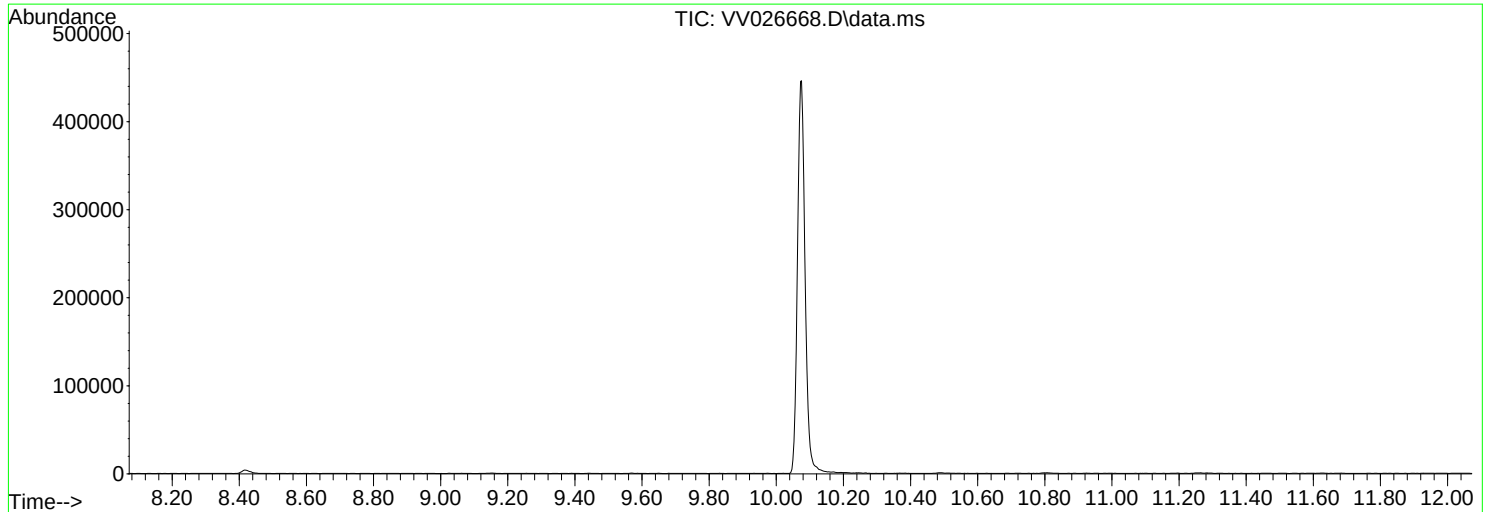

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2796

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.9	13832	PASS
75	95	30	80	48.3	42077	PASS
95	95	100	100	100.0	87099	PASS
96	95	5	9	6.5	5645	PASS
173	174	0.00	2	1.4	1034	PASS
174	95	50	120	87.4	76085	PASS
175	174	5	9	7.4	5606	PASS
176	174	95	105	95.7	72851	PASS
177	176	5	10	6.9	5020	PASS

Scan 2796 (10.030 min): VV026668.D\data.ms
BFB340

m/z	Abundance
39.80	210.0
43.90	338.0

Instrument :
MSVOA_V
ClientSampleId :
BFB340

m/z	Abundance
36.00	524.0
37.00	2879.0
38.00	2938.0
39.00	1140.0
40.00	338.0
40.60	165.0
44.00	752.0
45.00	474.0
46.00	217.0
47.10	1083.0
47.90	405.0
49.00	2940.0
50.00	12984.0
51.00	3964.0
51.90	175.0
53.10	168.0
53.90	117.0
54.90	214.0
55.90	1118.0
57.00	1871.0
60.10	727.0
61.00	3546.0
62.00	3556.0
63.10	3219.0
64.00	890.0
65.00	791.0
67.00	264.0
68.00	7528.0
69.00	7949.0
70.00	543.0
72.00	404.0
73.10	3463.0
74.00	12867.0
75.00	39808.0
76.00	3332.0
76.90	596.0
77.80	352.0
78.90	3930.0
79.90	923.0
80.90	3464.0
81.90	740.0
85.90	114.0
87.00	3382.0
88.00	3502.0
90.80	245.0
92.00	2471.0
93.00	3495.0
94.10	9556.0
95.00	81200.0
96.10	5280.0
97.00	109.0
103.90	288.0
105.90	363.0
114.80	115.0
115.90	368.0
116.90	848.0
117.80	365.0
119.00	667.0
127.90	391.0
128.90	195.0
129.80	298.0
130.90	133.0
135.00	237.0
136.80	256.0
140.80	797.0
141.80	101.0
143.00	1432.0
143.80	112.0
144.90	526.0
145.80	184.0
148.00	220.0
149.90	106.0
155.00	181.0
156.70	149.0
171.00	380.0
172.00	799.0
173.00	879.0
174.00	69280.0
175.00	5118.0
176.00	66376.0
177.00	4518.0
178.00	135.0

Instrument :
MSVOA_V
ClientSampleId :
BFB340

m/z	Abundance
36.00	580.0
37.00	3192.0
38.00	3070.0
39.00	1199.0
40.00	306.0
44.00	858.0
45.00	617.0
46.00	224.0
47.10	1095.0
48.00	413.0
49.00	3187.0
50.00	14320.0
51.00	4407.0
52.00	151.0
53.00	146.0
54.00	121.0
54.90	257.0
55.90	1210.0
57.00	2191.0
60.00	791.0
61.00	3704.0
62.10	3841.0
63.10	3692.0
64.00	924.0
65.00	913.0
67.10	303.0
68.00	8448.0
69.00	8520.0
70.00	572.0
72.00	495.0
73.10	3829.0
74.00	14053.0
75.00	43792.0
76.00	3581.0
76.90	593.0
77.80	364.0
78.90	4289.0
79.90	1024.0
80.90	3973.0
81.90	822.0
86.00	117.0
87.00	4032.0
88.00	3878.0
90.80	260.0
92.00	2908.0
93.00	4164.0
94.00	10436.0
95.00	90104.0
96.10	5856.0
97.00	103.0
103.90	341.0
104.90	100.0
105.90	417.0
106.80	102.0
114.80	145.0
115.90	406.0
116.90	981.0
117.80	373.0
118.90	770.0
128.00	384.0
128.80	223.0
129.80	305.0
130.90	158.0
134.90	240.0
136.80	270.0
140.90	936.0
141.90	128.0
142.90	1647.0
143.80	148.0
145.00	626.0
145.80	184.0
147.00	103.0
148.00	266.0
150.00	103.0
154.90	292.0
156.80	179.0
158.80	110.0
161.00	129.0
170.90	402.0
172.00	1003.0
173.00	1093.0
174.00	78760.0
175.00	5862.0
176.00	75168.0
177.00	5247.0
178.00	114.0

Instrument :
MSVOA_V
ClientSampleId :
BFB340

m/z	Abundance
36.00	559.0
37.00	3278.0
38.00	2809.0
39.00	1134.0
40.10	282.0
44.00	869.0
45.00	624.0
46.00	207.0
47.10	971.0
48.00	403.0
49.00	3146.0
50.00	14193.0
51.00	4220.0
52.00	186.0
53.00	130.0
54.00	115.0
54.80	249.0
55.90	1265.0
57.00	2272.0
60.00	780.0
61.00	3701.0
62.10	3885.0
63.00	3775.0
64.00	785.0
65.00	952.0
67.10	289.0
68.00	8427.0
69.00	8244.0
70.00	578.0
71.90	490.0
73.00	3796.0
74.00	13935.0
75.00	42632.0
76.00	3393.0
77.00	531.0
78.00	365.0
78.90	4289.0
79.90	1062.0
80.90	4205.0
82.00	879.0
86.10	132.0
87.00	4216.0
88.00	3783.0
90.80	245.0
92.00	2972.0
93.00	4285.0
94.00	10321.0
95.00	89992.0
96.10	5798.0
103.90	352.0
104.90	107.0
106.00	446.0
108.00	140.0
114.80	128.0
115.90	393.0
116.90	943.0
117.80	347.0
118.90	757.0
128.00	338.0
128.80	207.0
129.70	269.0
130.90	141.0
134.90	186.0
136.80	223.0
140.90	1016.0
142.10	146.0
142.90	1708.0
143.70	136.0
145.00	713.0
145.90	173.0
148.00	254.0
154.90	354.0
156.80	180.0
161.00	134.0
170.80	389.0
171.90	1168.0
173.00	1131.0
174.00	80216.0
175.00	5838.0
176.00	77008.0
177.00	5294.0

Instrument :
MSVOA_V
ClientSampleId :
BFB340