
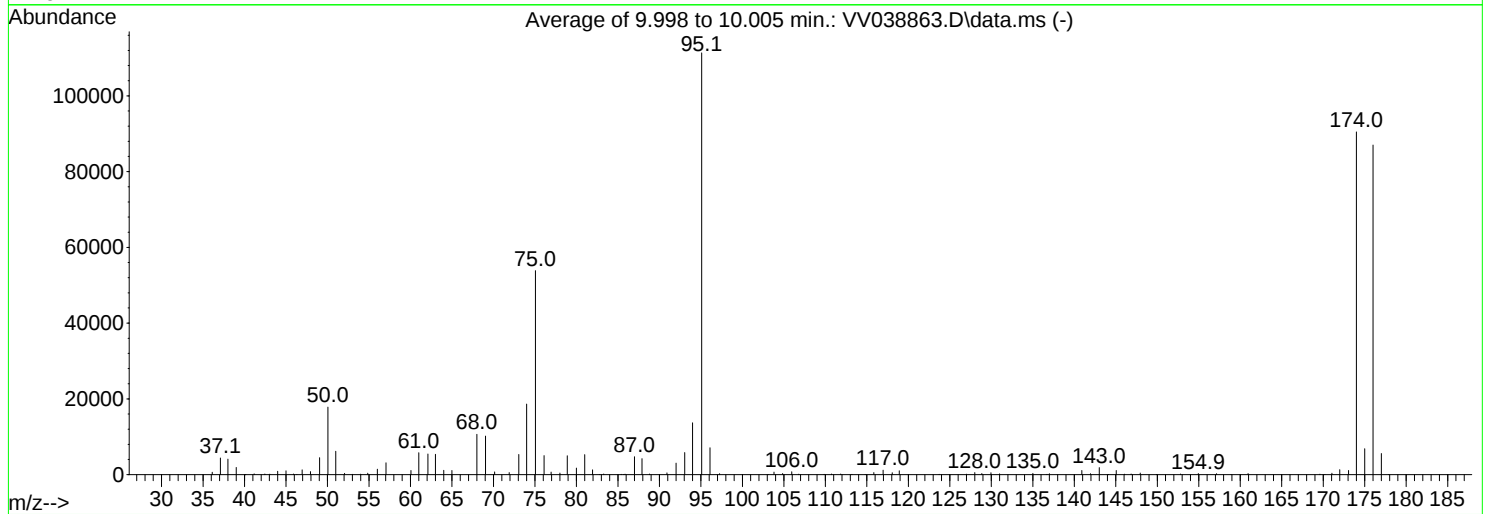


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV070725\
Data File : VV038863.D
Acq On : 07 Jul 2025 08:04
Operator : SY/MD
Sample : BFB
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\82V070225W.M
Title : SW846 8260
Last Update : Thu Jul 03 02:44:44 2025

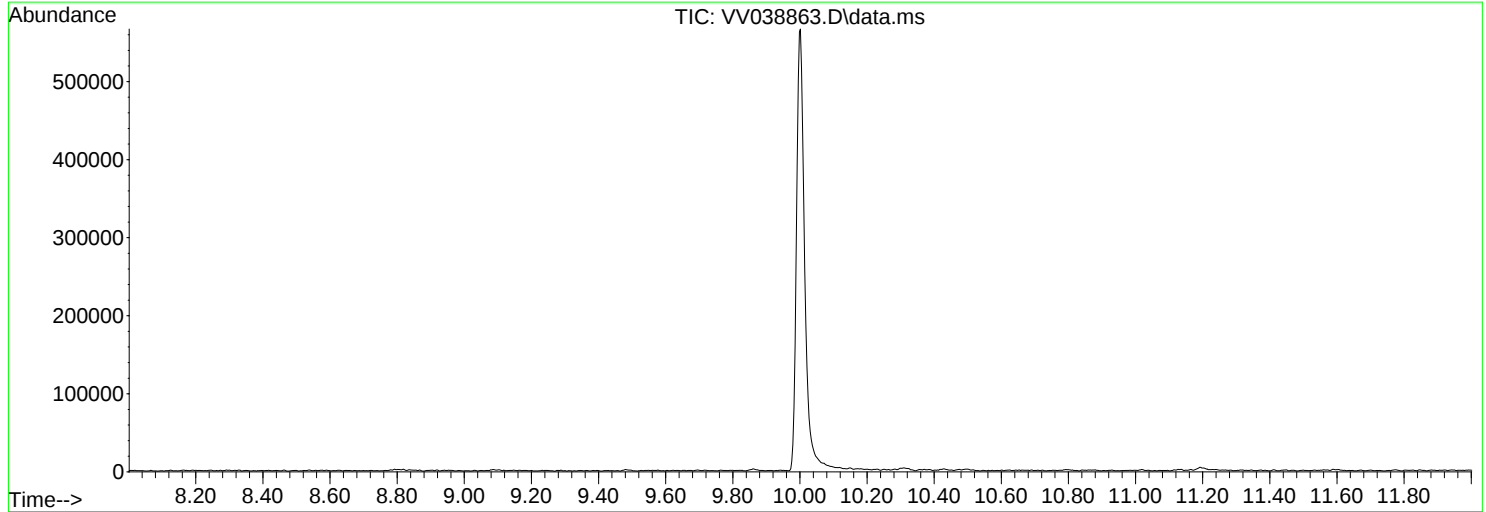

AutoFind: Scans 2786, 2787, 2788; Background Corrected with Scan 2775

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.0	17835	PASS
75	95	30	60	48.4	53880	PASS
95	95	100	100	100.0	111357	PASS
96	95	5	9	6.4	7107	PASS
173	174	0.00	2	1.2	1100	PASS
174	95	50	100	81.3	90483	PASS
175	174	5	9	7.6	6834	PASS
176	174	95	101	96.2	87008	PASS
177	176	5	9	6.4	5565	PASS