


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV070819\
Data File : VV011831.D
Acq On : 08 Jul 2019 10:58
Operator : SY/MD
Sample : BFB09
Misc : 25ML/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB091

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR070819SIM.M
Title : TRACE VOA SOM01.0
Last Update : Mon Jul 15 07:23:05 2019

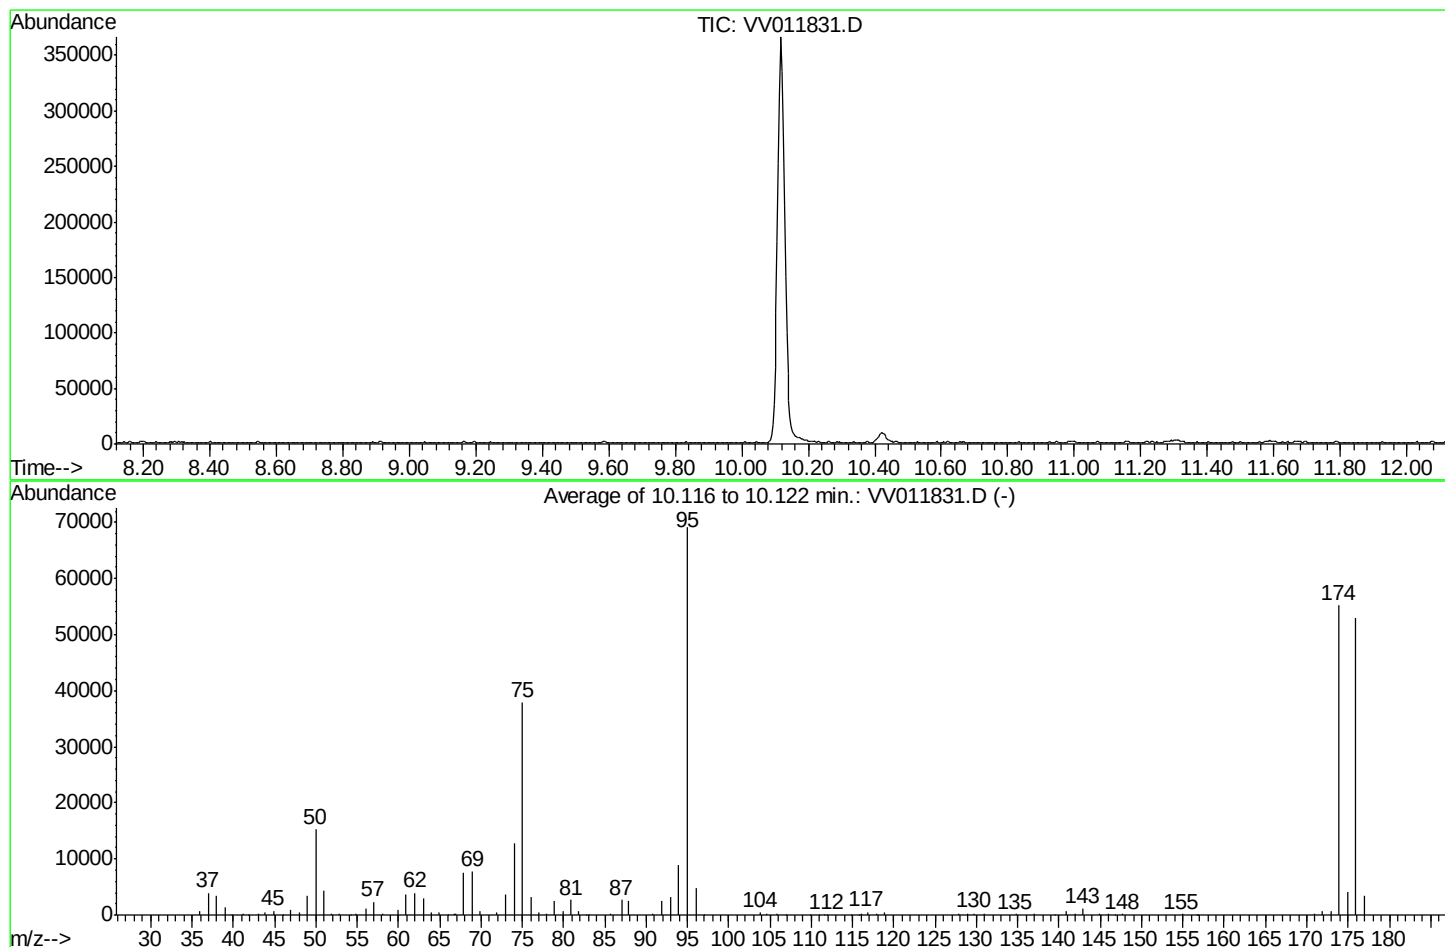

AutoFind: Scans 2807, 2808, 2809; Background Corrected with Scan 2794

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.0	15220	PASS
75	95	30	80	54.8	37866	PASS
95	95	100	100	100.0	69117	PASS
96	95	5	9	7.1	4873	PASS
173	174	0.00	2	1.1	606	PASS
174	95	50	120	79.8	55160	PASS
175	174	5	9	7.3	4011	PASS
176	174	95	101	96.2	53064	PASS
177	176	5	9	6.5	3429	PASS

m/z	Abundance
36.00	186.0
36.80	133.0
39.90	225.0
40.80	104.0
43.90	555.0
44.80	106.0
54.80	109.0
63.00	129.0

Instrument :
MSVOA_V
ClientSampleId :
BFB091

m/z	Abundance
35.90	912.0
37.00	4139.0
37.90	3476.0
39.00	1622.0
39.90	285.0
41.20	145.0
41.70	106.0
43.00	162.0
43.90	1059.0
44.90	784.0
46.90	971.0
48.00	490.0
49.00	3488.0
50.00	15786.0
50.90	4589.0
51.90	261.0
52.90	158.0
54.20	101.0
55.00	363.0
56.00	1269.0
56.90	2376.0
58.10	127.0
59.90	849.0
60.90	3872.0
62.00	4212.0
63.00	3237.0
64.00	488.0
65.00	537.0
65.90	105.0
66.80	238.0
67.00	230.0
67.90	7585.0
69.00	7975.0
69.90	721.0
71.90	466.0
73.00	3946.0
74.00	12933.0
75.00	38664.0
76.00	3500.0
76.90	553.0
77.90	291.0
78.90	2652.0
79.90	790.0
80.90	2909.0
81.80	635.0
82.70	128.0
85.70	134.0
87.00	2751.0
87.90	2633.0
90.70	269.0
92.00	2654.0
92.90	3318.0
93.90	9349.0
95.00	70408.0
96.00	4982.0
97.00	139.0
103.90	367.0
104.60	170.0
106.00	339.0
106.90	102.0
111.60	127.0
111.90	134.0
114.80	139.0
115.80	315.0
116.80	519.0
117.80	333.0
118.90	389.0
127.80	208.0
128.90	178.0
129.80	210.0
130.90	119.0
134.70	165.0
137.00	174.0
139.50	109.0
140.80	848.0
141.90	160.0
142.90	1157.0
144.80	228.0
145.90	159.0
147.70	178.0
155.00	138.0
156.90	125.0
171.00	132.0
171.90	661.0
173.00	898.0
173.90	54352.0
174.90	4026.0
175.90	52512.0
176.90	3347.0

Instrument :
MSVOA_V
ClientSampleId :
BFB091

m/z	Abundance
35.90	888.0
37.00	4204.0
37.90	3470.0
39.00	1522.0
39.80	319.0
41.20	153.0
41.70	117.0
43.00	154.0
43.90	992.0
45.00	847.0
46.90	1040.0
47.90	497.0
48.90	3703.0
50.00	15713.0
51.00	4469.0
51.90	227.0
52.80	164.0
55.00	309.0
56.00	1230.0
56.90	2433.0
58.00	135.0
60.00	891.0
60.90	3922.0
62.00	4133.0
63.00	3227.0
64.00	407.0
65.00	496.0
66.00	121.0
66.90	226.0
67.90	7916.0
69.00	7910.0
69.90	682.0
72.00	523.0
73.00	3776.0
74.00	13163.0
75.00	39320.0
76.00	3395.0
76.90	497.0
78.00	278.0
78.90	2677.0
79.90	826.0
80.90	2749.0
81.90	609.0
83.10	121.0
85.70	125.0
87.00	2722.0
87.90	2576.0
90.70	307.0
92.00	2500.0
92.90	3313.0
93.90	9378.0
95.00	71344.0
96.00	5036.0
97.00	112.0
103.80	338.0
104.70	167.0
105.90	312.0
106.90	120.0
109.80	111.0
110.90	112.0
111.90	116.0
114.80	123.0
116.00	284.0
116.80	516.0
117.90	349.0
118.80	398.0
127.80	221.0
128.90	211.0
129.70	231.0
130.90	130.0
134.80	188.0
137.00	195.0
140.80	741.0
141.90	151.0
142.90	1178.0
144.90	221.0
145.90	149.0
147.80	169.0
154.90	171.0
170.90	159.0
171.80	608.0
173.00	922.0
173.90	57368.0
174.90	4156.0
175.90	55128.0
176.90	3557.0

Instrument :
MSVOA_V
ClientSampleId :
BFB091

m/z	Abundance
35.90	767.0
37.00	3772.0
37.90	3164.0
38.90	1328.0
39.80	331.0
40.80	119.0
41.20	130.0
41.80	125.0
43.00	111.0
43.90	953.0
45.00	790.0
46.00	103.0
46.90	976.0
47.90	497.0
48.90	3275.0
50.00	14162.0
51.00	4019.0
51.90	216.0
52.90	133.0
54.20	112.0
54.90	234.0
56.00	1050.0
57.00	2331.0
58.00	146.0
60.00	802.0
60.90	3471.0
62.00	3633.0
63.00	2907.0
63.90	311.0
64.90	427.0
66.00	129.0
66.80	200.0
67.90	7415.0
69.00	7106.0
69.90	591.0
72.00	464.0
73.00	3112.0
74.00	12174.0
75.00	35616.0
76.00	2872.0
77.00	417.0
78.10	321.0
78.90	2453.0
79.90	780.0
80.90	2335.0
81.90	563.0
83.10	126.0
85.80	135.0
87.00	2530.0
87.90	2341.0
90.80	323.0
91.90	2128.0
92.90	2968.0
94.00	8278.0
95.00	65600.0
96.00	4603.0
96.80	117.0
103.80	367.0
104.70	159.0
105.80	312.0
106.80	134.0
109.80	114.0
110.90	129.0
116.00	273.0
116.80	529.0
118.00	342.0
118.80	391.0
127.80	221.0
128.80	193.0
129.70	258.0
130.90	126.0
134.80	196.0
137.00	168.0
140.80	607.0
141.90	137.0
142.90	983.0
144.80	198.0
145.90	128.0
146.80	103.0
147.80	165.0
154.90	186.0
156.60	103.0
170.80	146.0
171.90	512.0
173.90	53760.0
174.90	3852.0
175.90	51552.0
176.90	3385.0

Instrument :
MSVOA_V
ClientSampleId :
BFB091