


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV070820\
 Data File : VV017385.D
 Acq On : 08 Jul 2020 09:34
 Operator : SY/MD
 Sample : BFB97
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB97

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM070820WMA.M
 Title : VOC Analysis
 Last Update : Thu Jul 09 02:01:52 2020

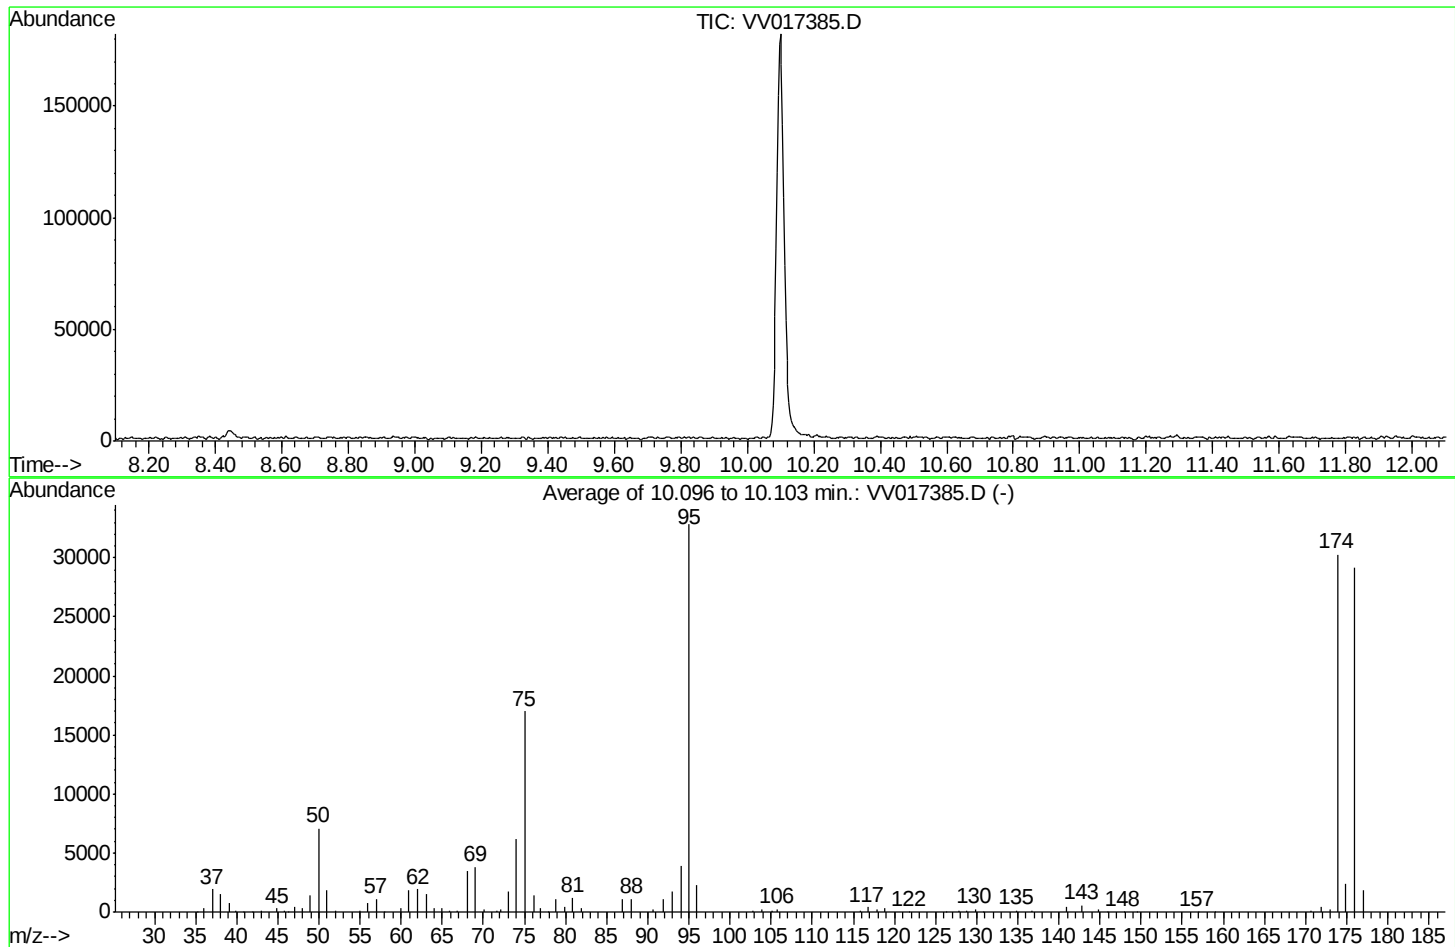

AutoFind: Scans 2801, 2802, 2803; Background Corrected with Scan 2790

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.6	7096	PASS
75	95	30	80	51.7	16977	PASS
95	95	100	100	100.0	32832	PASS
96	95	5	9	7.0	2302	PASS
173	174	0.00	2	0.7	205	PASS
174	95	50	120	92.2	30264	PASS
175	174	5	9	7.8	2354	PASS
176	174	95	101	96.3	29144	PASS
177	176	5	9	6.5	1893	PASS

m/z	Abundance
35.30	153.0
36.00	453.0
37.00	1834.0
38.00	1590.0
39.10	832.0
40.00	329.0
40.80	147.0
42.90	139.0
44.00	336.0
44.90	373.0
45.80	127.0
47.00	450.0
48.00	319.0
48.90	1486.0
50.00	7159.0
51.00	2002.0
52.10	179.0
55.10	226.0
56.00	776.0
57.00	1033.0
59.90	347.0
61.00	1848.0
62.00	1927.0
63.00	1634.0
64.00	333.0
65.00	330.0
65.90	115.0
66.70	133.0
68.00	3498.0
69.00	3785.0
70.10	175.0
72.10	173.0
73.00	1813.0
74.00	6315.0
75.00	17992.0
76.10	1524.0
76.90	417.0
78.90	1073.0
79.80	436.0
80.90	1188.0
81.80	279.0
87.00	1011.0
88.00	1088.0
90.70	273.0
91.90	1049.0
92.90	1792.0
94.00	4053.0
95.00	33808.0
96.00	2188.0
102.80	122.0
103.90	176.0
105.80	228.0
115.90	162.0
116.80	435.0
117.90	139.0
118.90	263.0
126.30	105.0
127.80	108.0
128.70	150.0
129.80	205.0
130.80	107.0
134.90	118.0
140.90	406.0
142.80	584.0
144.80	144.0
145.90	102.0
149.50	106.0
156.90	106.0
158.90	105.0
170.60	129.0
172.00	397.0
173.90	30064.0
174.90	2273.0
175.90	28768.0
177.00	1902.0

Instrument :
MSVOA_V
ClientSampleId :
BFB97

m/z	Abundance
35.30	143.0
36.00	372.0
37.00	2013.0
38.00	1630.0
39.00	798.0
40.00	318.0
40.80	168.0
41.90	105.0
42.90	148.0
44.00	358.0
44.90	320.0
45.70	124.0
47.00	392.0
47.90	355.0
48.90	1488.0
50.00	7290.0
51.00	2020.0
52.10	158.0
55.00	166.0
56.00	808.0
57.00	1165.0
59.90	355.0
61.00	1873.0
62.00	1987.0
63.00	1533.0
64.00	335.0
65.00	342.0
65.90	118.0
66.80	137.0
68.00	3604.0
69.00	3992.0
70.10	209.0
71.60	133.0
72.10	198.0
73.00	1797.0
74.00	6319.0
75.00	17448.0
76.10	1438.0
76.90	369.0
78.80	1132.0
79.80	416.0
80.80	1323.0
81.90	295.0
87.00	1124.0
88.00	1196.0
90.70	173.0
92.00	1193.0
92.90	1844.0
94.00	4065.0
95.00	33880.0
96.00	2408.0
102.80	129.0
103.90	224.0
105.00	145.0
105.80	262.0
115.80	122.0
116.70	482.0
117.90	178.0
118.70	301.0
127.80	167.0
128.80	170.0
129.80	233.0
134.90	160.0
136.70	112.0
140.90	493.0
142.80	600.0
144.80	209.0
170.60	141.0
171.90	453.0
173.90	31456.0
174.90	2458.0
175.90	30304.0
177.00	2012.0

Instrument :
MSVOA_V
ClientSampleId :
BFB97

m/z	Abundance
35.30	116.0
36.00	272.0
37.00	1931.0
38.00	1493.0
39.00	695.0
40.00	255.0
40.90	153.0
43.00	106.0
44.10	403.0
44.90	279.0
46.30	101.0
47.00	339.0
47.90	368.0
48.90	1424.0
50.00	6841.0
51.00	1843.0
51.90	152.0
55.10	104.0
55.90	670.0
57.00	1062.0
57.90	123.0
60.00	412.0
60.90	1684.0
62.00	1830.0
63.00	1277.0
64.00	328.0
65.00	318.0
68.00	3363.0
69.00	3691.0
70.00	220.0
71.60	149.0
72.10	169.0
73.00	1535.0
74.00	5843.0
75.00	15493.0
76.10	1293.0
76.90	273.0
77.90	107.0
78.80	1149.0
79.90	365.0
80.80	1239.0
81.90	313.0
86.90	1180.0
88.00	1125.0
90.60	130.0
92.00	1181.0
92.90	1636.0
94.00	3758.0
95.00	30808.0
96.00	2311.0
103.90	212.0
105.10	134.0
105.80	207.0
115.70	114.0
116.70	367.0
117.80	199.0
118.70	292.0
121.80	112.0
127.80	189.0
128.80	151.0
129.80	216.0
134.90	205.0
136.60	116.0
136.80	109.0
140.90	448.0
142.80	572.0
144.80	208.0
147.90	118.0
170.60	137.0
171.90	494.0
173.00	616.0
173.90	29272.0
174.90	2331.0
175.90	28360.0
177.00	1767.0

Instrument :
MSVOA_V
ClientSampleId :
BFB97

m/z	Abundance
35.20	107.0
36.50	104.0
38.80	111.0
39.80	205.0
40.70	106.0
41.50	106.0
44.00	367.0
47.50	104.0
50.80	143.0
77.60	124.0

Instrument :
MSVOA_V
ClientSampleId :
BFB97