

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW070822\
 Data File : VW026706.D
 Acq On : 08 Jul 2022 19:13
 Operator : SY/MD
 Sample : N3601-22 50X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUB7

Quant Time: Jul 08 23:59:20 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Jul 08 23:50:05 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.625	114	179216	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	173175	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	69432	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.320	65	53158	3.688	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	73.800%	
7) Chloroethane-d5	1.584	69	51481	4.446	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	89.000%	
11) 1,1-Dichloroethene-d2	2.121	63	75159	2.935	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	58.600%#	
20) 2-Butanone-d5	3.928	46	62418	43.560	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	87.120%	
24) Chloroform-d	4.365	84	113415	4.814	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	96.200%	
26) 1,2-Dichloroethane-d4	5.044	65	45426	5.006	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	100.200%	
32) Benzene-d6	5.060	84	197554	3.972	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	79.400%	
36) 1,2-Dichloropropane-d6	6.076	67	63724	4.659	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	93.200%	
41) Toluene-d8	7.320	98	142838	3.193	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	63.800%#	
43) trans-1,3-Dichloroprop...	7.629	79	12292	3.477	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	69.600%	
46) 2-Hexanone-d5	8.095	63	61270	45.496	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	91.000%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	46624	5.210	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	104.200%	
66) 1,2-Dichlorobenzene-d4	11.622	152	52900	4.604	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	92.000%	
Target Compounds						Qvalue
16) Methylene chloride	2.523	84	8794	0.684	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070822\
Data File : VV026706.D
Acq On : 08 Jul 2022 19:13
Operator : SY/MD
Sample : N3601-22 50X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUB7


Quant Time: Jul 08 23:59:20 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Jul 08 23:50:05 2022
Response via : Initial Calibration

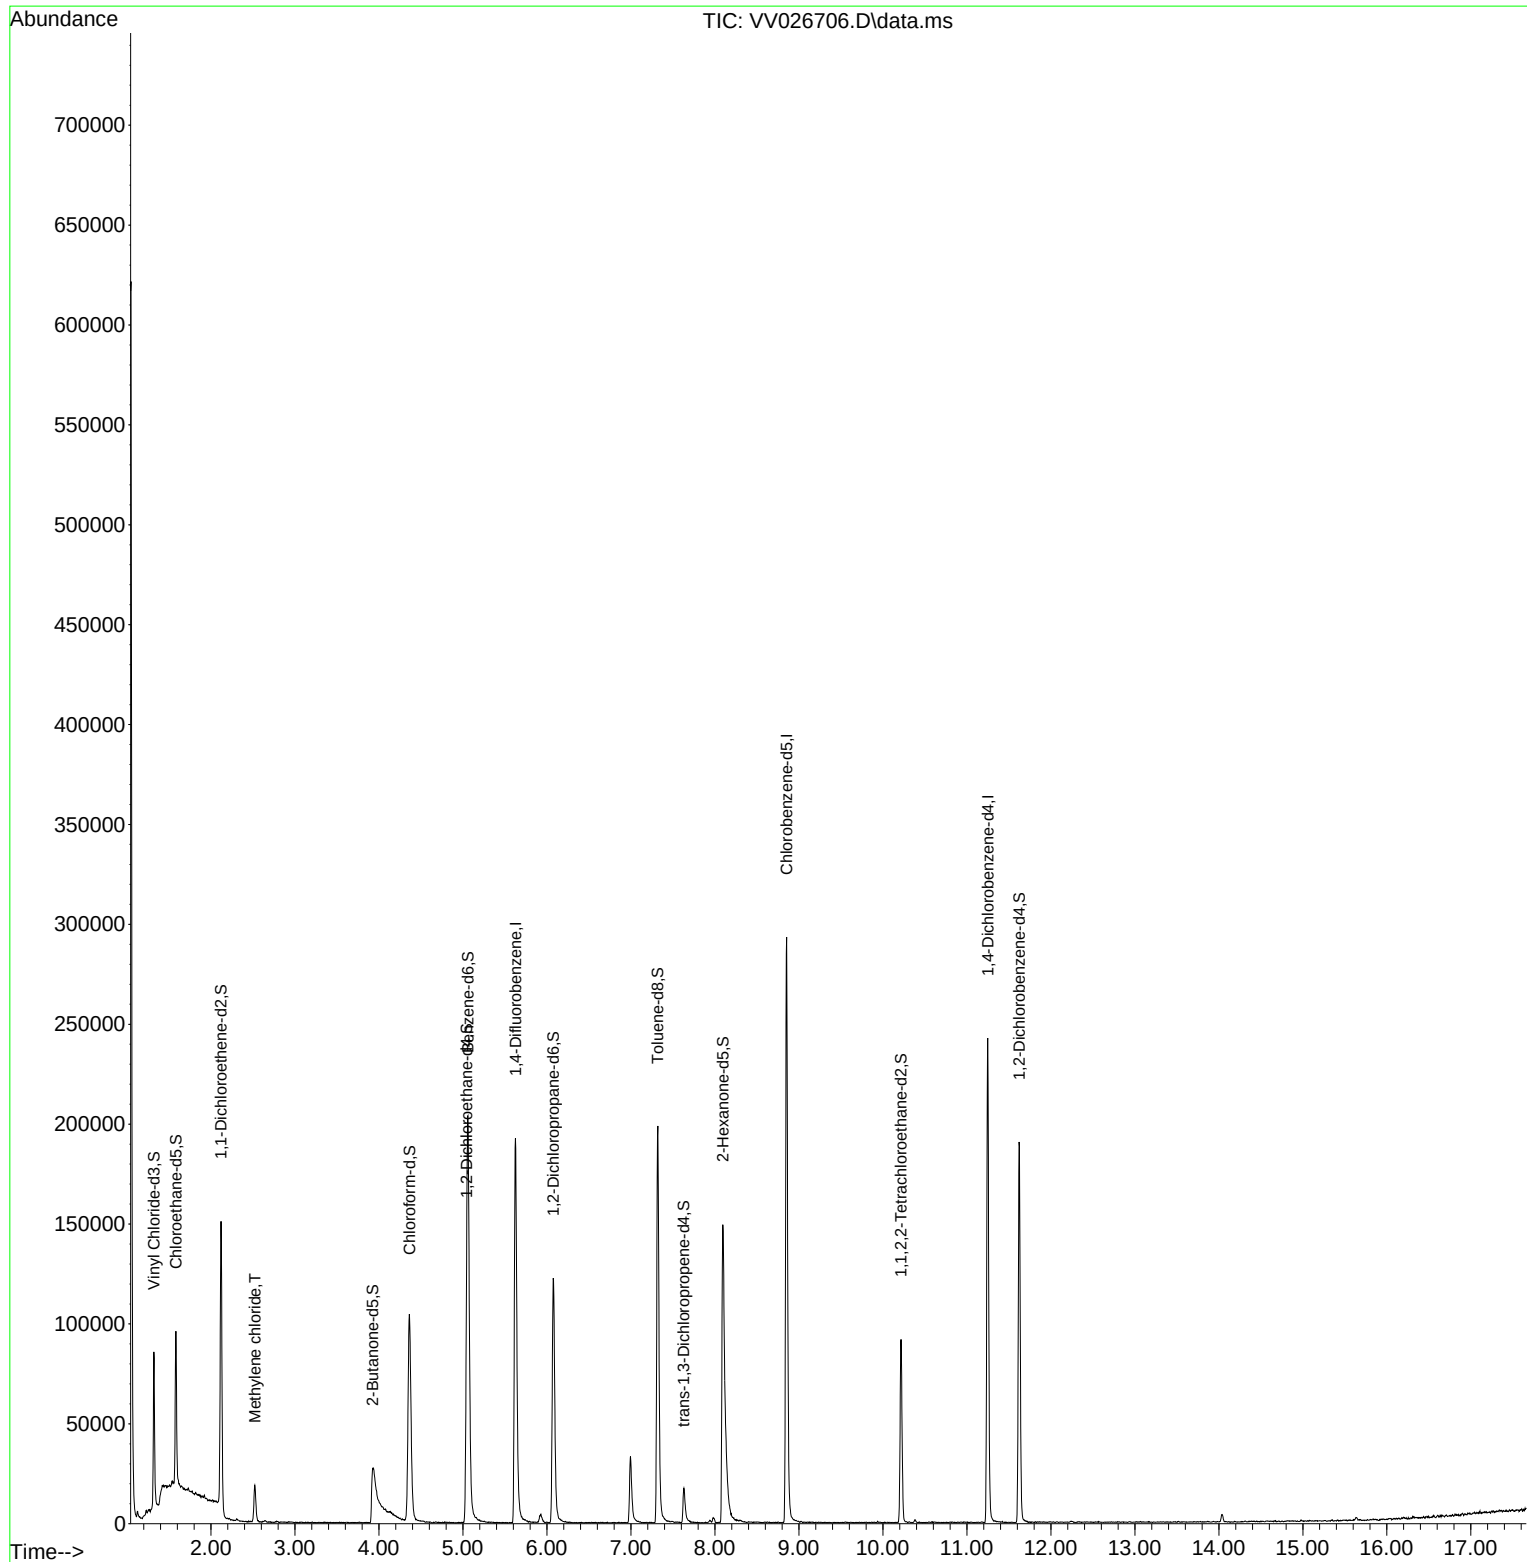

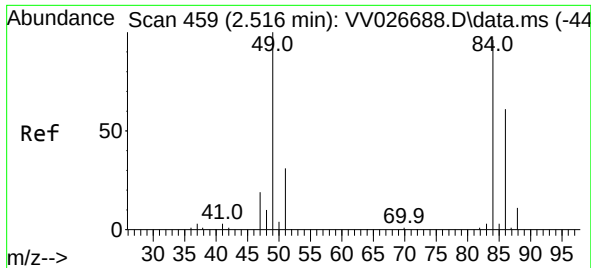

#16
Methylene chloride
Concen: 0.684 ug/L
RT: 2.523 min Scan# 4
Delta R.T. 0.007 min
Lab File: VV026706.D
Acq: 08 Jul 2022 19:13

Instrument :
MSVOA_V
ClientSampleId :
DBUB7

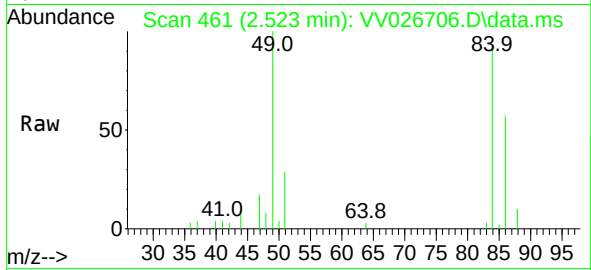

Tgt Ion: 84 Resp: 8794

Ion	Ratio	Lower	Upper
84	100		
86	61.8	46.0	85.4
49	108.8	77.7	144.3

