

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070822\
 Data File : VV026690.D
 Acq On : 08 Jul 2022 12:15
 Operator : SY/MD
 Sample : N3601-13
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUC0

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV026690.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.198	40	49	50	rBV2	9166	10274	1.51%	0.224%
2	1.311	78	84	97	rVB	91247	94834	13.96%	2.064%
3	1.574	159	166	178	rBV	87453	103831	15.28%	2.260%
4	2.111	324	333	344	rVB	172756	243297	35.82%	5.295%
5	3.954	889	906	925	rBV2	55996	185879	27.36%	4.045%
6	4.362	1017	1033	1057	rBV2	123562	297891	43.85%	6.483%
7	5.047	1231	1246	1266	rBV3	313285	679314	100.00%	14.784%
8	5.606	1408	1420	1435	rBV	289598	543501	80.01%	11.828%
9	6.053	1548	1559	1576	rVB	147292	292211	43.02%	6.359%
10	6.976	1834	1846	1859	rBV	38813	69131	10.18%	1.504%
11	7.310	1937	1950	1966	rBV	240705	421944	62.11%	9.183%
12	7.387	1966	1974	1993	rVV	20685	43312	6.38%	0.943%
13	7.635	2040	2051	2063	rBV3	18968	31990	4.71%	0.696%
14	7.953	2139	2150	2158	rBV2	5445	10154	1.49%	0.221%
15	8.117	2190	2201	2230	rBV2	165936	334234	49.20%	7.274%
16	8.857	2420	2431	2452	rBV	279754	448394	66.01%	9.758%
17	10.220	2842	2855	2872	rBV	86012	134453	19.79%	2.926%
18	10.381	2891	2905	2919	rBV	10294	16814	2.48%	0.366%
19	11.249	3163	3175	3194	rBV	226421	345882	50.92%	7.527%
20	11.622	3281	3291	3308	rBV	184502	287740	42.36%	6.262%




Sum of corrected areas: 4595080

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070822\
Data File : VV026690.D
Acq On : 08 Jul 2022 12:15
Operator : SY/MD
Sample : N3601-13
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUC0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

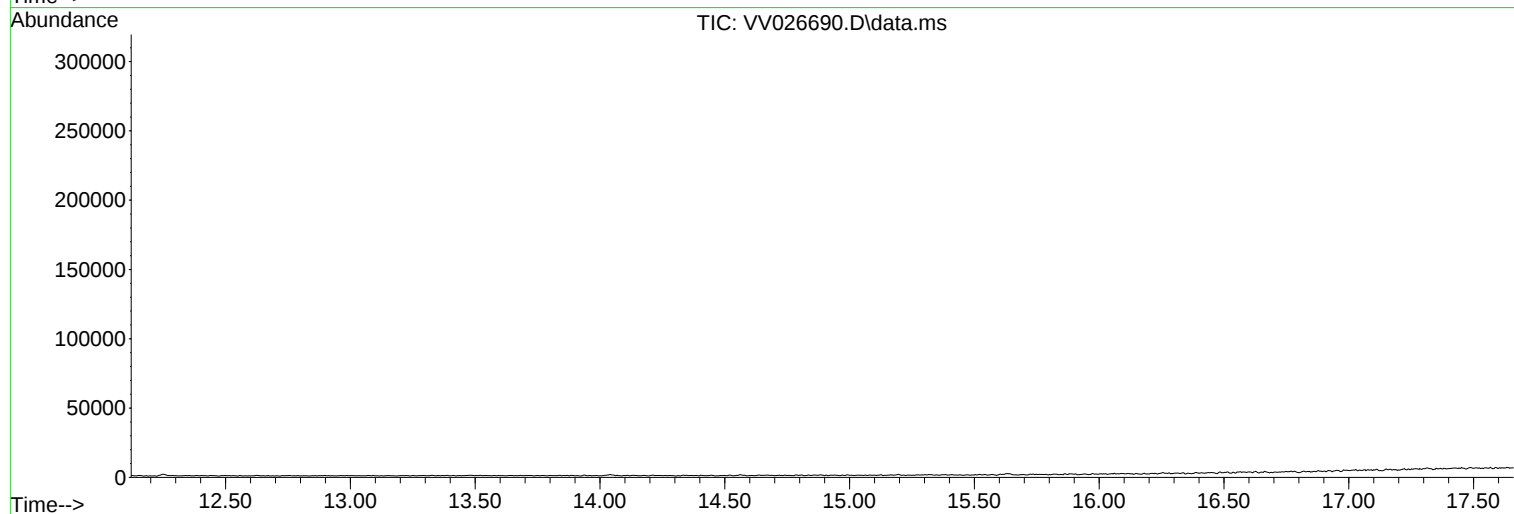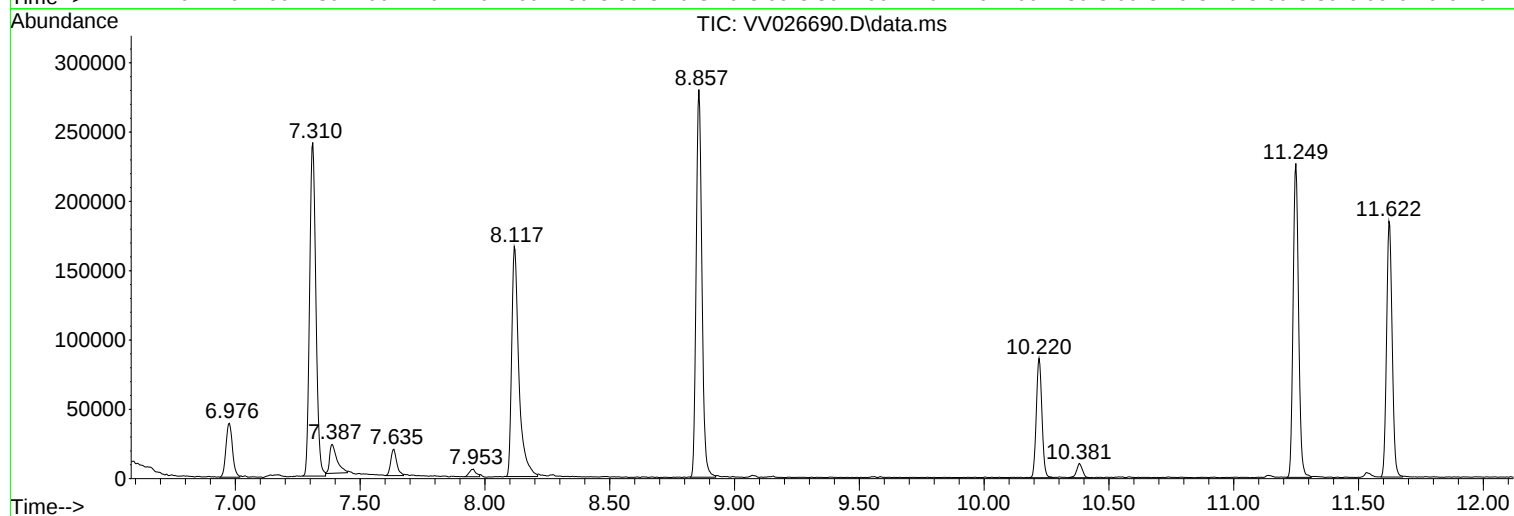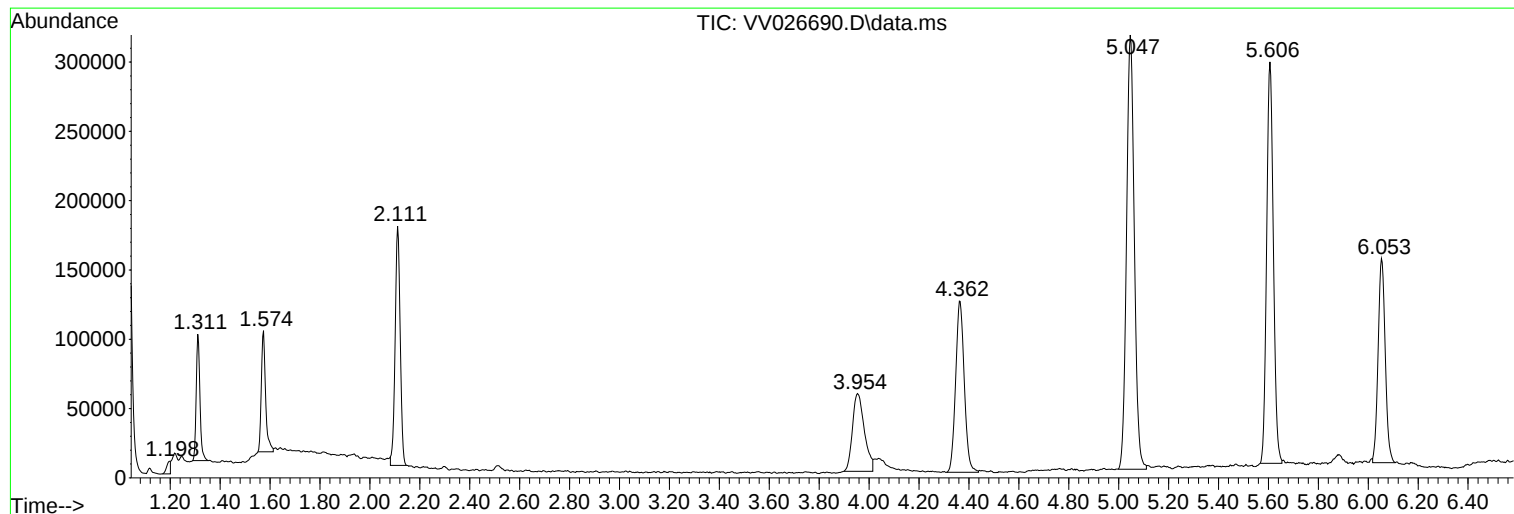

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070822\
Data File : VV026690.D
Acq On : 08 Jul 2022 12:15
Operator : SY/MD
Sample : N3601-13
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUC0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070822\
Data File : VV026690.D
Acq On : 08 Jul 2022 12:15
Operator : SY/MD
Sample : N3601-13
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUC0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc