

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070822\
 Data File : VV026697.D
 Acq On : 08 Jul 2022 15:11
 Operator : SY/MD
 Sample : N3601-15 50X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUA6

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV026697.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.233	44	60	65	rBV3	12159	30181	4.65%	0.645%
2	1.326	83	89	101	rVB	81144	83967	12.94%	1.795%
3	1.587	163	170	184	rBV	83425	108067	16.66%	2.310%
4	2.121	327	336	356	rVB	160079	238390	36.75%	5.095%
5	2.523	452	461	473	rVB	25713	40801	6.29%	0.872%
6	2.773	532	539	551	rVB7	5273	10015	1.54%	0.214%
7	3.982	891	915	962	rBV4	58419	302701	46.66%	6.470%
8	4.378	1022	1038	1062	rVB	124769	299499	46.17%	6.402%
9	5.050	1231	1247	1273	rBV3	306726	648682	100.00%	13.865%
10	5.619	1408	1424	1445	rBV	234588	468797	72.27%	10.020%
11	5.911	1503	1515	1521	rBV9	5110	10304	1.59%	0.220%
12	6.085	1555	1569	1596	rVB	131496	270167	41.65%	5.775%
13	6.426	1669	1675	1702	rBV2	15193	46579	7.18%	0.996%
14	7.024	1851	1861	1878	rBV2	37502	69018	10.64%	1.475%
15	7.346	1949	1961	1979	rBV	210837	363666	56.06%	7.773%
16	7.654	2048	2057	2075	rBV	18987	34702	5.35%	0.742%
17	8.124	2190	2203	2231	rBV2	182860	371718	57.30%	7.945%
18	8.866	2423	2434	2461	rBV	292956	468820	72.27%	10.021%
19	10.223	2843	2856	2873	rBV	94329	146463	22.58%	3.131%
20	11.252	3162	3176	3202	rBV	237564	365102	56.28%	7.804%
21	11.625	3281	3292	3312	rBV	192363	300817	46.37%	6.430%




Sum of corrected areas: 4678456

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070822\
Data File : VV026697.D
Acq On : 08 Jul 2022 15:11
Operator : SY/MD
Sample : N3601-15 50X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUA6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

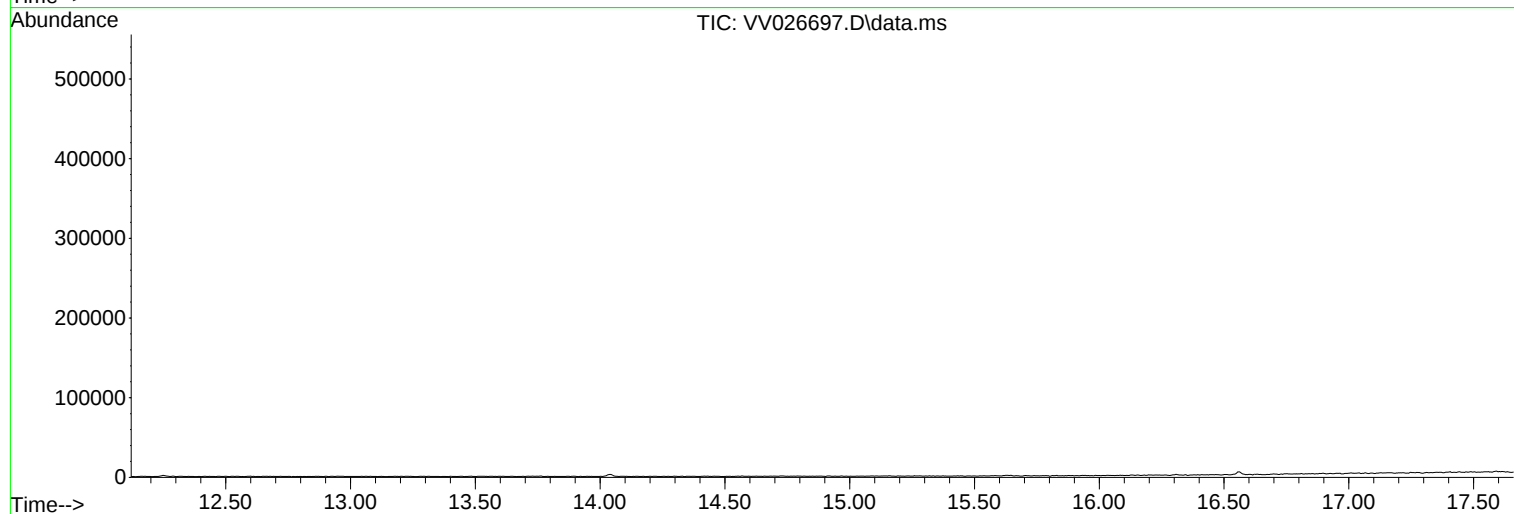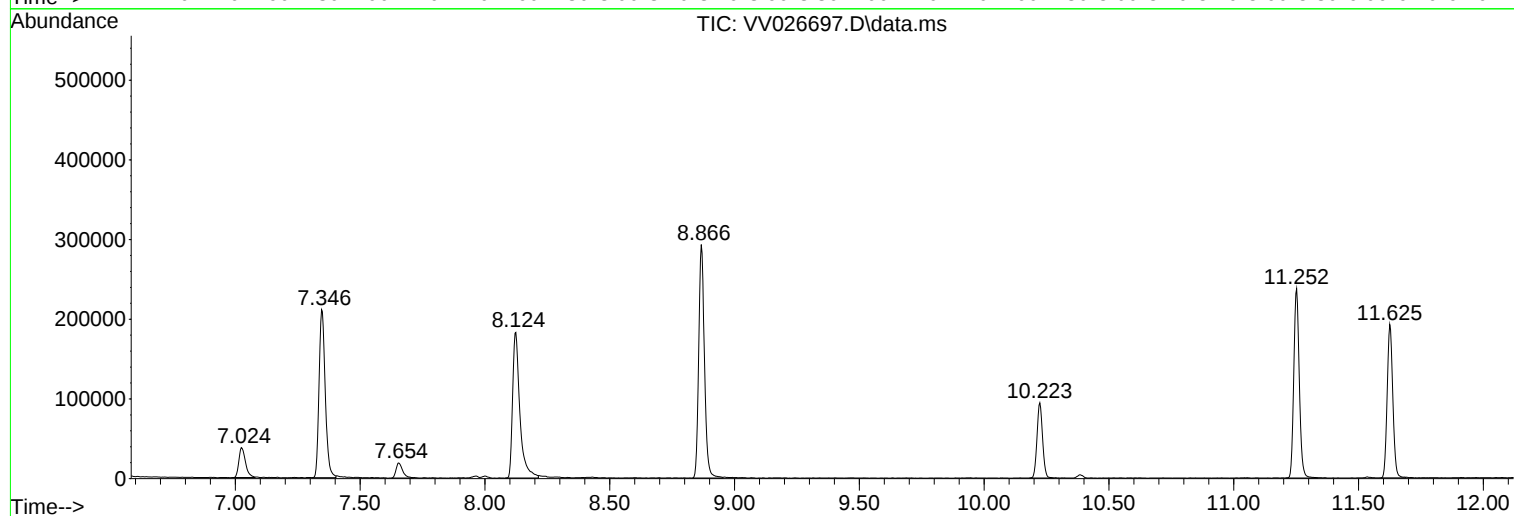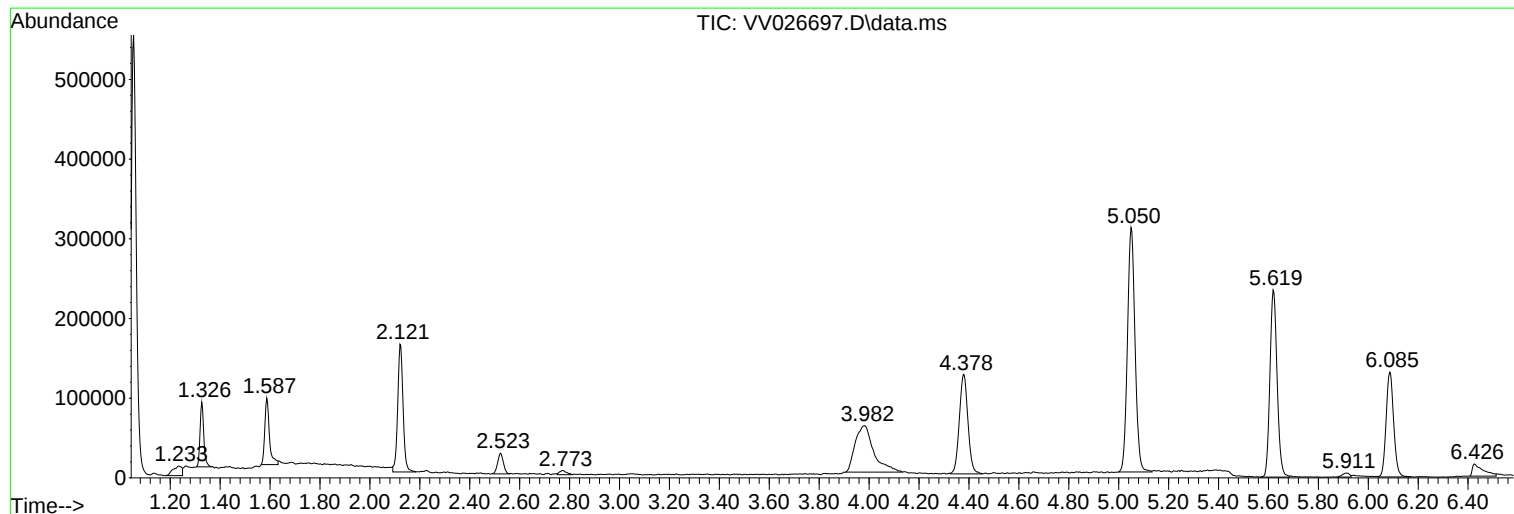

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070822\
Data File : VV026697.D
Acq On : 08 Jul 2022 15:11
Operator : SY/MD
Sample : N3601-15 50X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUA6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070822\
Data File : VV026697.D
Acq On : 08 Jul 2022 15:11
Operator : SY/MD
Sample : N3601-15 50X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUA6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc