

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070822\
 Data File : VV026698.D
 Acq On : 08 Jul 2022 15:33
 Operator : SY/MD
 Sample : N3638-02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUC2

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV026698.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.230	54	59	63	rVV2	6435	6050	1.21%	0.153%
2	1.256	63	67	75	rVV	4036	5118	1.02%	0.129%
3	1.323	79	88	102	rBV	78297	94399	18.90%	2.387%
4	1.584	163	169	183	rVB	79037	92256	18.47%	2.333%
5	2.121	327	336	351	rVB	149651	223677	44.79%	5.656%
6	3.944	891	903	910	rBV	22576	60364	12.09%	1.526%
7	4.368	1018	1035	1063	rVB	101818	252917	50.64%	6.396%
8	5.063	1234	1251	1283	rBV2	199773	499441	100.00%	12.630%
9	5.629	1414	1427	1453	rBV	182534	371629	74.41%	9.398%
10	5.921	1509	1518	1532	rVB10	2928	6195	1.24%	0.157%
11	6.079	1554	1567	1592	rBV	117636	248639	49.78%	6.288%
12	6.995	1840	1852	1880	rBV	30968	63924	12.80%	1.617%
13	7.320	1942	1953	1976	rBV	193397	344505	68.98%	8.712%
14	7.632	2041	2050	2073	rBV2	16169	31586	6.32%	0.799%
15	8.098	2184	2195	2232	rBV2	147675	366042	73.29%	9.256%
16	8.854	2417	2430	2452	rBV	281398	457037	91.51%	11.558%
17	10.217	2843	2854	2868	rBV	92834	147478	29.53%	3.729%
18	10.381	2898	2905	2916	rVB	5367	8743	1.75%	0.221%
19	11.249	3164	3175	3195	rBV	228674	357421	71.56%	9.038%
20	11.532	3255	3263	3278	rBV3	7319	13285	2.66%	0.336%
21	11.625	3280	3292	3308	rBV	193467	303755	60.82%	7.681%




Sum of corrected areas: 3954461

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070822\
Data File : VV026698.D
Acq On : 08 Jul 2022 15:33
Operator : SY/MD
Sample : N3638-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUC2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

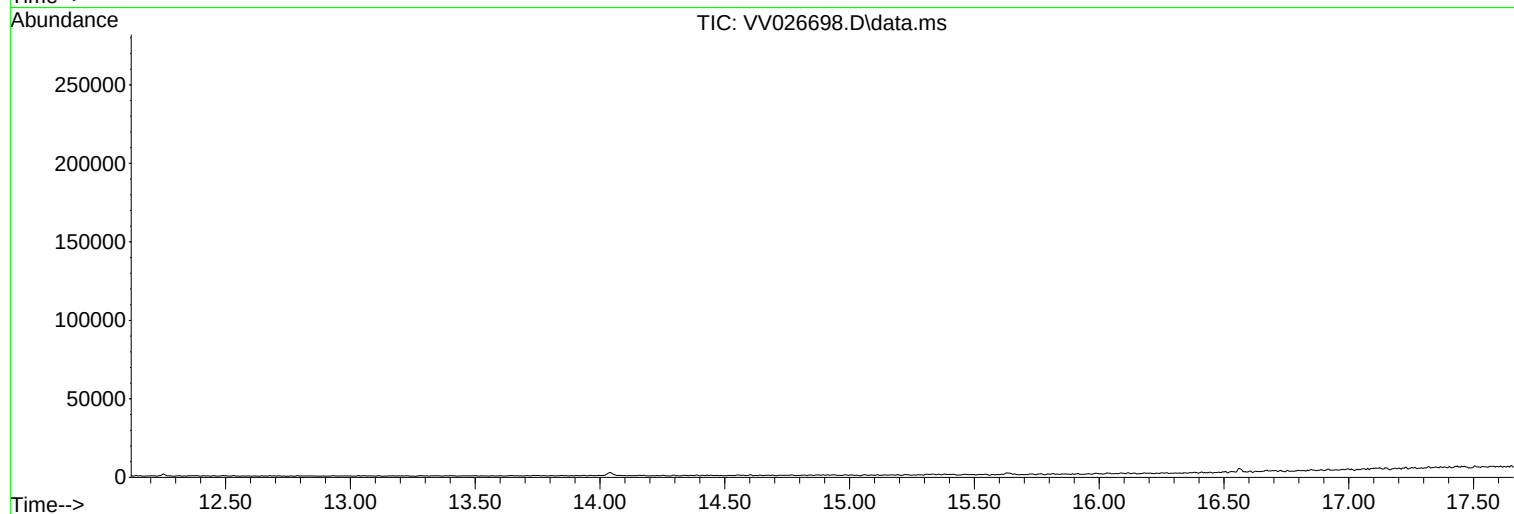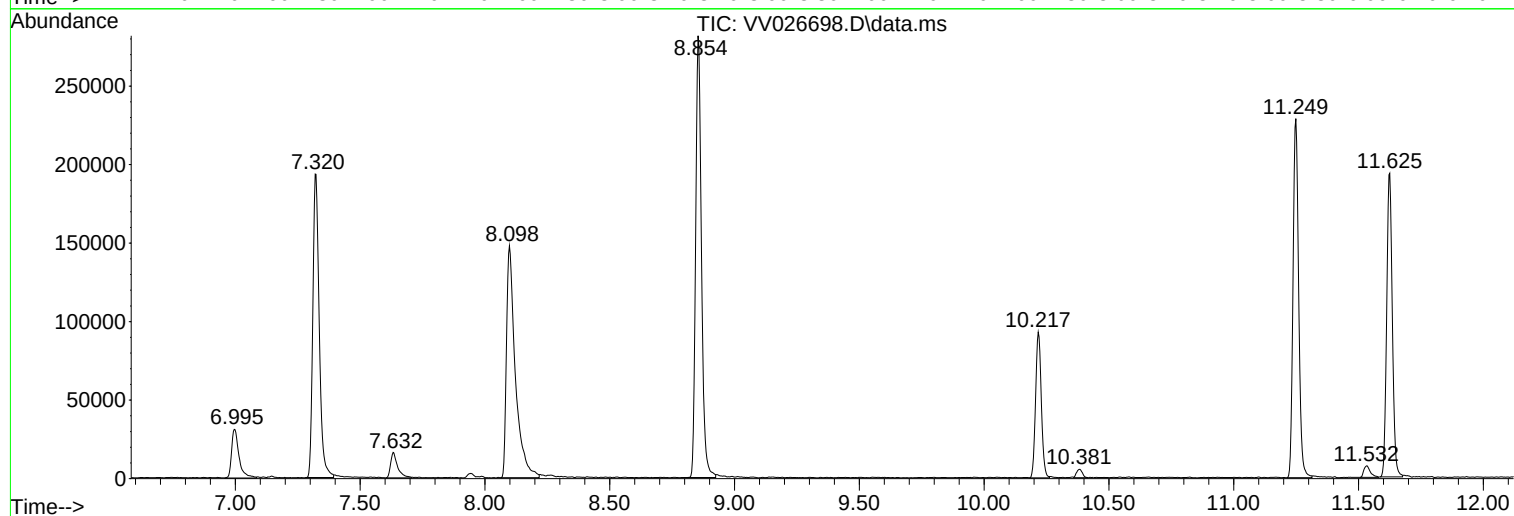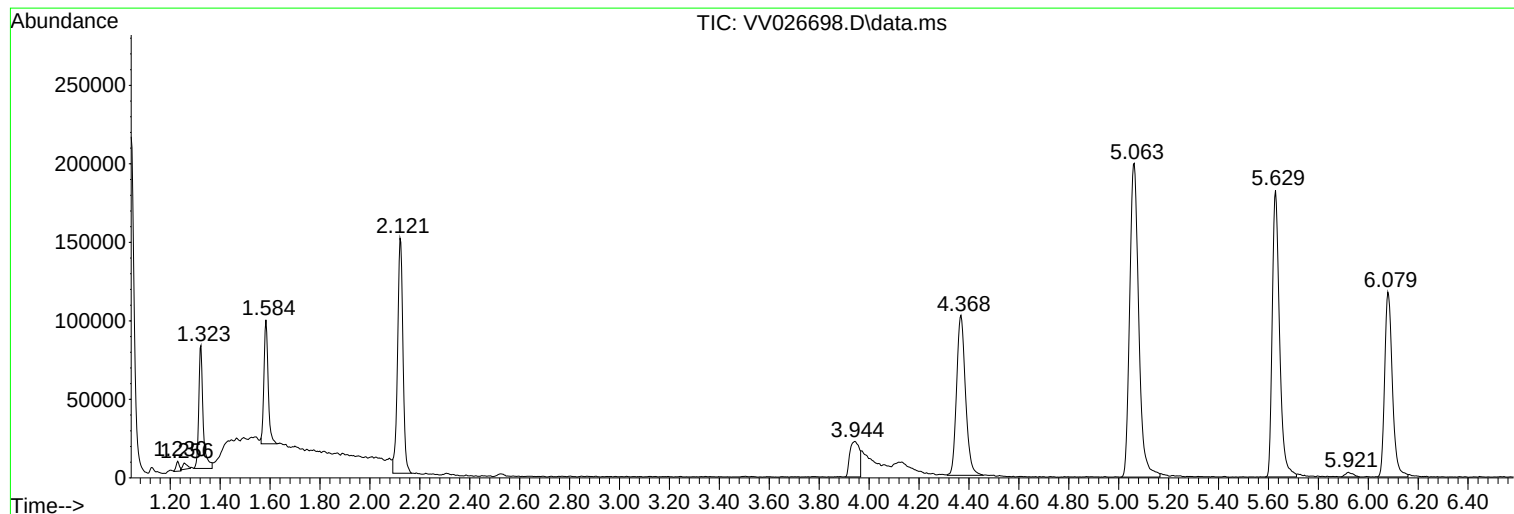

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070822\
Data File : VV026698.D
Acq On : 08 Jul 2022 15:33
Operator : SY/MD
Sample : N3638-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUC2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070822\
Data File : VV026698.D
Acq On : 08 Jul 2022 15:33
Operator : SY/MD
Sample : N3638-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUC2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc