

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070822\
 Data File : VV026700.D
 Acq On : 08 Jul 2022 16:23
 Operator : SY/MD
 Sample : N3601-17 50X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUA9

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV026700.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.224	44	57	61	rBV4	12227	25248	3.28%	0.434%
2	1.314	78	85	103	rVB	76011	84960	11.02%	1.461%
3	1.577	160	167	192	rVB	79490	100994	13.10%	1.737%
4	2.114	325	334	346	rVB	150707	216888	28.13%	3.731%
5	2.516	451	459	470	rVB	23173	36829	4.78%	0.633%
6	2.770	526	538	554	rBV	228792	386440	50.13%	6.647%
7	3.921	879	896	927	rBV3	242970	770899	100.00%	13.260%
8	4.355	1016	1031	1054	rVB	116115	275414	35.73%	4.737%
9	5.040	1229	1244	1267	rBV2	283263	610225	79.16%	10.496%
10	5.606	1407	1420	1442	rVB	277276	547896	71.07%	9.424%
11	5.899	1497	1511	1532	rBV	254185	492166	63.84%	8.466%
12	6.069	1550	1564	1587	rVB	126335	254728	33.04%	4.382%
13	6.645	1738	1743	1759	rBV	17385	37681	4.89%	0.648%
14	6.995	1840	1852	1867	rBV	31104	60197	7.81%	1.035%
15	7.333	1943	1957	1979	rBV	191464	335765	43.55%	5.775%
16	7.645	2042	2054	2071	rBV	16433	30309	3.93%	0.521%
17	8.117	2189	2201	2230	rBV2	169861	341985	44.36%	5.882%
18	8.860	2420	2432	2458	rBV	263578	443075	57.48%	7.621%
19	10.220	2843	2855	2871	rBV	90192	140782	18.26%	2.422%
20	11.249	3164	3175	3194	rBV	221235	343949	44.62%	5.916%
21	11.625	3281	3292	3310	rBV	173310	277265	35.97%	4.769%




Sum of corrected areas: 5813695

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070822\
Data File : VV026700.D
Acq On : 08 Jul 2022 16:23
Operator : SY/MD
Sample : N3601-17 50X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUA9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

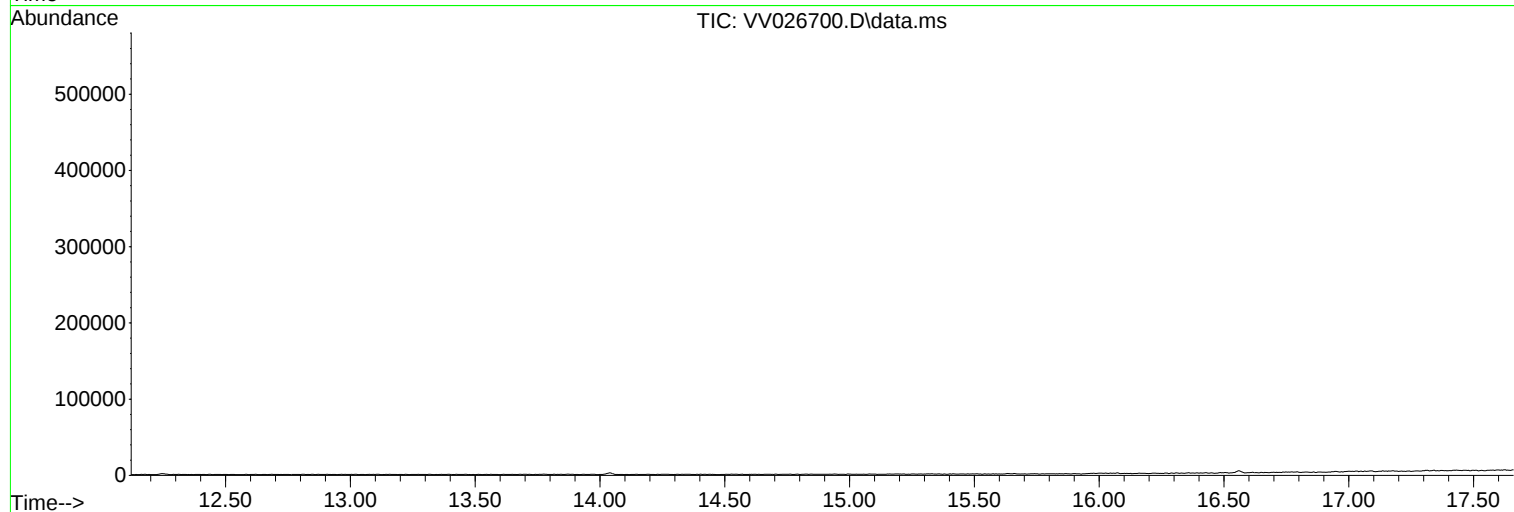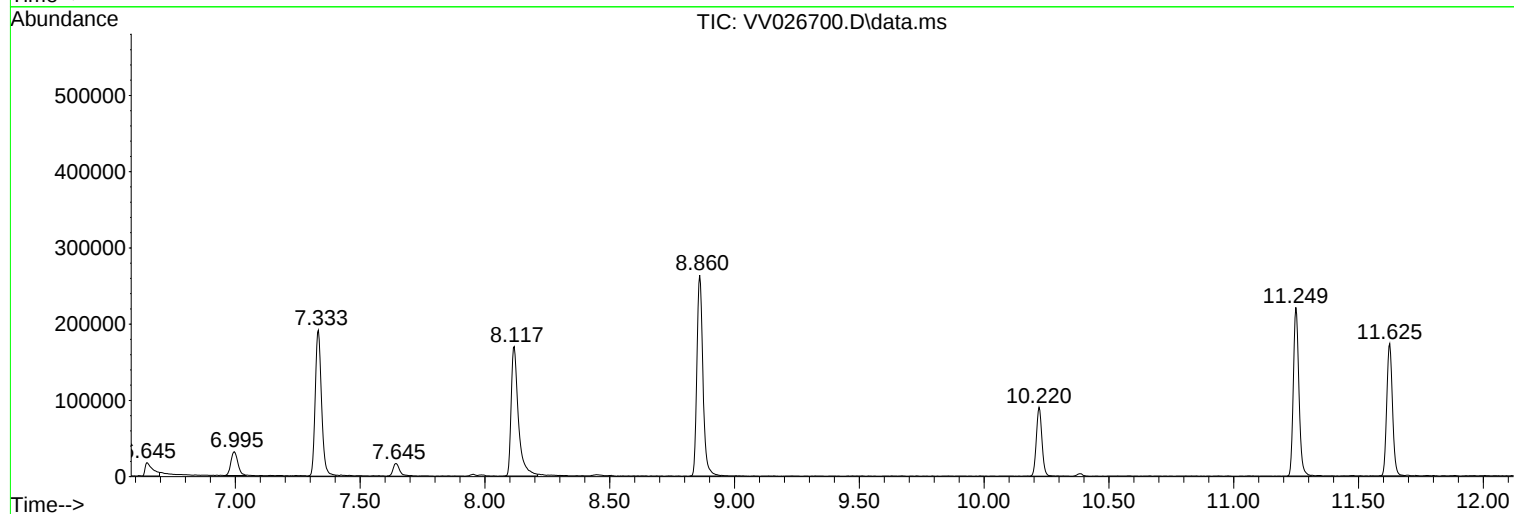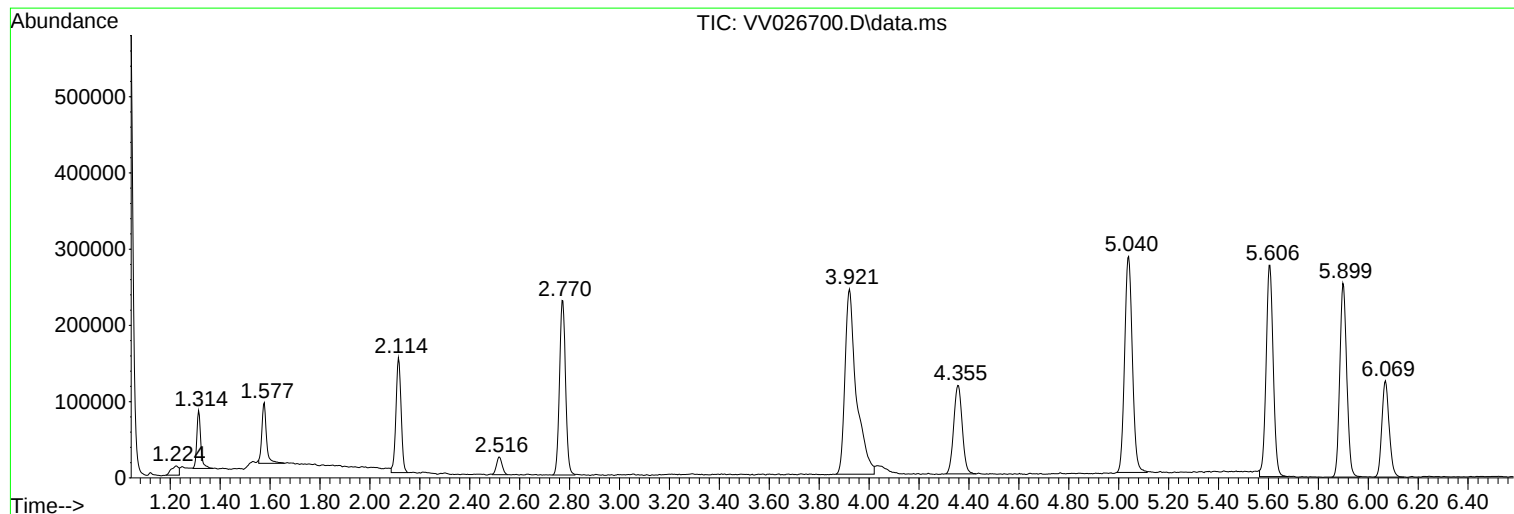

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070822\
Data File : VV026700.D
Acq On : 08 Jul 2022 16:23
Operator : SY/MD
Sample : N3601-17 50X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUA9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070822\
Data File : VV026700.D
Acq On : 08 Jul 2022 16:23
Operator : SY/MD
Sample : N3601-17 50X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUA9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc